
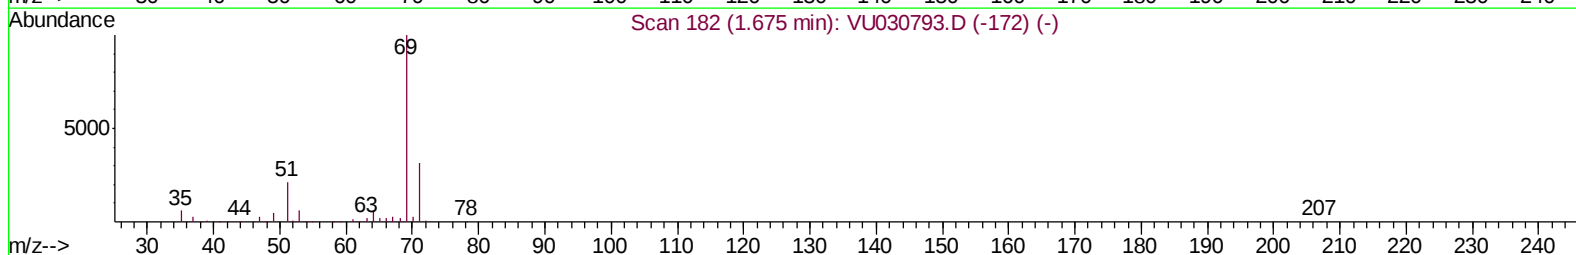
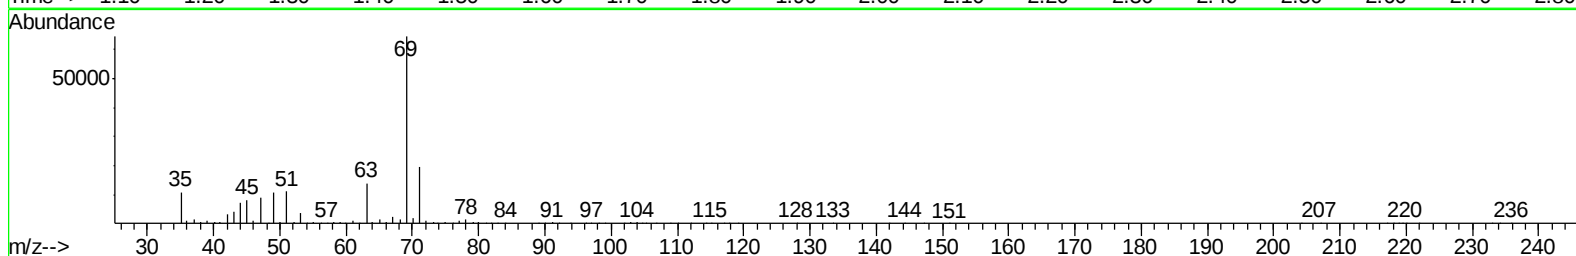


Data File : VU030801.D
Acq On : 06 Apr 2019 15:31
Operator : JC/SP
Sample : K2276-17ME
Misc : 5.64g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Apr 08 05:05:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 05:01:06 2019
Response via : Initial Calibration

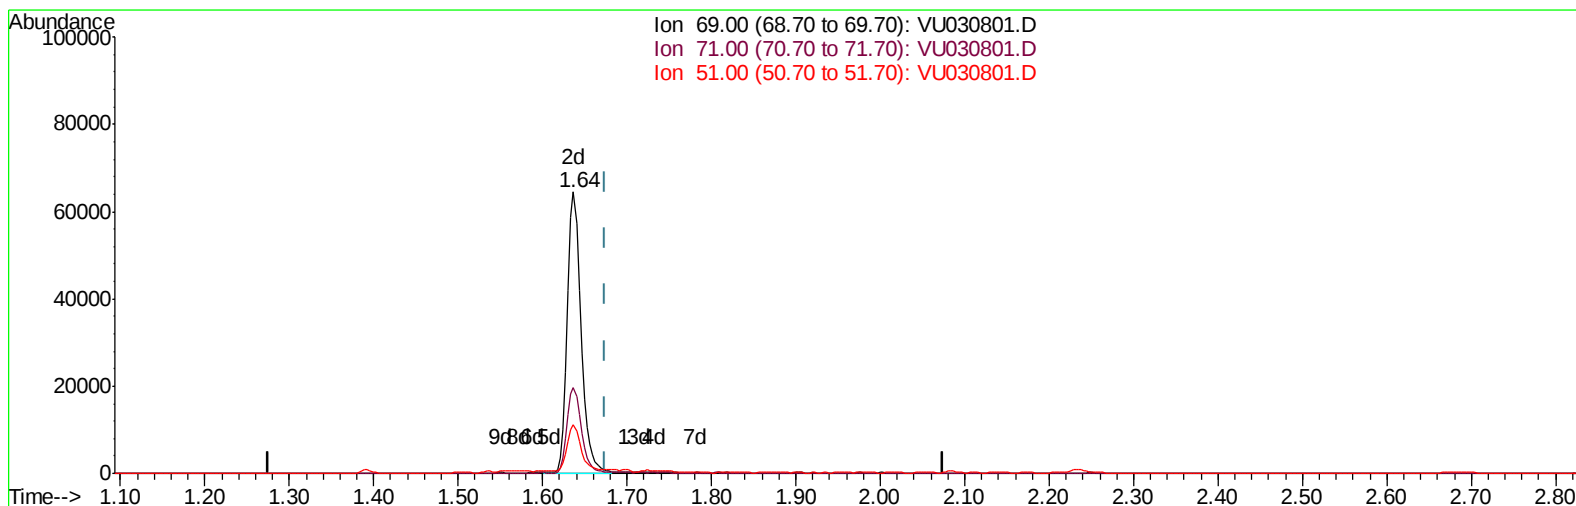

TIC: VU030801.D

(7) Chloroethane-d5 (S)

1.637min (-0.039) 21.84ug/L m

response 72911

Ion	Exp%	Act%
69.00	100	100
71.00	31.60	0.36#
51.00	27.70	0.46#
0.00	0.00	0.00