
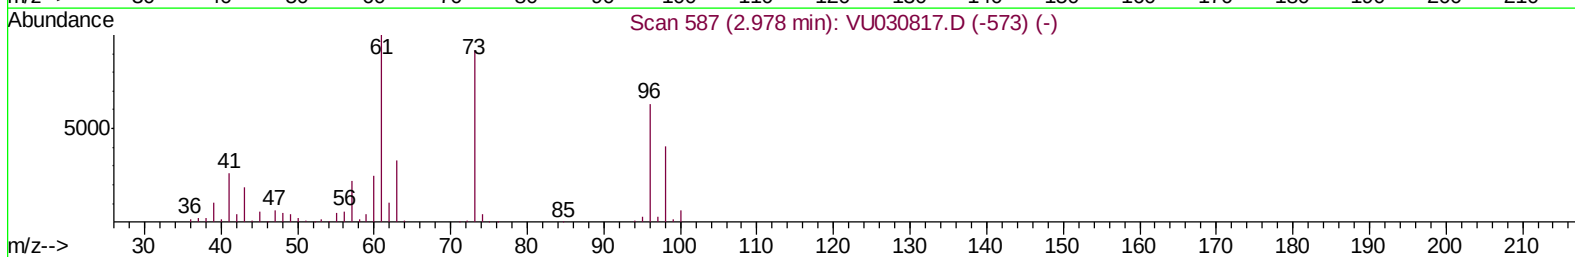
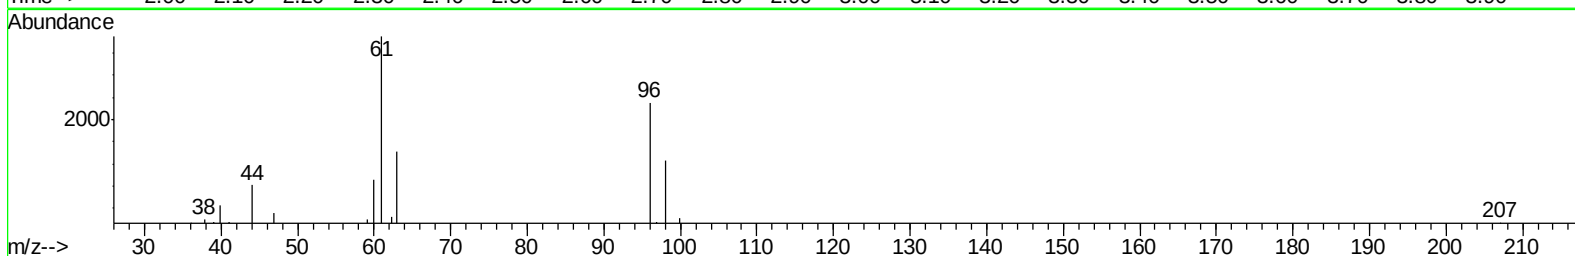


Data File : VU030829.D
Acq On : 07 Apr 2019 02:38
Operator : JC/SP
Sample : K2260-04DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Quant Time: Apr 08 07:09:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 07:03:53 2019
Response via : Initial Calibration

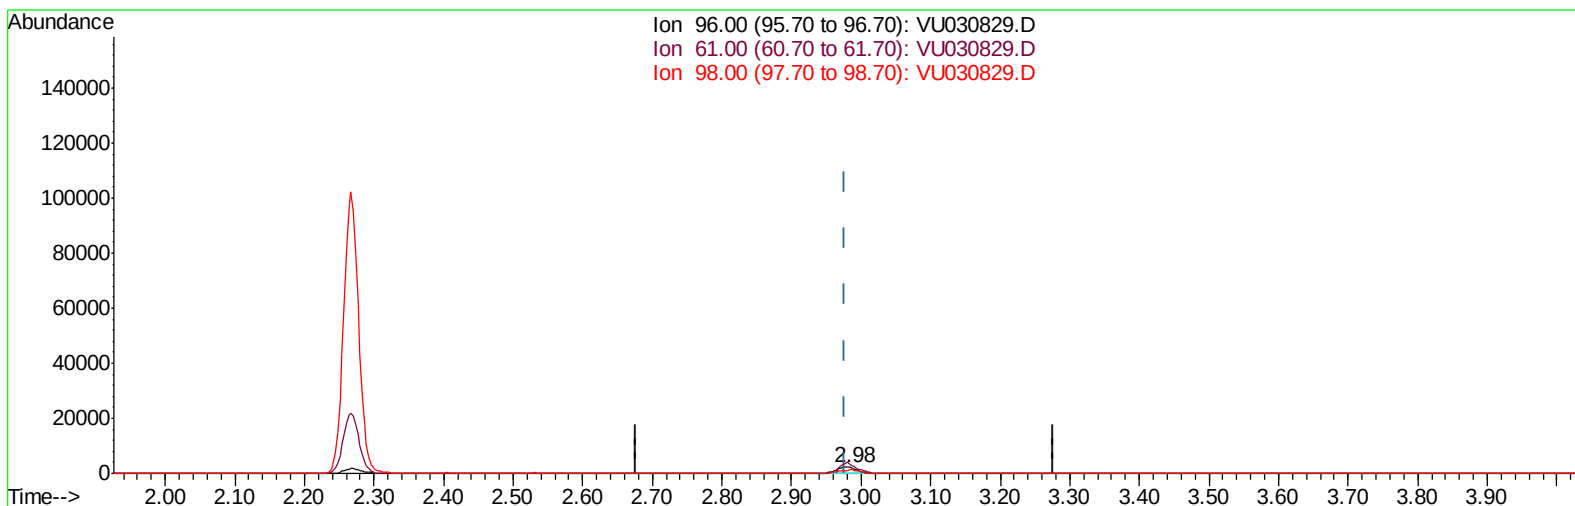

TIC: VU030829.D

(17) trans-1,2-Dichloroethene (T)

2.984min (+0.006) 1.33ug/L m

response 4530

Ion	Exp%	Act%
96.00	100	100
61.00	156.40	152.02
98.00	62.80	55.15
0.00	0.00	0.00