
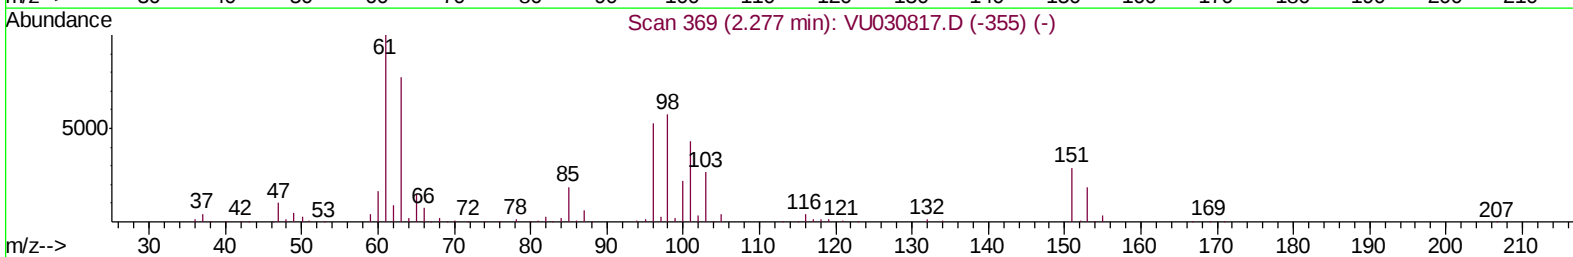
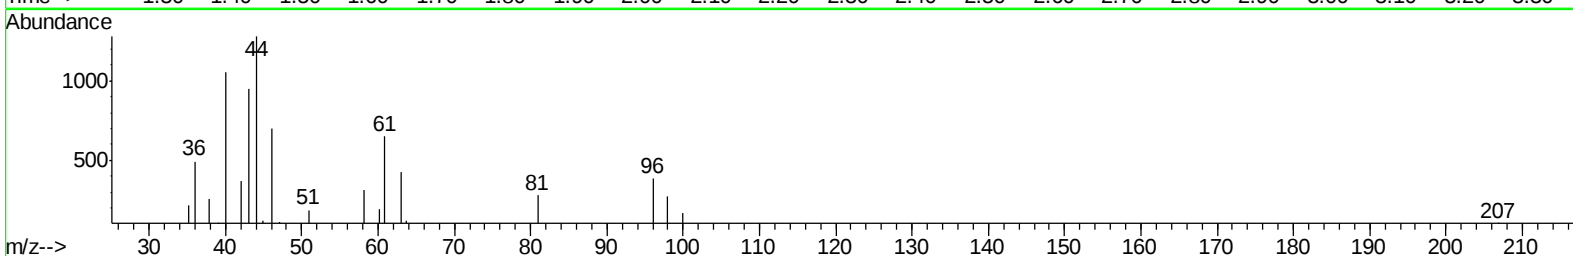


Data File : VU030840.D
Acq On : 07 Apr 2019 06:51
Operator : JC/SP
Sample : K2249-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Apr 08 09:22:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 07:03:53 2019
Response via : Initial Calibration

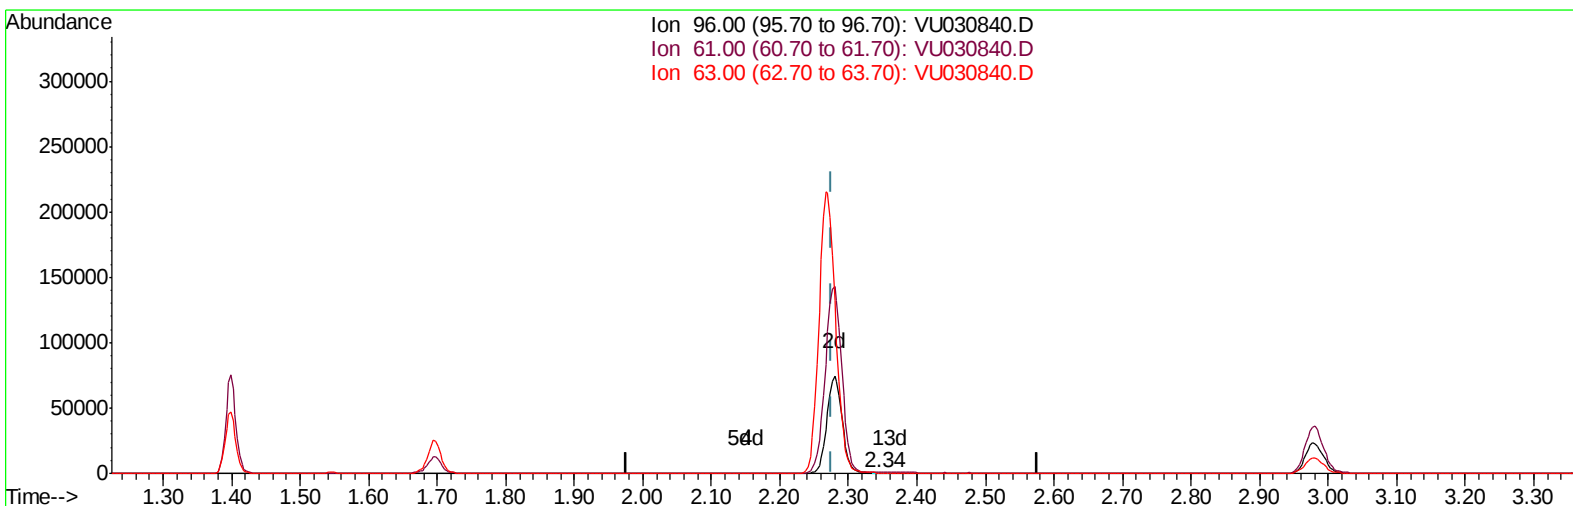

TIC: VU030840.D

(12) 1,1-Dichloroethene (T)

2.344min (+0.067) 0.06ug/L

response 203

Ion	Exp%	Act%
96.00	100	100
61.00	188.60	168.83
63.00	129.90	142.86
0.00	0.00	0.00