

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040719\
Quantitation Report (QT Reviewed)


Data File : VU030827.D
Acq On : 07 Apr 2019 01:53
Operator : JC/SP
Sample : K2269-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BR6

Manual Integrations
APPROVED

MMDadoda
4/10/2019 9:29:16 AM

Quant Time: Apr 08 08:24:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 07:03:53 2019
Response via : Initial Calibration

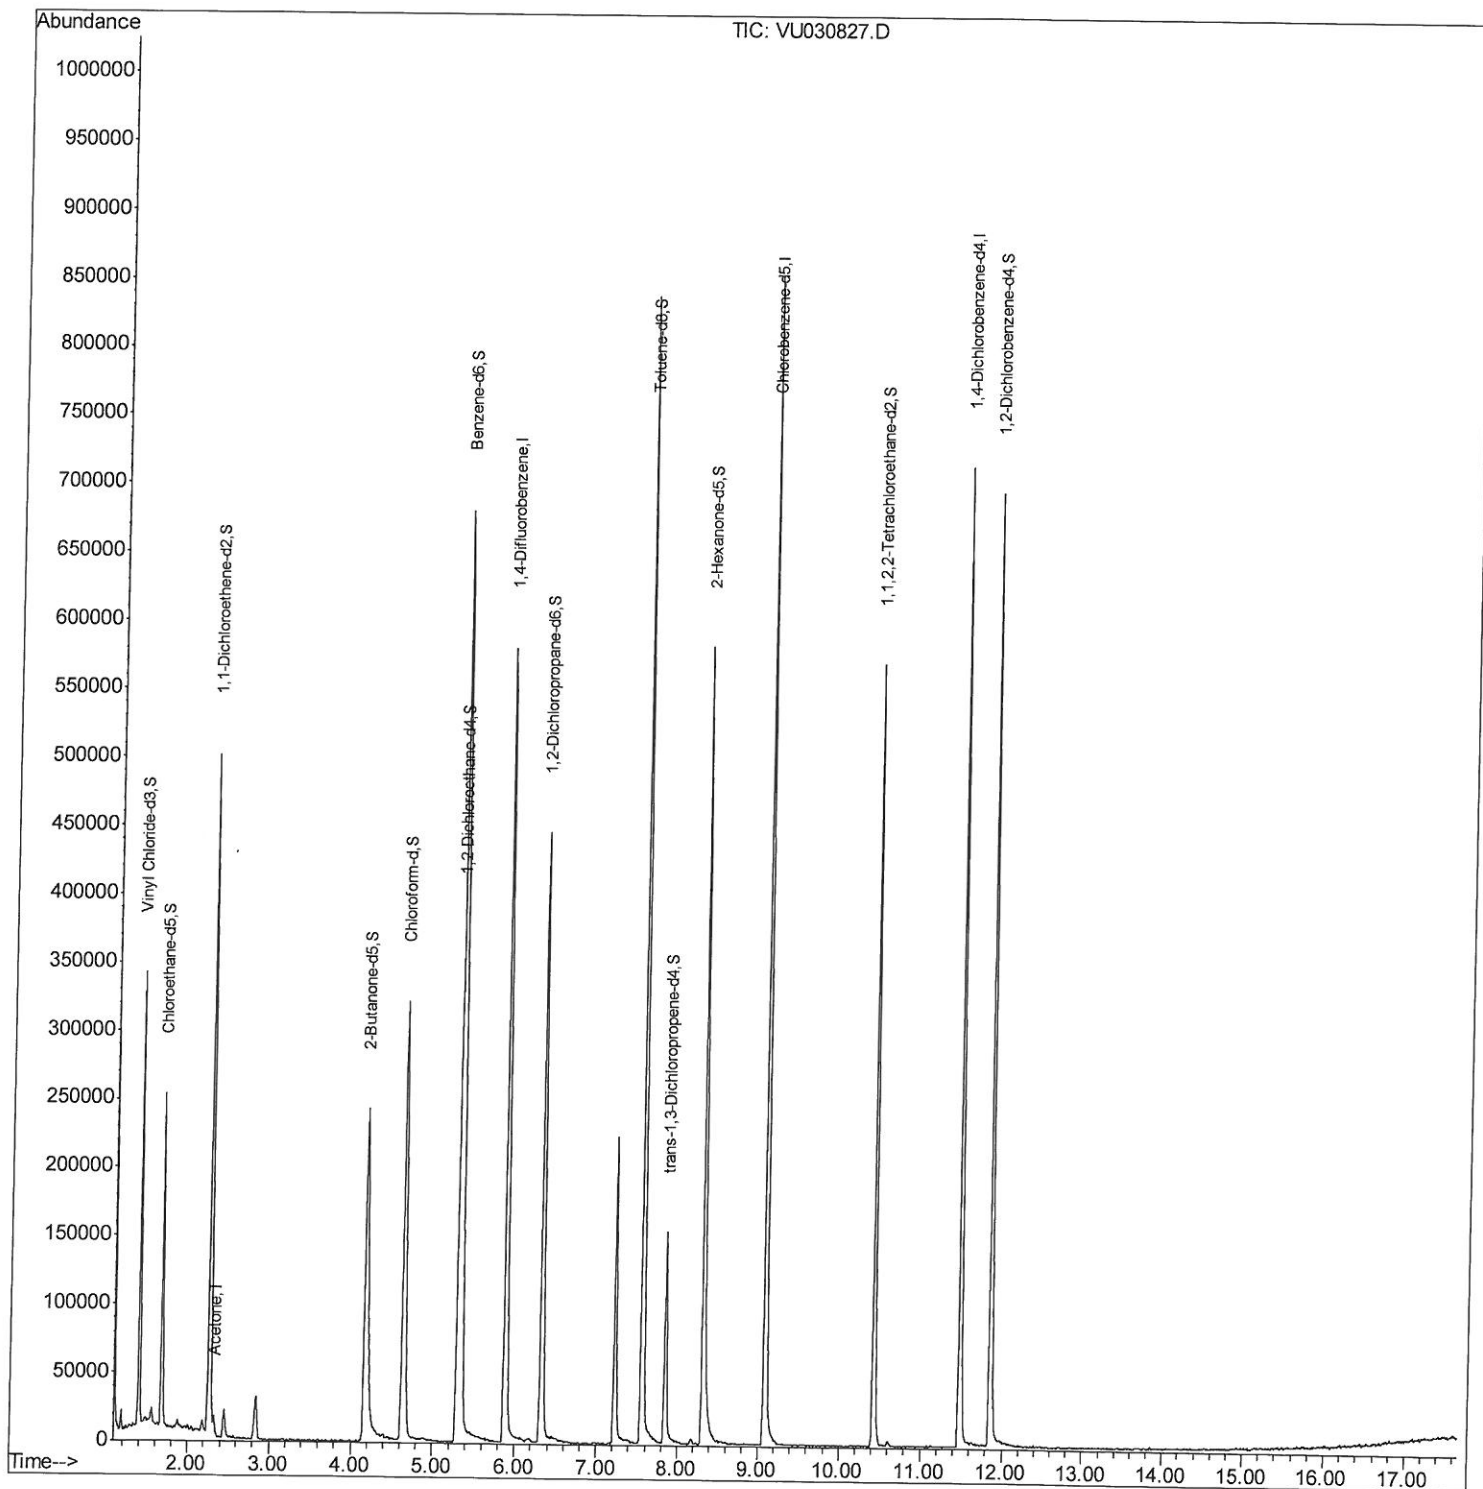

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040719\
Quantitation Report (Qedit)




Data File : VU030827.D
Acq On : 07 Apr 2019 01:53
Operator : JC/SP
Sample : K2269-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BR6

Manual Integrations
APPROVED

MMDadoda
4/10/2019 9:29:16 AM

Quant Time: Apr 08 07:08:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 07:03:53 2019
Response via : Initial Calibration

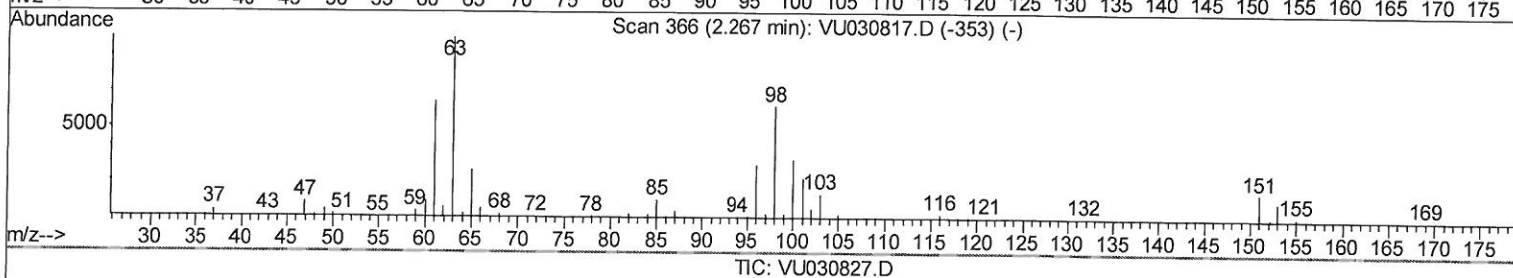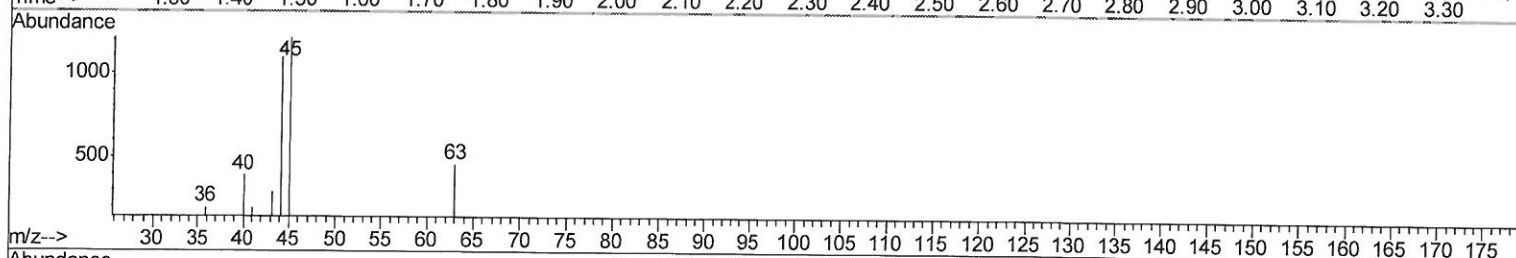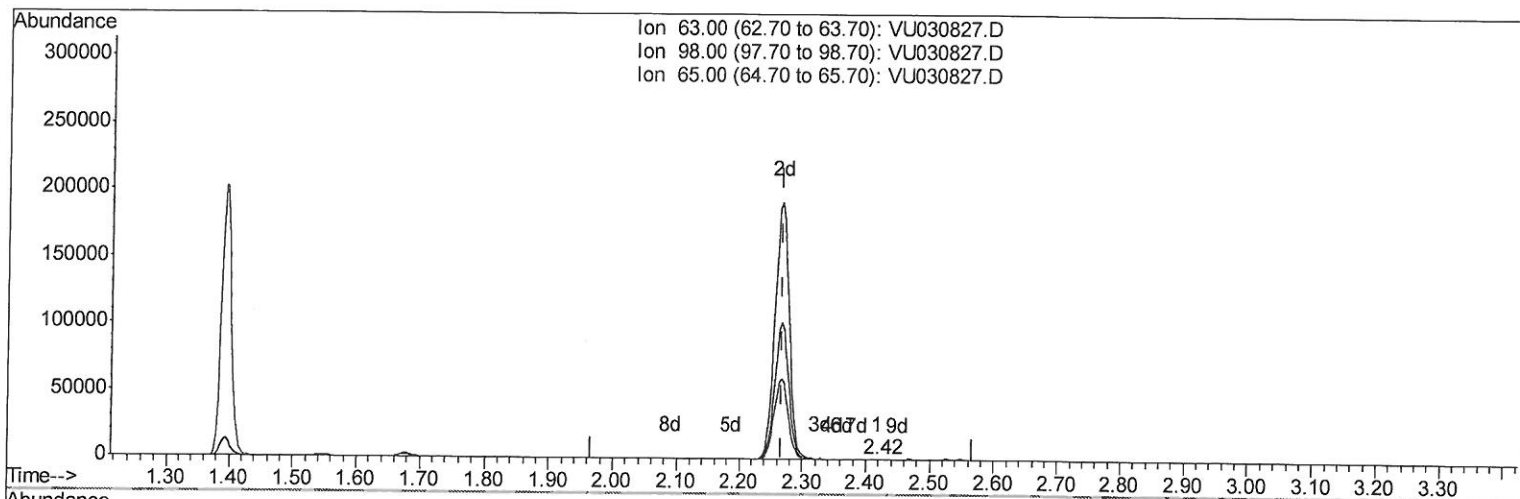

(11) 1,1-Dichloroethene-d2 (S)

2.418min (+0.151) 0.03ug/L

response 198

Ion	Exp%	Act%
63.00	100	100
98.00	67.20	78.79
65.00	24.00	24.24
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040719\
Quantitation Report (Qedit)




Data File : VU030827.D
Acq On : 07 Apr 2019 01:53
Operator : JC/SP
Sample : K2269-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BR6

Manual Integrations
APPROVED

MMDadoda
4/10/2019 9:29:16 AM

Quant Time: Apr 08 07:08:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 07:03:53 2019
Response via : Initial Calibration

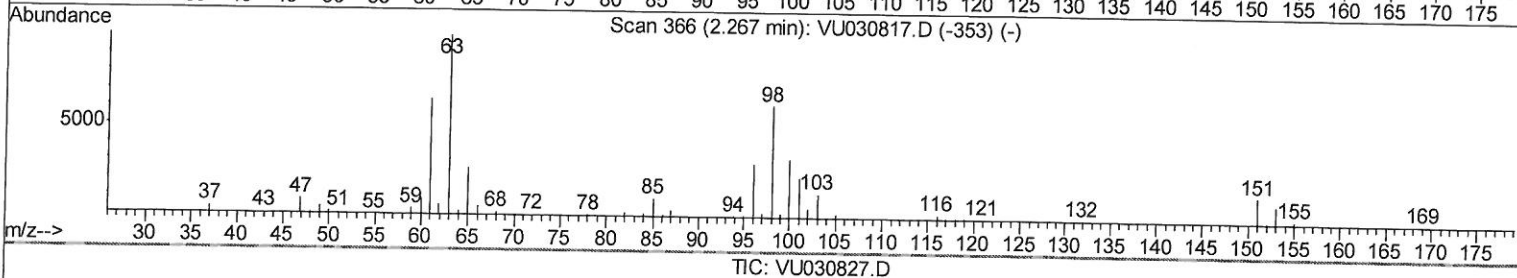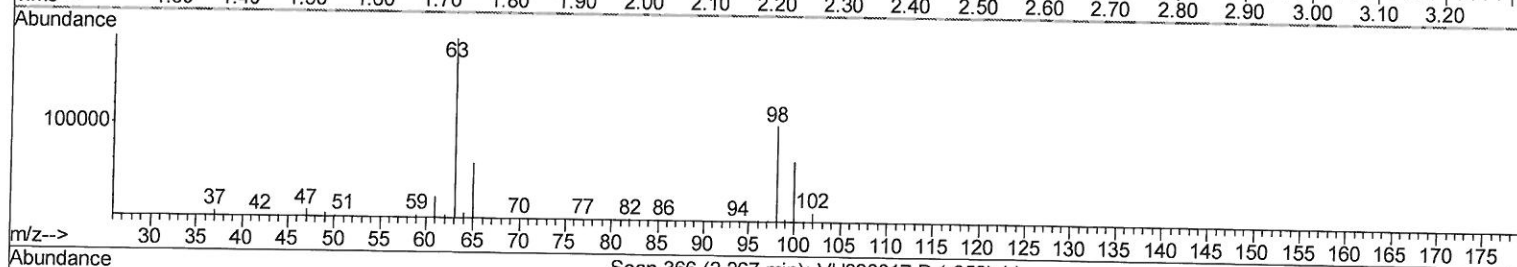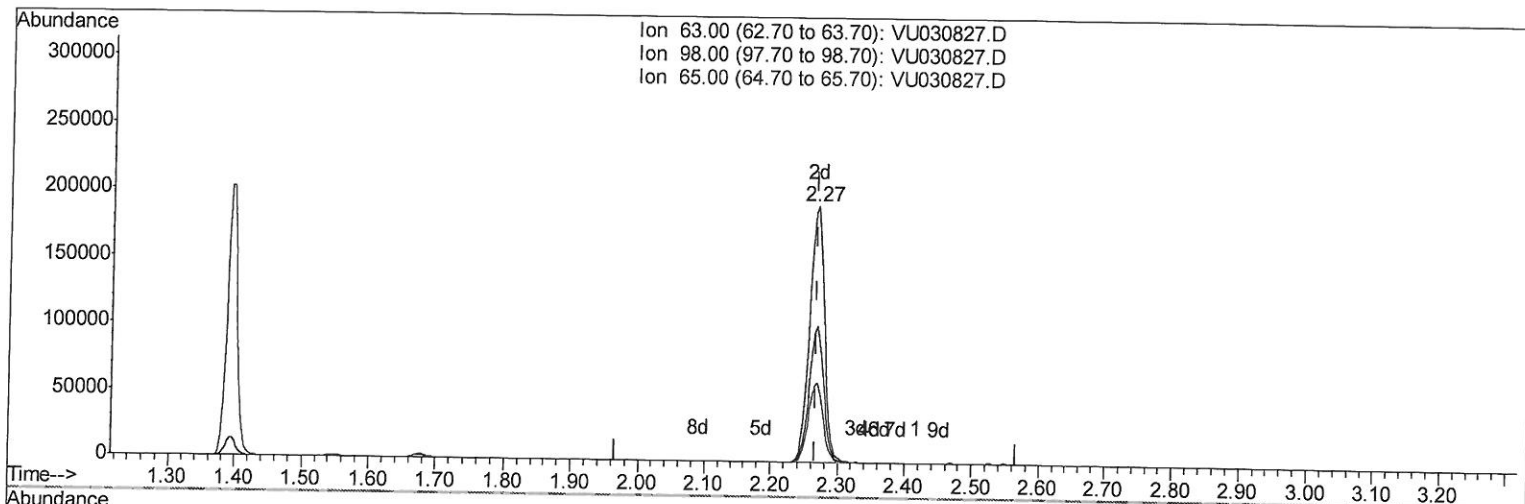

(11) 1,1-Dichloroethene-d2 (S)

2.267min (-0.000) 38.91ug/L m

response 294078

Ion	Exp%	Act%
63.00	100	100
98.00	67.20	0.05#
65.00	24.00	0.02#
0.00	0.00	0.00

7 mg
4/10/19

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040719\
Quantitation Report (QT Reviewed)

Data File : VU030827.D
Acq On : 07 Apr 2019 01:53
Operator : JC/SP
Sample : K2269-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BR6

Manual Integrations
APPROVED

MMDadoda
4/10/2019 9:29:16 AM

Quant Time: Apr 08 08:24:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 07:03:53 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	468084	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	458380	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	186683	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	209941	50.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.48%
7) Chloroethane-d5	1.68	69	168356	53.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.18%
11) 1,1-Dichloroethene-d2	2.27	63	294078m	38.91	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.82%
21) 2-Butanone-d5	4.17	46	330350	99.75	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.75%
24) Chloroform-d	4.64	84	317706	49.77	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.54%
26) 1,2-Dichloroethane-d4	5.30	65	225469	51.77	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.54%
32) Benzene-d6	5.34	84	652395	48.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.50%
36) 1,2-Dichloropropane-d6	6.33	67	223985	48.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.68%
41) Toluene-d8	7.56	98	553408	46.66	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.32%
43) trans-1,3-Dichloropropene-	7.85	79	94258	45.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.16%
47) 2-Hexanone-d5	8.31	63	194216	92.66	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.66%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	298588	48.27	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.54%
64) 1,2-Dichlorobenzene-d4	11.86	152	186460	50.79	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.58%

Target Compounds

13) Acetone	2.31	43	12960	3.824	ug/L	Qvalue 98
-------------	------	----	-------	-------	------	-----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7mL
4/10/19