

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040719\
 Data File : VU030811.D
 Acq On : 06 Apr 2019 19:22
 Operator : JC/SP
 Sample : K2299-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6X6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	38	rVB3	16201	16527	0.79%	0.105%
2	1.392	88	94	106	rBV	335520	364035	17.48%	2.310%
3	1.675	174	182	199	rVB	251027	321765	15.45%	2.042%
4	2.267	355	366	378	rVB	493455	751098	36.06%	4.766%
5	2.444	411	421	437	rBV2	15083	32007	1.54%	0.203%
6	2.611	469	473	474	rBV3	1090	747	0.04%	0.005%
7	2.691	491	498	499	rBV6	1873	1679	0.08%	0.011%
8	2.830	534	541	554	rVB6	3023	5988	0.29%	0.038%
9	2.987	583	590	600	rBV7	2297	3183	0.15%	0.020%
10	3.248	666	671	676	rVB4	941	908	0.04%	0.006%
11	3.305	686	689	694	rVB4	1256	1106	0.05%	0.007%
12	3.463	734	738	740	rVB2	819	570	0.03%	0.004%
13	3.479	740	743	748	rBV4	636	674	0.03%	0.004%
14	3.659	796	799	805	rBV3	584	562	0.03%	0.004%
15	3.981	896	899	904	rBV6	787	880	0.04%	0.006%
16	4.084	924	931	935	rBV7	1297	2015	0.10%	0.013%
17	4.174	947	959	993	rBV2	201782	665444	31.94%	4.223%
18	4.643	1085	1105	1132	rBV	317092	794322	38.13%	5.041%
19	4.756	1137	1140	1143	rBV2	1009	760	0.04%	0.005%
20	4.987	1203	1212	1216	rBV10	4730	7522	0.36%	0.048%
21	5.071	1236	1238	1242	rBV3	823	630	0.03%	0.004%
22	5.145	1258	1261	1264	rBV2	636	579	0.03%	0.004%
23	5.209	1279	1281	1287	rVB3	1249	1137	0.05%	0.007%
24	5.248	1287	1293	1297	rBV4	864	706	0.03%	0.004%
25	5.334	1297	1320	1348	rBV2	698507	2083100	100.00%	13.219%
26	5.614	1405	1407	1416	rVB6	1670	1635	0.08%	0.010%
27	5.688	1428	1430	1438	rVB6	1420	1062	0.05%	0.007%
28	5.720	1438	1440	1448	rVB4	1148	1177	0.06%	0.007%
29	5.817	1465	1470	1473	rBV4	881	872	0.04%	0.006%
30	5.881	1477	1490	1517	rBV	583466	1168907	56.11%	7.418%
31	6.186	1573	1585	1597	rBV5	19889	40099	1.92%	0.254%
32	6.328	1614	1629	1647	rBV	456137	934874	44.88%	5.932%
33	6.620	1717	1720	1722	rBV4	887	548	0.03%	0.003%
34	6.736	1752	1756	1759	rBV4	961	538	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040719\
 Data File : VU030811.D
 Acq On : 06 Apr 2019 19:22
 Operator : JC/SP
 Sample : K2299-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6X6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.813	1775	1780	1782	rBV3	776	671	0.03%	0.004%
36	6.887	1797	1803	1807	rVB4	795	791	0.04%	0.005%
37	6.926	1807	1815	1817	rBV5	836	991	0.05%	0.006%
38	7.051	1850	1854	1855	rBV3	1250	822	0.04%	0.005%
39	7.096	1865	1868	1873	rVB4	853	563	0.03%	0.004%
40	7.225	1895	1908	1926	rBV	235432	439835	21.11%	2.791%
41	7.476	1983	1986	1993	rVB6	539	677	0.03%	0.004%
42	7.514	1993	1998	1999	rBV4	1494	1255	0.06%	0.008%
43	7.563	1999	2013	2033	rBV	863572	1526309	73.27%	9.685%
44	7.849	2088	2102	2119	rBV	167382	300564	14.43%	1.907%
45	8.090	2173	2177	2181	rBV5	933	832	0.04%	0.005%
46	8.177	2188	2204	2213	rBV3	10317	20098	0.96%	0.128%
47	8.225	2213	2219	2227	rVB8	3638	5707	0.27%	0.036%
48	8.309	2233	2245	2286	rBV	621878	1152553	55.33%	7.314%
49	8.884	2420	2424	2426	rBV2	1310	1126	0.05%	0.007%
50	9.038	2460	2472	2475	rBV2	2993	5201	0.25%	0.033%
51	9.087	2475	2487	2508	rBV	861881	1448473	69.53%	9.192%
52	9.299	2550	2553	2558	rVB6	2296	1716	0.08%	0.011%
53	9.334	2562	2564	2567	rVV3	1009	648	0.03%	0.004%
54	9.379	2567	2578	2599	rVB2	14152	28849	1.38%	0.183%
55	9.456	2599	2602	2604	rBV4	879	559	0.03%	0.004%
56	9.553	2627	2632	2633	rBV4	1036	692	0.03%	0.004%
57	9.736	2687	2689	2693	rBV3	962	676	0.03%	0.004%
58	9.778	2698	2702	2706	rBV4	2481	2321	0.11%	0.015%
59	9.878	2729	2733	2737	rVB4	936	939	0.05%	0.006%
60	9.903	2737	2741	2742	rBV2	937	563	0.03%	0.004%
61	9.948	2745	2755	2759	rBV9	2361	3662	0.18%	0.023%
62	10.151	2814	2818	2819	rBV3	1055	689	0.03%	0.004%
63	10.312	2863	2868	2872	rVB3	1309	1294	0.06%	0.008%
64	10.427	2889	2904	2921	rBV	587047	963768	46.27%	6.116%
65	10.604	2951	2959	2971	rVB4	10645	17674	0.85%	0.112%
66	10.688	2980	2985	2988	rBV6	2243	2412	0.12%	0.015%
67	10.746	2997	3003	3007	rBV6	1362	2019	0.10%	0.013%
68	10.874	3039	3043	3047	rBV3	877	844	0.04%	0.005%
69	10.958	3066	3069	3070	rVV2	1686	886	0.04%	0.006%
70	10.971	3070	3073	3081	rVB5	3416	3672	0.18%	0.023%
71	11.061	3096	3101	3105	rBV3	1575	1575	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040719\
 Data File : VU030811.D
 Acq On : 06 Apr 2019 19:22
 Operator : JC/SP
 Sample : K2299-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6X6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	11.151	3124	3129	3137	rVB6	2088	2261	0.11%	0.014%
73	11.292	3169	3173	3176	rVV4	1817	1806	0.09%	0.011%
74	11.321	3179	3182	3191	rVB4	3481	3759	0.18%	0.024%
75	11.479	3220	3231	3253	rBV	740126	1235612	59.32%	7.841%
76	11.765	3311	3320	3334	rBV6	20135	38969	1.87%	0.247%
77	11.855	3336	3348	3372	rBV	740373	1241968	59.62%	7.881%
78	12.357	3496	3504	3508	rBV6	4113	6038	0.29%	0.038%
79	12.488	3537	3545	3551	rVB6	3929	6604	0.32%	0.042%
80	12.533	3557	3559	3568	rVB6	3322	3761	0.18%	0.024%
81	12.595	3575	3578	3581	rBV3	1054	664	0.03%	0.004%
82	12.617	3582	3585	3587	rBV2	1691	1140	0.05%	0.007%
83	12.665	3597	3600	3604	rBV3	1010	861	0.04%	0.005%
84	12.720	3613	3617	3623	rVB9	1806	2295	0.11%	0.015%
85	12.900	3669	3673	3676	rBV4	884	757	0.04%	0.005%
86	12.929	3676	3682	3690	rVB9	3030	4214	0.20%	0.027%
87	12.977	3694	3697	3702	rBV5	1518	1407	0.07%	0.009%
88	13.003	3702	3705	3711	rVB5	1047	1123	0.05%	0.007%
89	13.125	3736	3743	3755	rVB4	8529	14108	0.68%	0.090%
90	13.193	3760	3764	3766	rBV4	1536	1355	0.07%	0.009%
91	13.247	3779	3781	3784	rBV4	1518	1023	0.05%	0.006%
92	13.511	3853	3863	3873	rBV9	5401	10131	0.49%	0.064%
93	13.720	3922	3928	3930	rBV5	3501	3435	0.16%	0.022%
94	13.919	3988	3990	3992	rBV3	1032	577	0.03%	0.004%
95	13.961	3996	4003	4008	rVB8	2911	4519	0.22%	0.029%
96	14.012	4016	4019	4029	rVB9	2976	3836	0.18%	0.024%
97	14.131	4052	4056	4057	rBV3	1339	852	0.04%	0.005%
98	14.337	4112	4120	4124	rBV7	4966	7784	0.37%	0.049%
99	14.482	4159	4165	4170	rBV7	3064	4029	0.19%	0.026%
100	14.688	4222	4229	4230	rBV6	3506	4280	0.21%	0.027%


Sum of corrected areas: 15758750

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040719\
Data File : VU030811.D
Acq On : 06 Apr 2019 19:22
Operator : JC/SP
Sample : K2299-02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB6X6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

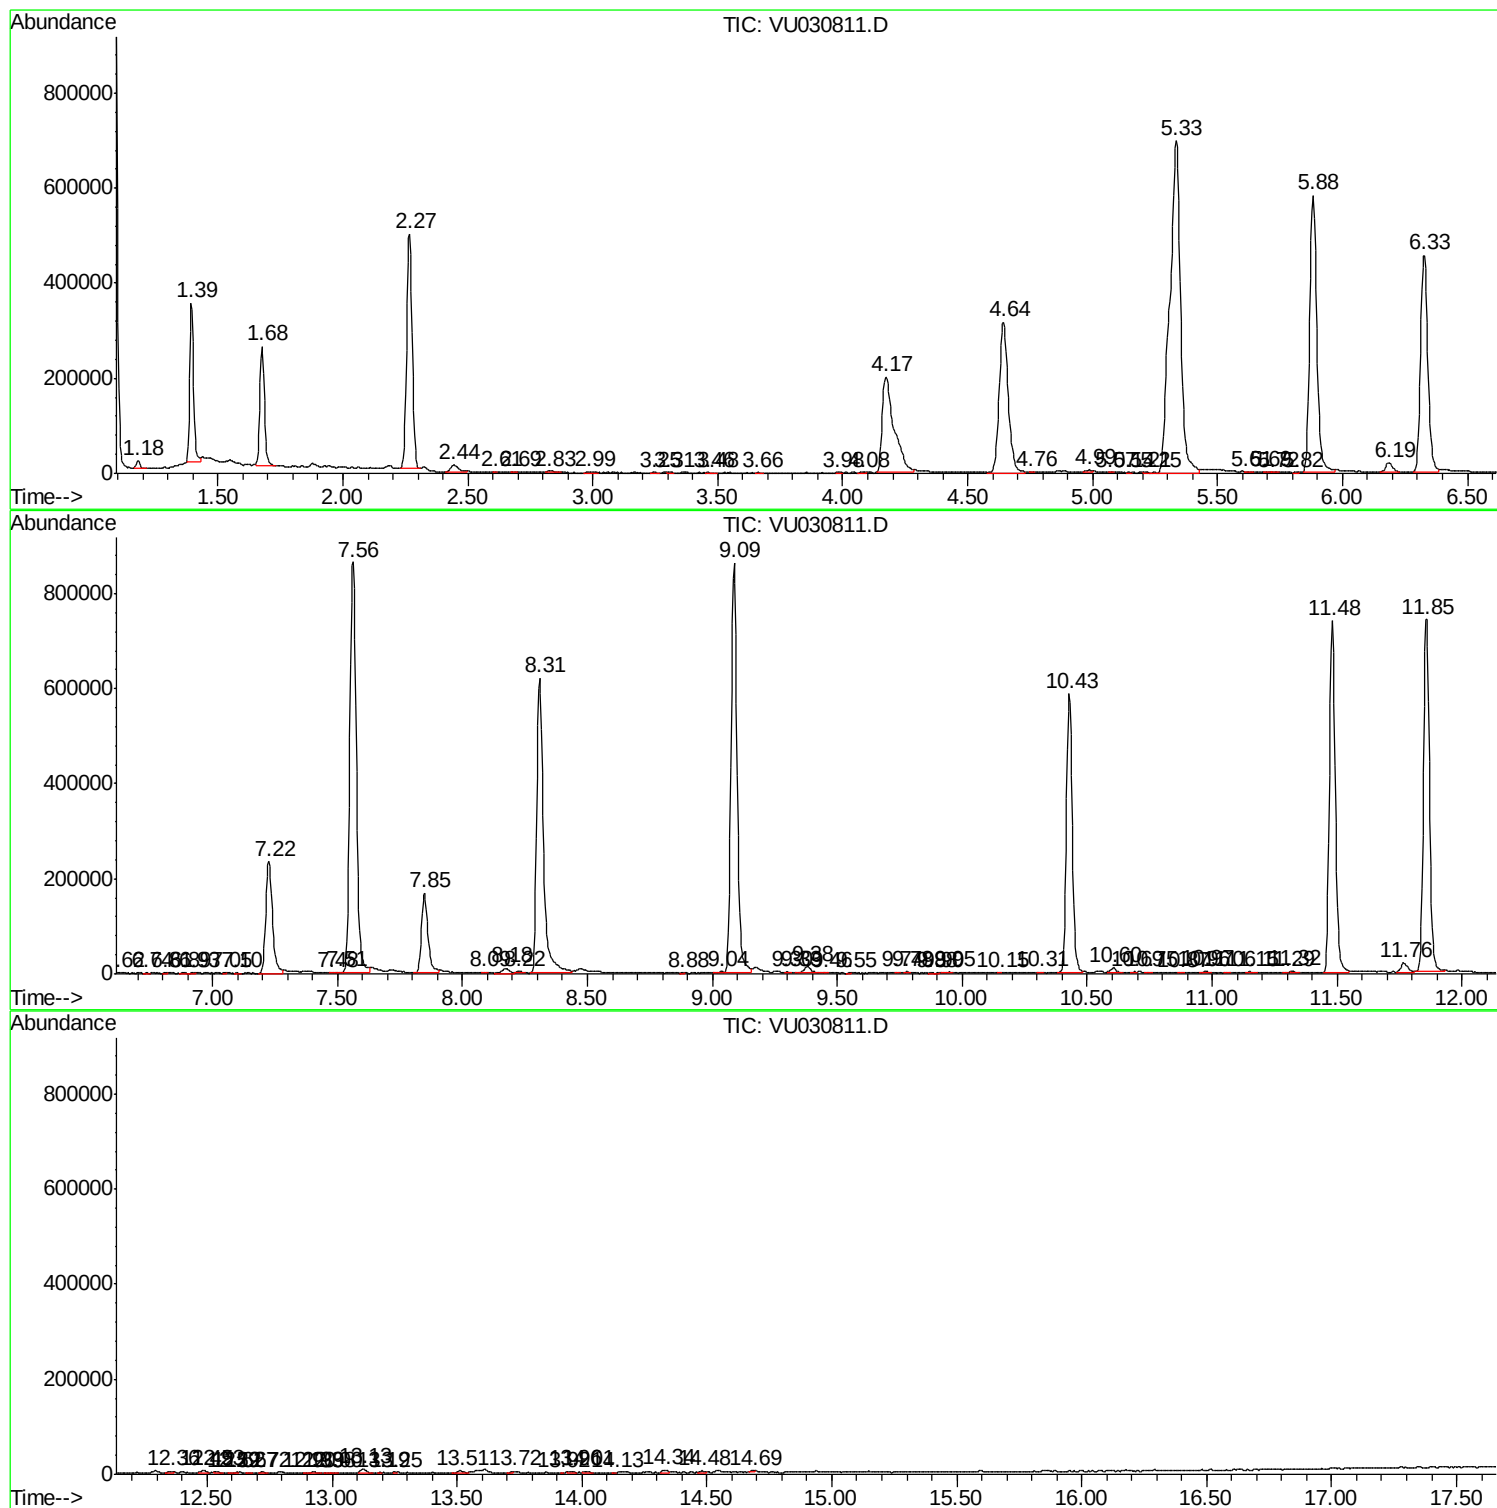

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040719\
Data File : VU030811.D
Acq On : 06 Apr 2019 19:22
Operator : JC/SP
Sample : K2299-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB6X6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040719\
Data File : VU030811.D
Acq On : 06 Apr 2019 19:22
Operator : JC/SP
Sample : K2299-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB6X6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc