

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040719\
 Data File : VU030831.D
 Acq On : 07 Apr 2019 03:24
 Operator : JC/SP
 Sample : K2260-09DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETJ58DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	37	rVB	14565	13013	0.65%	0.081%
2	1.395	88	95	109	rBV	318913	334590	16.71%	2.094%
3	1.675	174	182	197	rBV	232377	299231	14.94%	1.873%
4	2.267	355	366	379	rVB	480855	729503	36.43%	4.566%
5	2.617	473	475	479	rVB3	1022	775	0.04%	0.005%
6	2.640	479	482	485	rBV2	518	398	0.02%	0.002%
7	2.691	495	498	499	rBV3	1003	510	0.03%	0.003%
8	2.701	499	501	509	rVB6	2449	2704	0.14%	0.017%
9	2.778	520	525	527	rBV3	711	578	0.03%	0.004%
10	2.826	536	540	545	rBV3	985	1147	0.06%	0.007%
11	2.891	555	560	562	rBV	604	509	0.03%	0.003%
12	2.977	576	587	603	rVV2	30975	57931	2.89%	0.363%
13	3.087	618	621	627	rBV3	529	621	0.03%	0.004%
14	3.132	632	635	642	rVB4	684	709	0.04%	0.004%
15	3.167	642	646	650	rBV2	730	637	0.03%	0.004%
16	3.312	687	691	696	rVB3	732	890	0.04%	0.006%
17	3.434	727	729	735	rVB2	567	452	0.02%	0.003%
18	3.479	740	743	748	rVB	811	521	0.03%	0.003%
19	3.511	748	753	754	rBV	1149	974	0.05%	0.006%
20	3.579	769	774	778	rVB3	642	577	0.03%	0.004%
21	3.627	786	789	793	rVB4	774	596	0.03%	0.004%
22	3.649	793	796	802	rBV3	584	720	0.04%	0.005%
23	3.868	862	864	871	rVB2	657	458	0.02%	0.003%
24	3.907	871	876	879	rBV2	892	716	0.04%	0.004%
25	3.952	887	890	894	rVB2	489	410	0.02%	0.003%
26	4.173	946	959	963	rBV	212359	412150	20.58%	2.579%
27	4.643	1087	1105	1134	rBV	314857	788437	39.37%	4.934%
28	4.865	1172	1174	1178	rBV3	960	676	0.03%	0.004%
29	4.958	1201	1203	1208	rBV4	750	549	0.03%	0.003%
30	5.019	1219	1222	1227	rBV3	600	663	0.03%	0.004%
31	5.045	1227	1230	1232	rVV3	681	442	0.02%	0.003%
32	5.119	1249	1253	1257	rVB3	579	407	0.02%	0.003%
33	5.189	1271	1275	1278	rVB3	781	699	0.03%	0.004%
34	5.334	1295	1320	1344	rBV2	671564	2002617	100.00%	12.534%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040719\
 Data File : VU030831.D
 Acq On : 07 Apr 2019 03:24
 Operator : JC/SP
 Sample : K2260-09DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETJ58DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.652	1416	1419	1423	rBV5	756	703	0.04%	0.004%
36	5.733	1439	1444	1447	rBV5	638	641	0.03%	0.004%
37	5.749	1447	1449	1454	rVV5	1020	736	0.04%	0.005%
38	5.807	1464	1467	1472	rVB3	677	486	0.02%	0.003%
39	5.881	1475	1490	1515	rBV	570638	1142023	57.03%	7.147%
40	6.061	1542	1546	1552	rBV6	1416	1759	0.09%	0.011%
41	6.183	1570	1584	1606	rBV	566553	1117182	55.79%	6.992%
42	6.324	1615	1628	1648	rBV	454502	907030	45.29%	5.677%
43	6.611	1715	1717	1722	rVB3	976	684	0.03%	0.004%
44	6.646	1726	1728	1732	rVB3	1048	718	0.04%	0.004%
45	6.669	1732	1735	1739	rBV4	659	469	0.02%	0.003%
46	6.733	1750	1755	1758	rBV3	733	817	0.04%	0.005%
47	6.771	1764	1767	1770	rVB3	851	555	0.03%	0.003%
48	6.787	1770	1772	1775	rBV3	513	369	0.02%	0.002%
49	6.810	1775	1779	1783	rVB5	546	479	0.02%	0.003%
50	6.961	1824	1826	1831	rVB	948	660	0.03%	0.004%
51	7.112	1871	1873	1880	rVB3	617	551	0.03%	0.003%
52	7.225	1896	1908	1939	rBV	228877	432559	21.60%	2.707%
53	7.427	1969	1971	1974	rBV3	645	381	0.02%	0.002%
54	7.562	1999	2013	2033	rBV	838136	1477508	73.78%	9.247%
55	7.849	2088	2102	2121	rBV2	158669	288491	14.41%	1.806%
56	8.093	2177	2178	2182	rVV3	812	466	0.02%	0.003%
57	8.167	2196	2201	2203	rBV4	1677	1101	0.05%	0.007%
58	8.228	2211	2220	2234	rVB6	9477	17184	0.86%	0.108%
59	8.308	2234	2245	2277	rBV	608809	1159517	57.90%	7.257%
60	8.646	2346	2350	2355	rBV4	775	823	0.04%	0.005%
61	8.784	2390	2393	2399	rVB4	1274	1135	0.06%	0.007%
62	8.823	2401	2405	2406	rBV2	884	633	0.03%	0.004%
63	9.086	2471	2487	2517	rBV	832451	1436503	71.73%	8.990%
64	9.331	2562	2563	2567	rVB2	814	464	0.02%	0.003%
65	9.575	2635	2639	2642	rBV4	564	449	0.02%	0.003%
66	9.601	2645	2647	2653	rVB3	731	545	0.03%	0.003%
67	9.807	2705	2711	2714	rBV2	953	904	0.05%	0.006%
68	9.922	2742	2747	2750	rVB3	607	495	0.02%	0.003%
69	10.009	2769	2774	2776	rBV2	516	468	0.02%	0.003%
70	10.057	2785	2789	2795	rVB2	525	579	0.03%	0.004%
71	10.106	2800	2804	2808	rBV3	520	427	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040719\
 Data File : VU030831.D
 Acq On : 07 Apr 2019 03:24
 Operator : JC/SP
 Sample : K2260-09DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETJ58DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.199	2831	2833	2837	rVB3	734	433	0.02%	0.003%
73	10.228	2837	2842	2847	rVB2	889	923	0.05%	0.006%
74	10.257	2847	2851	2856	rBV2	720	975	0.05%	0.006%
75	10.363	2881	2884	2888	rBV2	784	794	0.04%	0.005%
76	10.427	2892	2904	2924	rBV	585325	953856	47.63%	5.970%
77	10.594	2950	2956	2960	rBV5	1375	1662	0.08%	0.010%
78	10.900	3048	3051	3055	rBV3	666	568	0.03%	0.004%
79	10.942	3061	3064	3071	rVB2	558	582	0.03%	0.004%
80	10.987	3075	3078	3084	rVB2	552	618	0.03%	0.004%
81	11.048	3094	3097	3100	rVV2	542	406	0.02%	0.003%
82	11.080	3105	3107	3111	rVB5	1205	608	0.03%	0.004%
83	11.176	3135	3137	3142	rVB3	834	650	0.03%	0.004%
84	11.205	3142	3146	3147	rBV	688	501	0.03%	0.003%
85	11.273	3163	3167	3171	rBV2	751	640	0.03%	0.004%
86	11.337	3182	3187	3190	rVB2	606	501	0.03%	0.003%
87	11.366	3190	3196	3198	rBV2	891	993	0.05%	0.006%
88	11.427	3213	3215	3219	rBV3	696	455	0.02%	0.003%
89	11.482	3219	3232	3255	rBV	695917	1165233	58.19%	7.293%
90	11.694	3295	3298	3302	rVB2	1453	966	0.05%	0.006%
91	11.858	3336	3349	3380	rBV	707695	1188551	59.35%	7.439%
92	12.353	3500	3503	3504	rBV2	777	464	0.02%	0.003%
93	12.755	3625	3628	3630	rBV2	777	494	0.02%	0.003%
94	13.083	3728	3730	3735	rVB2	848	501	0.03%	0.003%
95	13.202	3764	3767	3774	rBV3	1046	1284	0.06%	0.008%
96	13.315	3798	3802	3806	rBV3	800	828	0.04%	0.005%
97	13.434	3837	3839	3845	rVB	1298	828	0.04%	0.005%
98	13.466	3845	3849	3852	rBV3	654	580	0.03%	0.004%
99	13.729	3928	3931	3934	rBV2	772	446	0.02%	0.003%
100	13.839	3962	3965	3968	rBV2	773	454	0.02%	0.003%


Sum of corrected areas: 15978098

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040719\
Data File : VU030831.D
Acq On : 07 Apr 2019 03:24
Operator : JC/SP
Sample : K2260-09DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETJ58DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

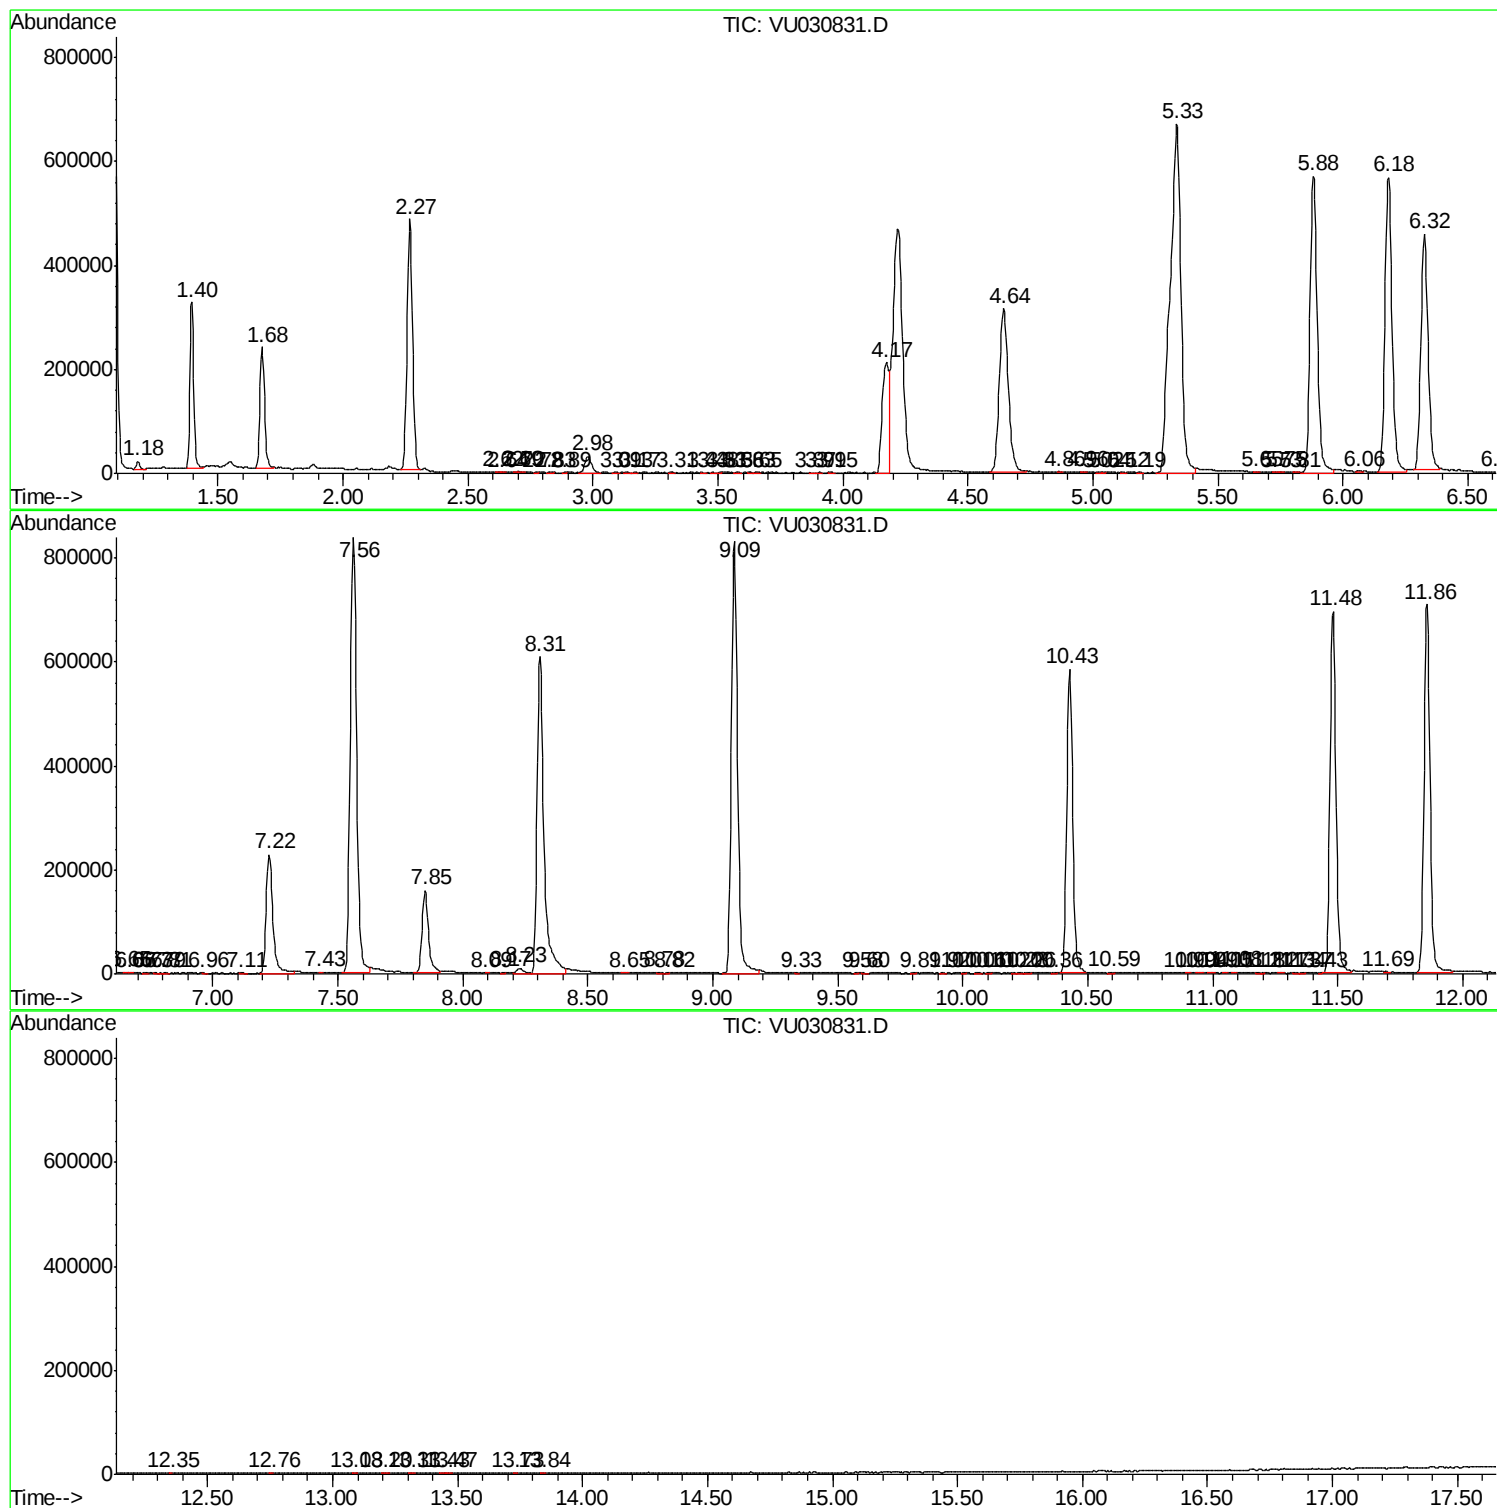

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040719\
Data File : VU030831.D
Acq On : 07 Apr 2019 03:24
Operator : JC/SP
Sample : K2260-09DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETJ58DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040719\
Data File : VU030831.D
Acq On : 07 Apr 2019 03:24
Operator : JC/SP
Sample : K2260-09DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETJ58DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc