

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040719\
 Data File : VU030834.D
 Acq On : 07 Apr 2019 04:33
 Operator : JC/SP
 Sample : K2327-08 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2S2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	37	rVB3	14812	14362	0.71%	0.095%
2	1.395	88	95	107	rBV	329927	340592	16.91%	2.253%
3	1.675	174	182	196	rBV	234789	304151	15.10%	2.012%
4	2.267	355	366	379	rVB	485869	742627	36.87%	4.912%
5	2.434	415	418	420	rBV3	1631	1236	0.06%	0.008%
6	2.476	428	431	435	rBV4	1163	1014	0.05%	0.007%
7	2.691	492	498	499	rBV3	2099	1839	0.09%	0.012%
8	2.736	510	512	520	rBV3	663	716	0.04%	0.005%
9	2.775	520	524	526	rBV2	637	446	0.02%	0.003%
10	2.810	533	535	538	rBV3	548	405	0.02%	0.003%
11	2.829	538	541	547	rVB4	951	712	0.04%	0.005%
12	2.862	547	551	555	rBV3	723	618	0.03%	0.004%
13	2.974	583	586	590	rBV3	565	407	0.02%	0.003%
14	3.039	605	606	613	rVB3	527	501	0.02%	0.003%
15	3.190	649	653	655	rBV2	675	501	0.02%	0.003%
16	3.318	690	693	696	rBV	1095	738	0.04%	0.005%
17	3.341	696	700	702	rBV3	636	546	0.03%	0.004%
18	3.411	718	722	724	rBV3	559	393	0.02%	0.003%
19	3.489	743	746	749	rBV2	441	393	0.02%	0.003%
20	3.543	759	763	767	rBV2	731	644	0.03%	0.004%
21	3.669	799	802	805	rVV2	634	510	0.03%	0.003%
22	3.714	809	816	820	rVB5	456	638	0.03%	0.004%
23	3.826	846	851	853	rBV3	817	620	0.03%	0.004%
24	3.849	856	858	861	rBV	469	391	0.02%	0.003%
25	4.003	903	906	913	rVB3	474	493	0.02%	0.003%
26	4.083	927	931	934	rVB2	614	427	0.02%	0.003%
27	4.109	934	939	941	rBV	572	395	0.02%	0.003%
28	4.170	945	958	990	rBV	207573	567211	28.16%	3.752%
29	4.524	1066	1068	1072	rBV3	964	667	0.03%	0.004%
30	4.643	1088	1105	1131	rBV	315166	798752	39.66%	5.283%
31	4.952	1199	1201	1204	rVB3	854	440	0.02%	0.003%
32	5.035	1224	1227	1232	rVB3	660	610	0.03%	0.004%
33	5.067	1232	1237	1242	rBV4	655	856	0.04%	0.006%
34	5.135	1254	1258	1263	rVB3	1005	851	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040719\
 Data File : VU030834.D
 Acq On : 07 Apr 2019 04:33
 Operator : JC/SP
 Sample : K2327-08 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2S2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.334	1297	1320	1343	rBV2	677875	2014060	100.00%	13.322%
36	5.678	1425	1427	1432	rVB4	1087	811	0.04%	0.005%
37	5.881	1477	1490	1512	rBV	567091	1146133	56.91%	7.581%
38	6.186	1574	1585	1596	rVB10	5778	12388	0.62%	0.082%
39	6.263	1606	1609	1612	rBV	693	341	0.02%	0.002%
40	6.328	1612	1629	1653	rBV	455729	935694	46.46%	6.189%
41	6.582	1706	1708	1713	rVB4	885	693	0.03%	0.005%
42	6.771	1765	1767	1773	rVB4	670	551	0.03%	0.004%
43	6.945	1817	1821	1824	rBV	585	539	0.03%	0.004%
44	7.019	1842	1844	1850	rVB3	587	486	0.02%	0.003%
45	7.148	1879	1884	1886	rVB3	533	446	0.02%	0.003%
46	7.225	1895	1908	1927	rBV	230579	421321	20.92%	2.787%
47	7.505	1992	1995	2000	rVB3	904	806	0.04%	0.005%
48	7.562	2000	2013	2037	rBV	843694	1502408	74.60%	9.937%
49	7.849	2090	2102	2121	rBV	157721	288519	14.33%	1.908%
50	7.987	2143	2145	2150	rVB5	1209	735	0.04%	0.005%
51	8.009	2150	2152	2154	rVV2	871	401	0.02%	0.003%
52	8.022	2154	2156	2161	rVB2	1027	721	0.04%	0.005%
53	8.048	2161	2164	2165	rBV3	736	394	0.02%	0.003%
54	8.058	2165	2167	2171	rVB2	698	465	0.02%	0.003%
55	8.135	2189	2191	2195	rBV4	875	758	0.04%	0.005%
56	8.225	2212	2219	2229	rVB6	7667	12740	0.63%	0.084%
57	8.308	2234	2245	2278	rBV	610573	1182867	58.73%	7.824%
58	8.681	2358	2361	2364	rBV3	1070	922	0.05%	0.006%
59	8.720	2371	2373	2377	rBV3	590	365	0.02%	0.002%
60	8.739	2377	2379	2384	rVB2	920	572	0.03%	0.004%
61	8.839	2404	2410	2413	rBV4	945	1069	0.05%	0.007%
62	8.910	2428	2432	2434	rBV3	726	577	0.03%	0.004%
63	8.942	2437	2442	2446	rBV3	957	1089	0.05%	0.007%
64	9.086	2474	2487	2516	rBV	844528	1441307	71.56%	9.533%
65	9.617	2649	2652	2657	rBV2	656	520	0.03%	0.003%
66	9.685	2671	2673	2678	rVB2	597	478	0.02%	0.003%
67	9.723	2682	2685	2687	rBV2	633	390	0.02%	0.003%
68	9.865	2725	2729	2731	rBV3	776	619	0.03%	0.004%
69	9.932	2747	2750	2753	rBV3	778	466	0.02%	0.003%
70	10.041	2780	2784	2787	rBV2	624	506	0.03%	0.003%
71	10.180	2824	2827	2833	rVB3	596	668	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040719\
 Data File : VU030834.D
 Acq On : 07 Apr 2019 04:33
 Operator : JC/SP
 Sample : K2327-08 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2S2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.225	2833	2841	2846	rBV6	819	1472	0.07%	0.010%
73	10.340	2873	2877	2880	rVV2	619	522	0.03%	0.003%
74	10.427	2890	2904	2931	rBV	596768	981185	48.72%	6.490%
75	10.710	2989	2992	2998	rBV5	492	540	0.03%	0.004%
76	11.019	3084	3088	3089	rBV	648	424	0.02%	0.003%
77	11.389	3201	3203	3207	rVB3	593	346	0.02%	0.002%
78	11.408	3207	3209	3211	rBV3	697	354	0.02%	0.002%
79	11.424	3211	3214	3217	rBV2	593	410	0.02%	0.003%
80	11.482	3220	3232	3250	rBV	710623	1155036	57.35%	7.640%
81	11.855	3336	3348	3373	rBV	714167	1207425	59.95%	7.986%
82	12.250	3468	3471	3473	rBV2	895	532	0.03%	0.004%
83	12.356	3501	3504	3507	rBV3	823	583	0.03%	0.004%
84	12.385	3510	3513	3515	rBV2	608	370	0.02%	0.002%
85	12.549	3562	3564	3568	rVB3	986	524	0.03%	0.003%
86	12.572	3568	3571	3574	rBV2	687	437	0.02%	0.003%
87	12.800	3640	3642	3644	rBV2	681	446	0.02%	0.003%
88	12.900	3670	3673	3677	rBV3	770	708	0.04%	0.005%
89	12.938	3682	3685	3687	rVV3	1062	613	0.03%	0.004%
90	12.964	3690	3693	3696	rBV2	1387	1139	0.06%	0.008%
91	13.086	3729	3731	3733	rVB	925	395	0.02%	0.003%
92	13.102	3733	3736	3739	rBV	616	453	0.02%	0.003%
93	13.164	3753	3755	3759	rBV2	849	619	0.03%	0.004%
94	13.517	3862	3865	3868	rBV2	935	728	0.04%	0.005%
95	13.536	3868	3871	3875	rVV	1027	724	0.04%	0.005%
96	13.565	3877	3880	3885	rVV2	797	693	0.03%	0.005%
97	13.691	3917	3919	3922	rBV2	782	484	0.02%	0.003%
98	13.794	3948	3951	3953	rBV	1018	666	0.03%	0.004%
99	14.337	4118	4120	4123	rBV2	756	590	0.03%	0.004%
100	14.880	4286	4289	4291	rBV3	1131	875	0.04%	0.006%


Sum of corrected areas: 15118820

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040719\
Data File : VU030834.D
Acq On : 07 Apr 2019 04:33
Operator : JC/SP
Sample : K2327-08 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF2S2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

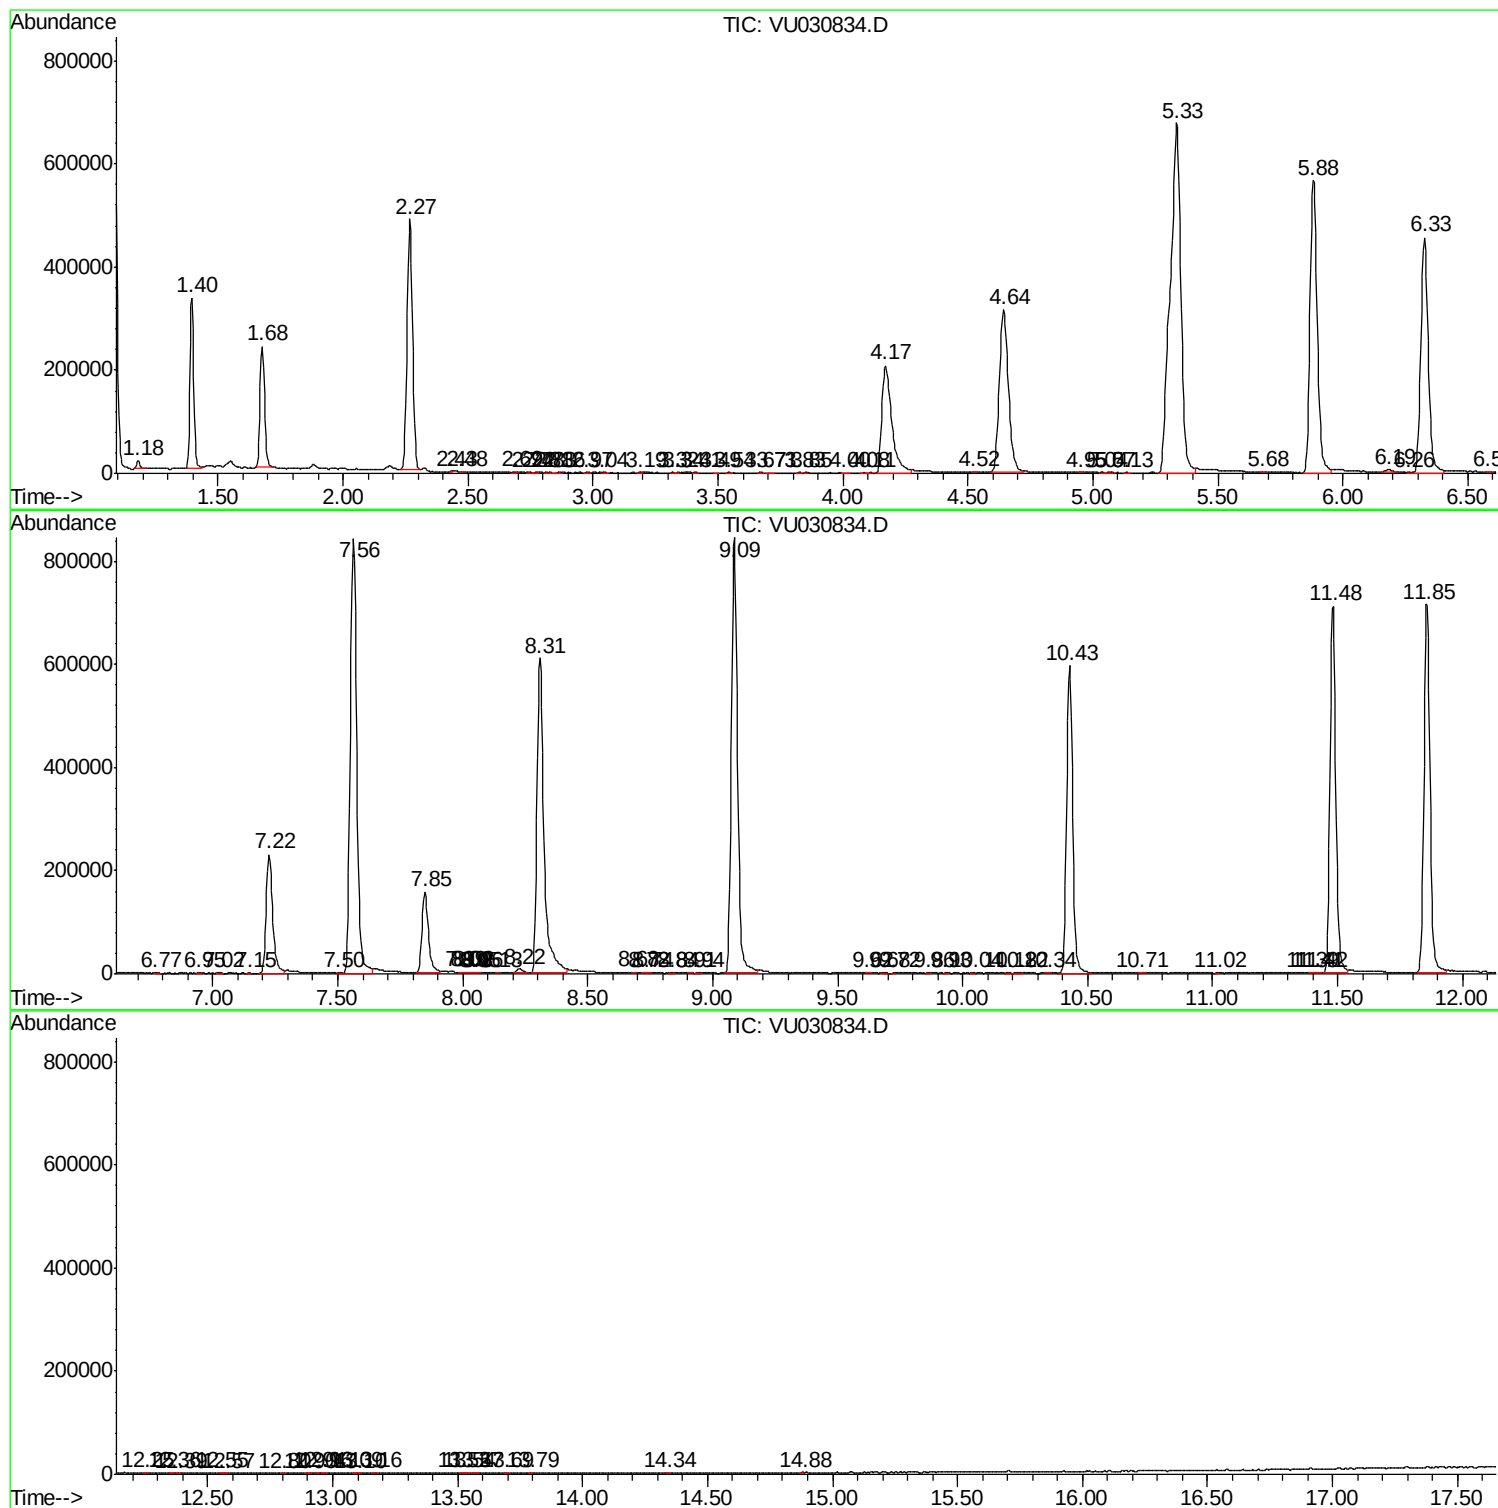

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040719\
Data File : VU030834.D
Acq On : 07 Apr 2019 04:33
Operator : JC/SP
Sample : K2327-08 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF2S2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040719\
Data File : VU030834.D
Acq On : 07 Apr 2019 04:33
Operator : JC/SP
Sample : K2327-08 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF2S2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc