


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040719\
 Data File : VU030792.D
 Acq On : 06 Apr 2019 11:59
 Operator : JC/SP
 Sample : BFB52
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB52

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 09 02:16:31 2019

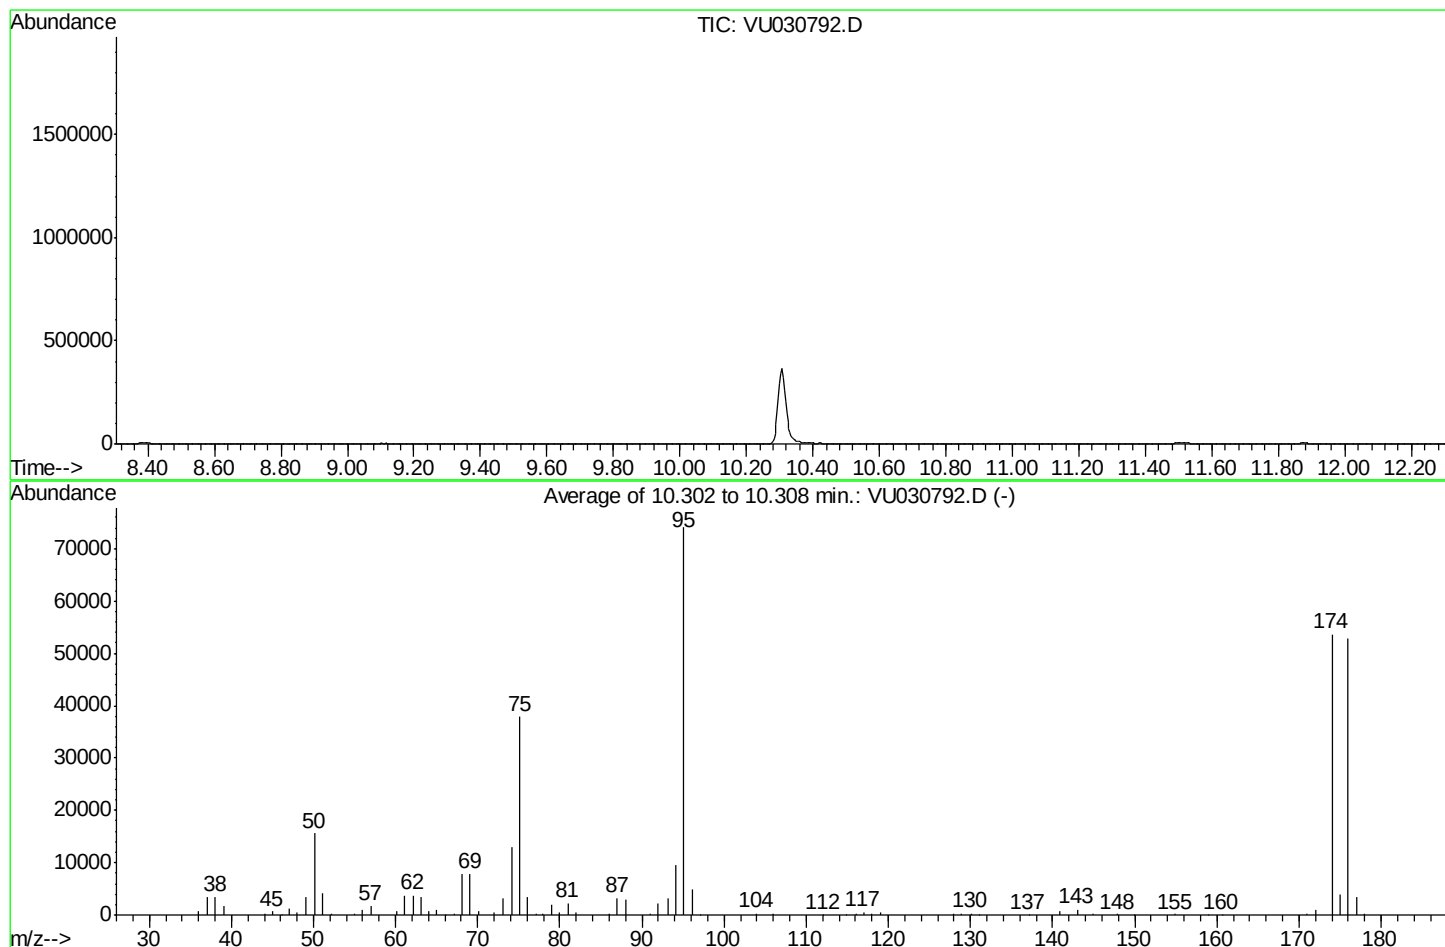

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	15637	PASS
75	95	30	80	51.2	37914	PASS
95	95	100	100	100.0	74082	PASS
96	95	5	9	6.7	4957	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.4	53658	PASS
175	174	5	9	7.2	3869	PASS
176	174	95	101	98.6	52893	PASS
177	176	5	9	6.3	3358	PASS

Scan 2854 (10.267 min): VU030792.D
BFB52

m/z	Abundance
39.90	492.0
44.00	800.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	706.0
37.00	3466.0
38.10	3420.0
39.10	1679.0
39.90	433.0
44.00	1189.0
44.90	735.0
47.10	1228.0
47.90	526.0
49.00	3162.0
50.10	15691.0
51.10	4431.0
52.20	181.0
54.90	197.0
56.00	999.0
57.00	1841.0
60.10	713.0
61.10	3795.0
62.10	3653.0
63.00	3511.0
64.10	654.0
65.00	1008.0
67.10	132.0
68.00	7293.0
69.10	7753.0
70.10	690.0
72.10	553.0
73.10	3002.0
74.10	12351.0
75.10	37072.0
76.10	3398.0
77.10	362.0
77.90	338.0
79.00	2072.0
79.80	558.0
81.00	2388.0
81.90	621.0
86.00	263.0
87.00	3043.0
88.10	2726.0
91.10	292.0
92.00	1998.0
93.10	3185.0
94.10	9177.0
95.10	70768.0
96.10	4822.0
97.10	105.0
103.90	353.0
105.90	354.0
116.10	228.0
117.00	544.0
117.90	328.0
119.00	362.0
128.00	257.0
128.80	170.0
130.10	228.0
140.90	675.0
143.00	954.0
145.00	317.0
148.00	109.0
154.90	140.0
170.90	193.0
172.10	862.0
174.00	50928.0
175.00	3612.0
176.00	49944.0
177.10	3279.0
177.90	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	752.0
37.00	3402.0
38.10	3681.0
39.10	1883.0
39.90	454.0
44.00	1130.0
45.00	738.0
46.10	105.0
47.10	1214.0
47.90	618.0
49.10	3653.0
50.10	16076.0
51.10	4293.0
52.20	206.0
55.00	238.0
56.00	1139.0
57.00	1917.0
60.10	769.0
61.10	3860.0
62.10	3936.0
63.10	3640.0
64.10	700.0
65.00	1120.0
66.00	169.0
67.10	150.0
68.00	8153.0
69.10	8243.0
70.10	738.0
72.10	520.0
73.10	3255.0
74.10	13299.0
75.10	39336.0
76.10	3403.0
77.10	319.0
77.90	290.0
79.00	2113.0
79.80	623.0
81.00	2351.0
82.00	582.0
86.00	317.0
87.00	3439.0
88.10	3074.0
91.10	295.0
92.00	2245.0
93.10	3307.0
94.10	9755.0
95.10	76576.0
96.10	5112.0
97.10	109.0
104.00	273.0
105.90	307.0
112.10	103.0
116.10	271.0
117.00	578.0
118.00	336.0
119.00	448.0
128.00	265.0
128.80	231.0
130.10	283.0
131.10	112.0
137.10	122.0
140.90	719.0
143.10	1140.0
145.00	282.0
147.90	139.0
155.00	217.0
170.90	150.0
172.10	869.0
174.00	55296.0
175.00	3982.0
176.00	54432.0
177.10	3427.0
177.90	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	753.0
37.00	3301.0
38.00	3480.0
39.10	1880.0
40.00	495.0
44.00	1178.0
45.00	710.0
46.00	131.0
47.10	1007.0
48.00	645.0
49.10	3755.0
50.10	15145.0
51.10	4087.0
52.30	217.0
54.90	323.0
56.00	1080.0
57.00	1715.0
60.10	675.0
61.10	3392.0
62.10	3776.0
63.10	3380.0
64.00	722.0
65.00	1008.0
66.00	199.0
67.20	153.0
68.10	8183.0
69.00	7811.0
70.00	656.0
72.00	485.0
73.10	3314.0
74.10	13272.0
75.10	37336.0
76.10	3231.0
77.10	296.0
79.00	1972.0
79.90	664.0
81.00	2099.0
82.00	460.0
86.00	240.0
87.00	3287.0
88.00	3194.0
90.90	361.0
92.00	2307.0
93.10	3032.0
94.10	9428.0
95.10	74904.0
96.10	4939.0
97.00	106.0
104.10	307.0
105.90	244.0
112.10	116.0
114.80	124.0
116.10	254.0
117.00	569.0
118.00	300.0
119.00	461.0
127.90	210.0
128.80	218.0
130.10	290.0
131.10	222.0
137.10	127.0
140.90	682.0
143.00	1089.0
145.00	308.0
147.90	181.0
149.90	121.0
155.00	232.0
159.00	136.0
160.60	108.0
170.90	102.0
172.00	913.0
174.00	54752.0
175.00	4013.0
176.00	54304.0
177.00	3370.0
178.00	190.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52