

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040720\
 Data File : VU037599.D
 Acq On : 07 Apr 2020 10:35
 Operator : JC/MD
 Sample : VU0407WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	77	85	94	rBV	112137	117404	16.66%	2.192%
2	1.929	175	183	195	rBV	77157	101701	14.43%	1.899%
3	2.591	377	389	407	rBV	154761	252948	35.89%	4.723%
4	2.819	456	460	467	rVB	437	432	0.06%	0.008%
5	2.900	480	485	486	rBV2	237	188	0.03%	0.004%
6	2.948	498	500	502	rBV	147	47	0.01%	0.001%
7	2.977	506	509	512	rBV	224	126	0.02%	0.002%
8	3.076	537	540	545	rBV2	309	223	0.03%	0.004%
9	3.266	596	599	601	rBV	117	77	0.01%	0.001%
10	3.369	628	631	634	rBV	214	192	0.03%	0.004%
11	3.462	658	660	661	rBV	139	35	0.00%	0.001%
12	3.539	682	684	688	rBV	147	55	0.01%	0.001%
13	3.572	692	694	697	rBV	197	121	0.02%	0.002%
14	3.748	746	749	751	rBV	200	102	0.01%	0.002%
15	3.880	787	790	794	rBV	224	244	0.03%	0.005%
16	3.903	794	797	799	rVV2	204	144	0.02%	0.003%
17	3.941	807	809	814	rBV	176	104	0.01%	0.002%
18	3.964	814	816	821	rVB	322	168	0.02%	0.003%
19	4.064	844	847	855	rVB	221	173	0.02%	0.003%
20	4.121	861	865	868	rBB	174	169	0.02%	0.003%
21	4.144	868	872	875	rBV	199	236	0.03%	0.004%
22	4.186	880	885	888	rBV2	396	463	0.07%	0.009%
23	4.285	915	916	917	rBV	162	41	0.01%	0.001%
24	4.327	928	929	930	rBV	117	27	0.00%	0.001%
25	4.417	955	957	959	rBV	119	59	0.01%	0.001%
26	4.501	980	983	986	rVB2	219	149	0.02%	0.003%
27	4.665	1020	1034	1060	rBV	79220	186120	26.41%	3.475%
28	4.829	1082	1085	1088	rBV2	429	323	0.05%	0.006%
29	4.912	1110	1111	1114	rBV	225	80	0.01%	0.001%
30	5.102	1153	1170	1191	rVB	126432	273660	38.83%	5.110%
31	5.176	1191	1193	1194	rBV	232	124	0.02%	0.002%
32	5.237	1209	1212	1213	rBV	160	107	0.02%	0.002%
33	5.324	1235	1239	1240	rBV	353	307	0.04%	0.006%
34	5.453	1277	1279	1281	rBV	115	50	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040720\
 Data File : VU037599.D
 Acq On : 07 Apr 2020 10:35
 Operator : JC/MD
 Sample : VU0407WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

35	5.572	1314	1316	1317	rBV	270	69	0.01%	0.001%
36	5.761	1352	1375	1394	rBV2	270789	704849	100.00%	13.161%
37	5.951	1432	1434	1439	rVB2	230	163	0.02%	0.003%
38	5.996	1445	1448	1452	rVB	222	156	0.02%	0.003%
39	6.041	1460	1462	1464	rVB	200	81	0.01%	0.002%
40	6.144	1491	1494	1498	rVB	369	276	0.04%	0.005%
41	6.211	1514	1515	1517	rVB	164	41	0.01%	0.001%
42	6.282	1522	1537	1552	rBV	192047	356272	50.55%	6.652%
43	6.401	1572	1574	1577	rVB2	314	176	0.02%	0.003%
44	6.433	1582	1584	1585	rBV2	148	47	0.01%	0.001%
45	6.523	1610	1612	1613	rBV2	181	60	0.01%	0.001%
46	6.723	1660	1674	1692	rBV	170601	322575	45.77%	6.023%
47	6.835	1707	1709	1714	rBV2	390	364	0.05%	0.007%
48	7.083	1782	1786	1787	rBV	189	161	0.02%	0.003%
49	7.192	1817	1820	1823	rBV	258	208	0.03%	0.004%
50	7.211	1823	1826	1828	rVB2	271	189	0.03%	0.004%
51	7.240	1833	1835	1837	rVV	220	79	0.01%	0.001%
52	7.305	1853	1855	1858	rBV	174	60	0.01%	0.001%
53	7.427	1891	1893	1898	rBV	173	85	0.01%	0.002%
54	7.452	1898	1901	1902	rBV	130	50	0.01%	0.001%
55	7.488	1910	1912	1914	rBV	158	54	0.01%	0.001%
56	7.536	1925	1927	1932	rVB	185	87	0.01%	0.002%
57	7.591	1932	1944	1959	rBV	109191	185689	26.34%	3.467%
58	7.700	1976	1978	1980	rVB	259	97	0.01%	0.002%
59	7.755	1994	1995	2000	rVB	137	55	0.01%	0.001%
60	7.822	2008	2016	2021	rBV3	541	791	0.11%	0.015%
61	7.922	2033	2047	2063	rBV	340203	581507	82.50%	10.858%
62	8.076	2091	2095	2098	rBV	239	215	0.03%	0.004%
63	8.202	2123	2134	2147	rBV	75983	125309	17.78%	2.340%
64	8.298	2161	2164	2165	rBV2	150	85	0.01%	0.002%
65	8.443	2208	2209	2210	rBV	137	31	0.00%	0.001%
66	8.517	2230	2232	2234	rBV	150	68	0.01%	0.001%
67	8.613	2256	2262	2263	rBV	242	234	0.03%	0.004%
68	8.655	2263	2275	2301	rVV	237704	410812	58.28%	7.671%
69	8.800	2317	2320	2326	rVB	320	255	0.04%	0.005%
70	8.938	2354	2363	2369	rBV	2202	3362	0.48%	0.063%
71	8.977	2373	2375	2378	rVB	302	106	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040720\
 Data File : VU037599.D
 Acq On : 07 Apr 2020 10:35
 Operator : JC/MD
 Sample : VU0407WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

72	9.050	2395	2398	2399	rBV	164	79	0.01%	0.001%
73	9.134	2422	2424	2428	rVB	219	107	0.02%	0.002%
74	9.195	2440	2443	2444	rBV	167	73	0.01%	0.001%
75	9.436	2505	2518	2535	rBV	272321	440324	62.47%	8.222%
76	9.591	2562	2566	2569	rBV2	255	236	0.03%	0.004%
77	9.883	2655	2657	2658	rBV	153	44	0.01%	0.001%
78	10.179	2747	2749	2752	rVB	304	117	0.02%	0.002%
79	10.774	2922	2934	2951	rVB	222276	352265	49.98%	6.577%
80	10.899	2970	2973	2980	rBV	488	250	0.04%	0.005%
81	11.475	3150	3152	3155	rBV3	619	405	0.06%	0.008%
82	11.758	3236	3240	3241	rBV	426	263	0.04%	0.005%
83	11.825	3249	3261	3277	rVB	270012	420157	59.61%	7.845%
84	12.205	3367	3379	3397	rVB	315522	501387	71.13%	9.362%
85	12.800	3557	3564	3569	rVB2	658	737	0.10%	0.014%
86	13.870	3889	3897	3903	rVB4	982	1476	0.21%	0.028%
87	13.899	3903	3906	3908	rBV	359	227	0.03%	0.004%
88	14.118	3965	3974	3983	rVB2	4202	6159	0.87%	0.115%
89	15.674	4457	4458	4462	rBV	467	249	0.04%	0.005%


Sum of corrected areas: 5355672

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040720\
Data File : VU037599.D
Acq On : 07 Apr 2020 10:35
Operator : JC/MD
Sample : VU0407WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK48

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

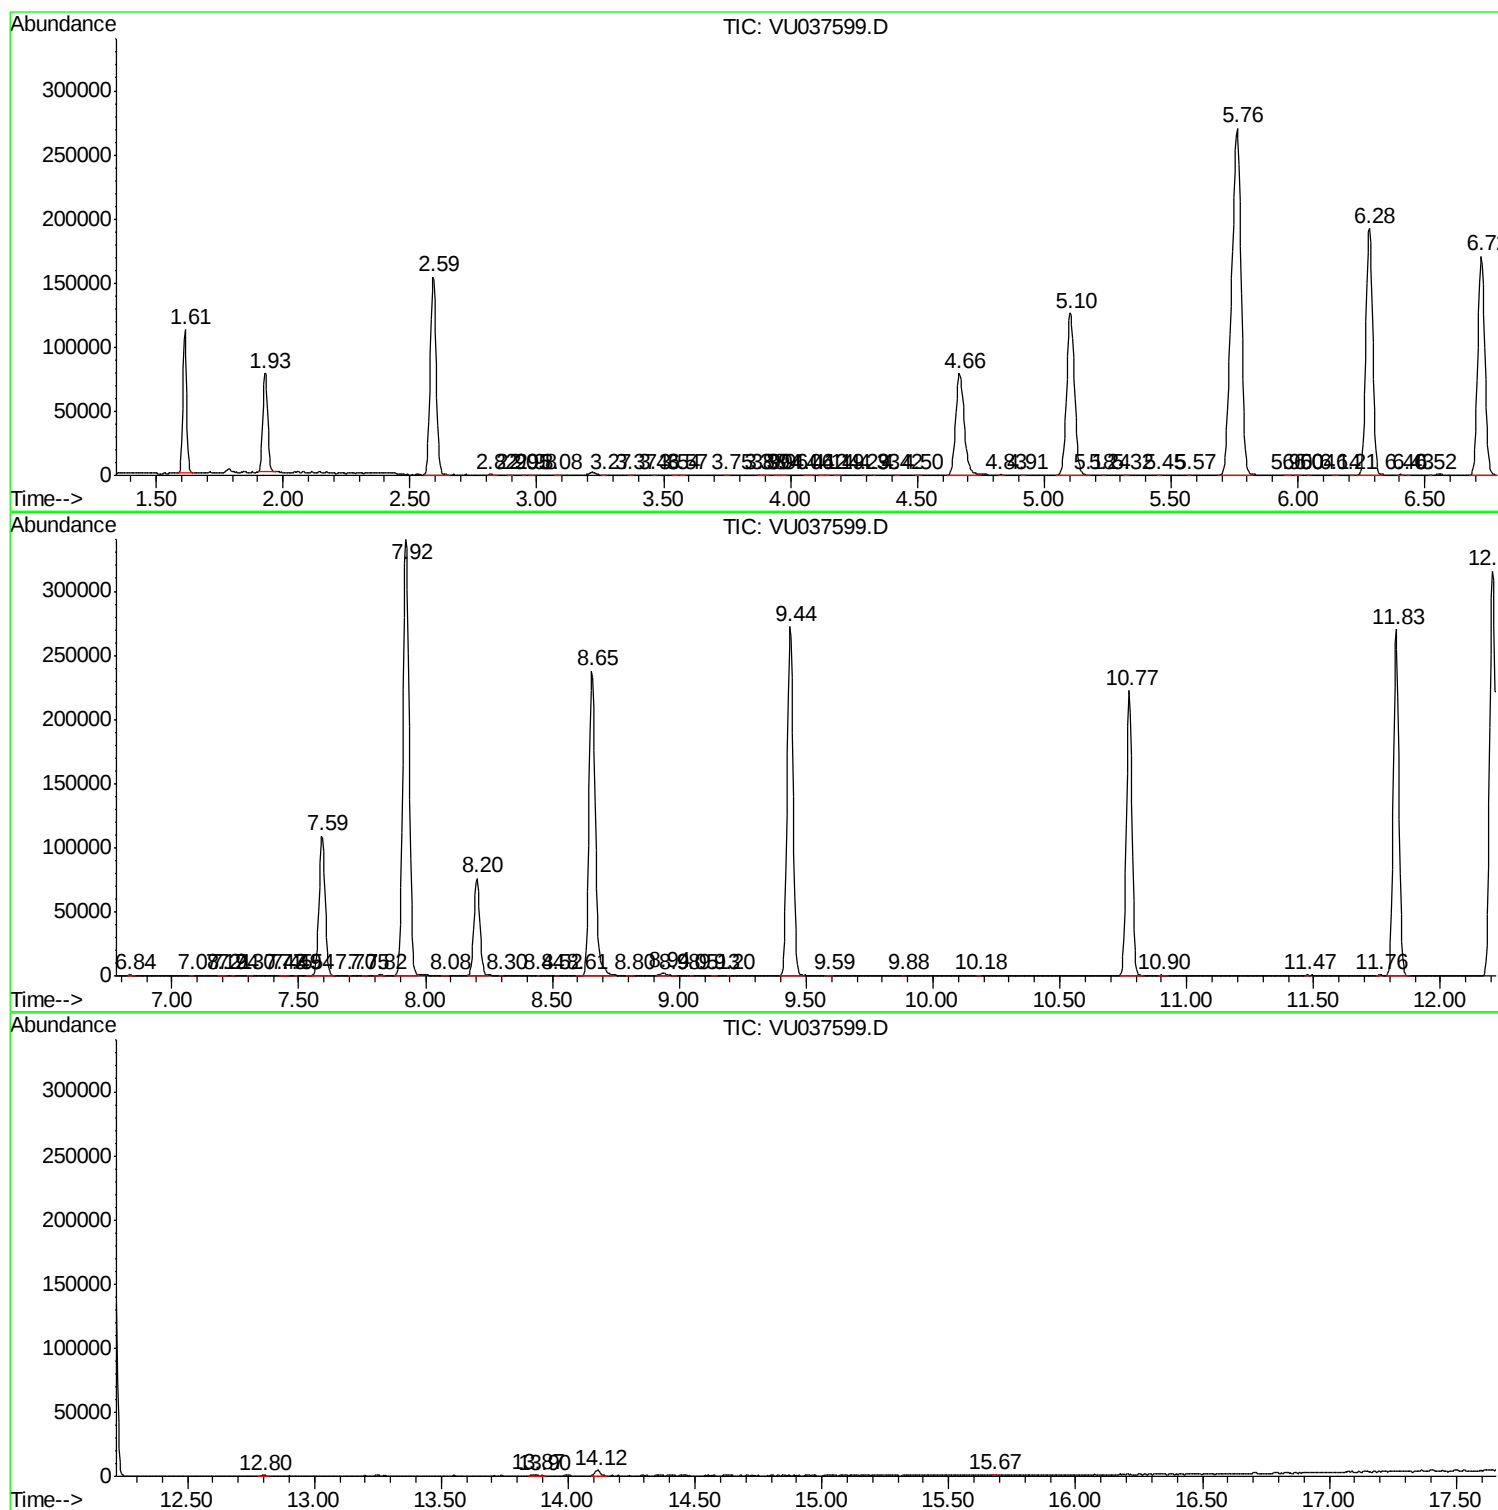

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040720\
Data File : VU037599.D
Acq On : 07 Apr 2020 10:35
Operator : JC/MD
Sample : VU0407WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK48

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040720\
Data File : VU037599.D
Acq On : 07 Apr 2020 10:35
Operator : JC/MD
Sample : VU0407WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK48

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc