

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040720\
 Data File : VU037603.D
 Acq On : 07 Apr 2020 12:33
 Operator : JC/MD
 Sample : L2173-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFS69

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	93	rBV	94049	100770	15.60%	1.901%
2	1.928	176	183	199	rVB	71315	94053	14.56%	1.775%
3	2.591	377	389	406	rBV	140198	228922	35.44%	4.319%
4	2.790	440	451	464	rBV	7047	12866	1.99%	0.243%
5	2.951	498	501	504	rVB2	311	160	0.02%	0.003%
6	3.105	546	549	552	rVB	208	127	0.02%	0.002%
7	3.215	577	583	584	rBV	666	627	0.10%	0.012%
8	3.256	595	596	598	rBV	175	85	0.01%	0.002%
9	3.752	748	750	753	rVB	228	111	0.02%	0.002%
10	3.819	768	771	776	rVB	298	193	0.03%	0.004%
11	3.970	817	818	819	rBV	120	33	0.01%	0.001%
12	4.006	828	829	832	rBV	130	48	0.01%	0.001%
13	4.208	890	892	896	rVB2	262	197	0.03%	0.004%
14	4.356	934	938	940	rBV	208	193	0.03%	0.004%
15	4.369	940	942	945	rVB	157	86	0.01%	0.002%
16	4.436	962	963	965	rVB	174	39	0.01%	0.001%
17	4.668	1019	1035	1062	rBV	71946	177820	27.53%	3.355%
18	4.874	1097	1099	1101	rBV	175	78	0.01%	0.001%
19	4.896	1104	1106	1108	rVB	188	56	0.01%	0.001%
20	4.967	1126	1128	1130	rBV	137	37	0.01%	0.001%
21	5.002	1137	1139	1140	rBV	131	72	0.01%	0.001%
22	5.031	1145	1148	1152	rVV	295	194	0.03%	0.004%
23	5.102	1154	1170	1188	rVV2	116214	251649	38.96%	4.748%
24	5.189	1194	1197	1203	rBV	158	145	0.02%	0.003%
25	5.346	1240	1246	1247	rBV2	847	896	0.14%	0.017%
26	5.552	1308	1310	1311	rVB	111	25	0.00%	0.000%
27	5.761	1351	1375	1394	rBV2	246148	645859	100.00%	12.186%
28	5.931	1426	1428	1431	rVB	211	79	0.01%	0.001%
29	5.954	1431	1435	1438	rVB2	230	162	0.03%	0.003%
30	6.083	1474	1475	1479	rBV	262	121	0.02%	0.002%
31	6.099	1479	1480	1481	rVB	138	27	0.00%	0.001%
32	6.282	1523	1537	1554	rBV2	195149	360790	55.86%	6.807%
33	6.385	1568	1569	1573	rBV2	223	118	0.02%	0.002%
34	6.433	1582	1584	1588	rVB	165	86	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040720\
 Data File : VU037603.D
 Acq On : 07 Apr 2020 12:33
 Operator : JC/MD
 Sample : L2173-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFS69

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

35	6.575	1614	1628	1643	rBV	112652	209579	32.45%	3.954%
36	6.661	1652	1655	1659	rBV	216	204	0.03%	0.004%
37	6.722	1660	1674	1693	rVB	155130	296539	45.91%	5.595%
38	6.790	1693	1695	1698	rVB	287	130	0.02%	0.002%
39	6.806	1698	1700	1701	rBV	284	95	0.01%	0.002%
40	6.922	1733	1736	1737	rBV	208	110	0.02%	0.002%
41	7.185	1816	1818	1820	rVB	157	41	0.01%	0.001%
42	7.356	1868	1871	1875	rVB	215	137	0.02%	0.003%
43	7.439	1895	1897	1900	rVB	155	43	0.01%	0.001%
44	7.591	1931	1944	1966	rVB2	98731	169780	26.29%	3.203%
45	7.668	1966	1968	1970	rBV	286	146	0.02%	0.003%
46	7.726	1984	1986	1988	rBV2	122	67	0.01%	0.001%
47	7.922	2033	2047	2065	rBV	315004	536667	83.09%	10.126%
48	8.028	2078	2080	2084	rBV	166	92	0.01%	0.002%
49	8.095	2099	2101	2106	rBV	241	149	0.02%	0.003%
50	8.140	2114	2115	2116	rBV	101	23	0.00%	0.000%
51	8.201	2123	2134	2148	rBV2	70349	115851	17.94%	2.186%
52	8.587	2251	2254	2256	rBV	155	102	0.02%	0.002%
53	8.655	2262	2275	2304	rBV	221418	387420	59.99%	7.310%
54	8.777	2311	2313	2317	rVB	159	76	0.01%	0.001%
55	8.809	2321	2323	2324	rBV	126	27	0.00%	0.001%
56	8.935	2356	2362	2364	rBV	305	236	0.04%	0.004%
57	9.131	2419	2423	2426	rBV	222	207	0.03%	0.004%
58	9.436	2505	2518	2533	rBV	276281	450094	69.69%	8.492%
59	9.787	2620	2627	2632	rBV	315	498	0.08%	0.009%
60	9.906	2662	2664	2675	rVB	296	302	0.05%	0.006%
61	10.105	2725	2726	2727	rBV	134	36	0.01%	0.001%
62	10.774	2921	2934	2949	rBV	208584	335413	51.93%	6.329%
63	11.108	3036	3038	3040	rBV	222	90	0.01%	0.002%
64	11.433	3137	3139	3142	rBV	164	106	0.02%	0.002%
65	11.754	3236	3239	3243	rBV	370	251	0.04%	0.005%
66	11.825	3249	3261	3274	rVB	278406	435338	67.40%	8.214%
67	11.996	3313	3314	3317	rBV	331	102	0.02%	0.002%
68	12.205	3367	3379	3396	rBV	302500	483265	74.83%	9.118%


Sum of corrected areas: 5299940

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040720\
Data File : VU037603.D
Acq On : 07 Apr 2020 12:33
Operator : JC/MD
Sample : L2173-02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFS69

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

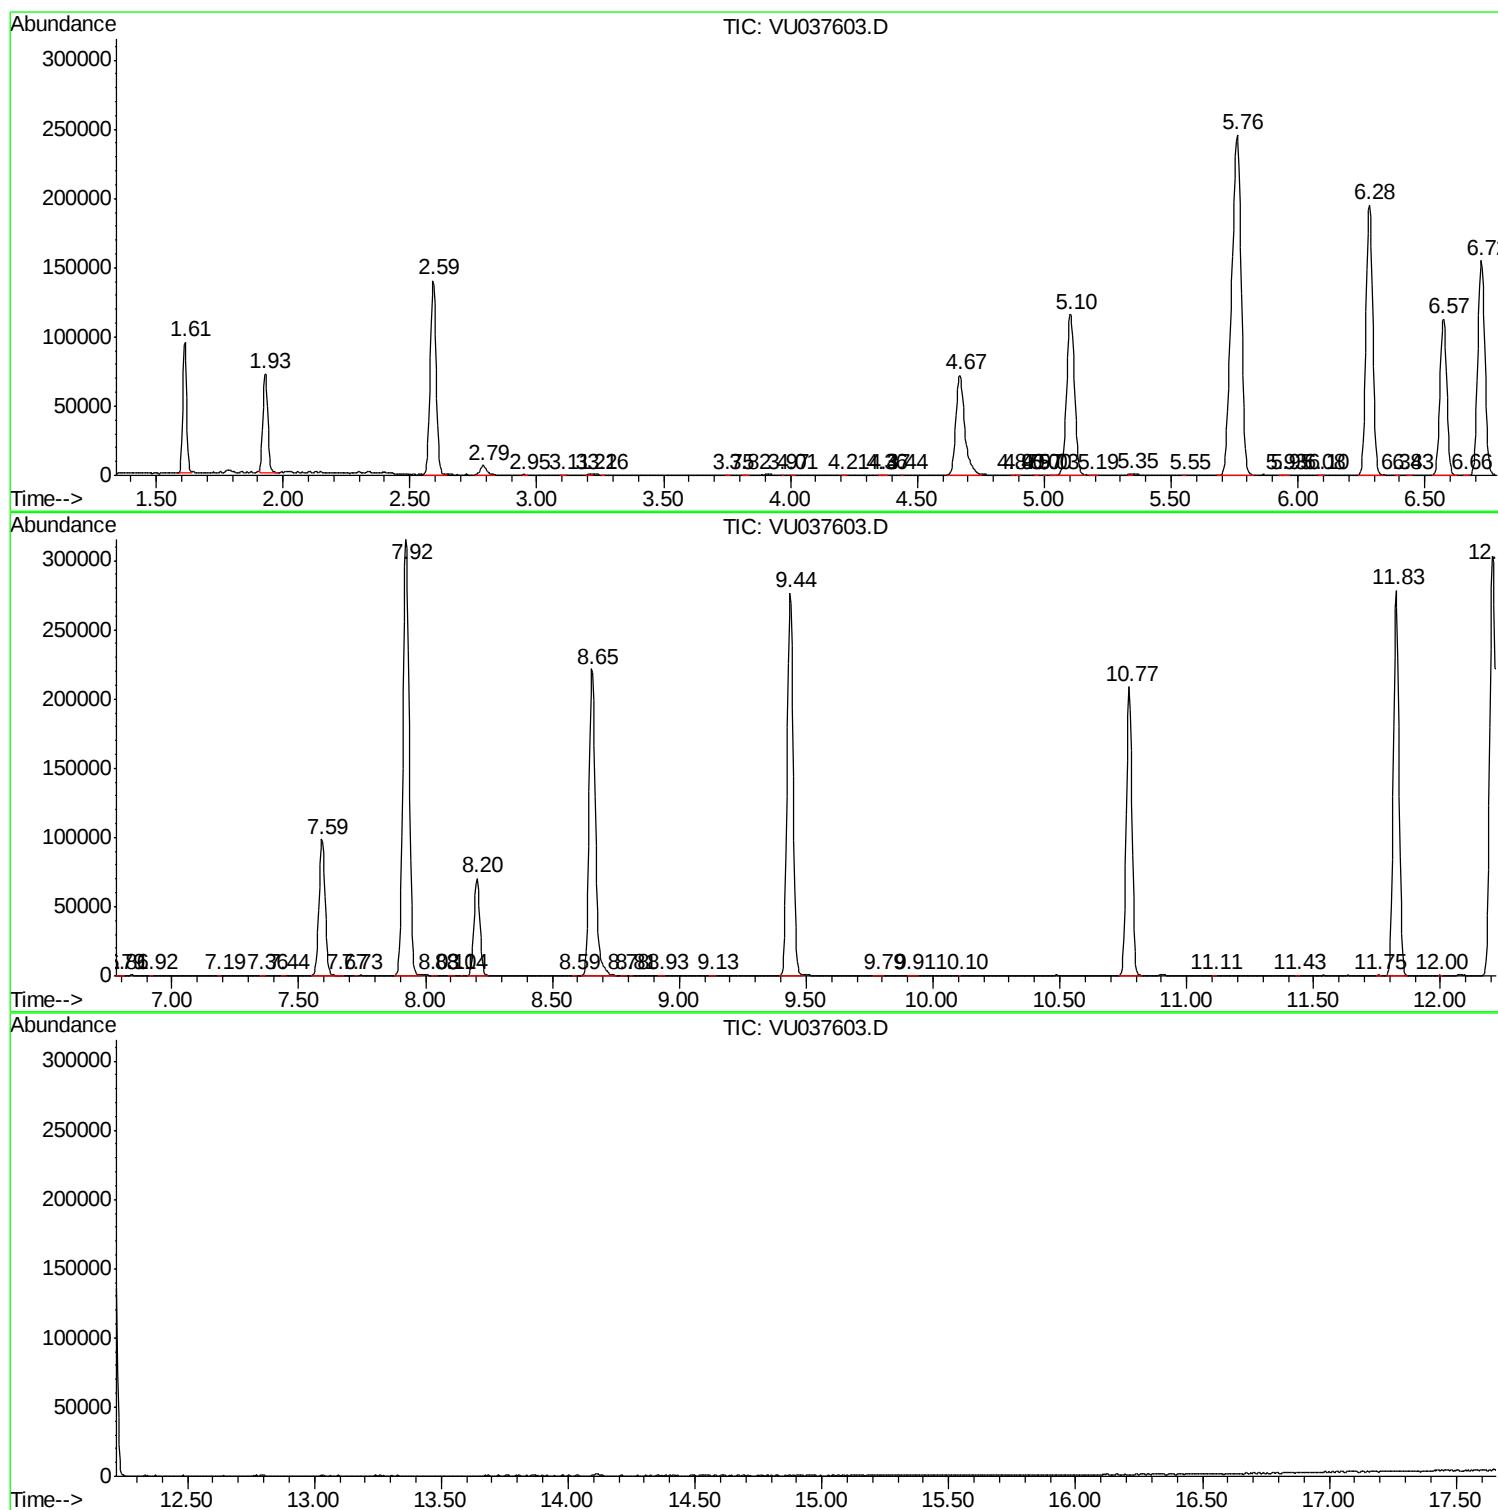

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040720\
Data File : VU037603.D
Acq On : 07 Apr 2020 12:33
Operator : JC/MD
Sample : L2173-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFS69

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040720\
Data File : VU037603.D
Acq On : 07 Apr 2020 12:33
Operator : JC/MD
Sample : L2173-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFS69

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc