


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040720\
 Data File : VU037597.D
 Acq On : 07 Apr 2020 08:59
 Operator : JC/MD
 Sample : BFB37
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB37

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis
 Last Update : Wed Apr 08 02:25:30 2020

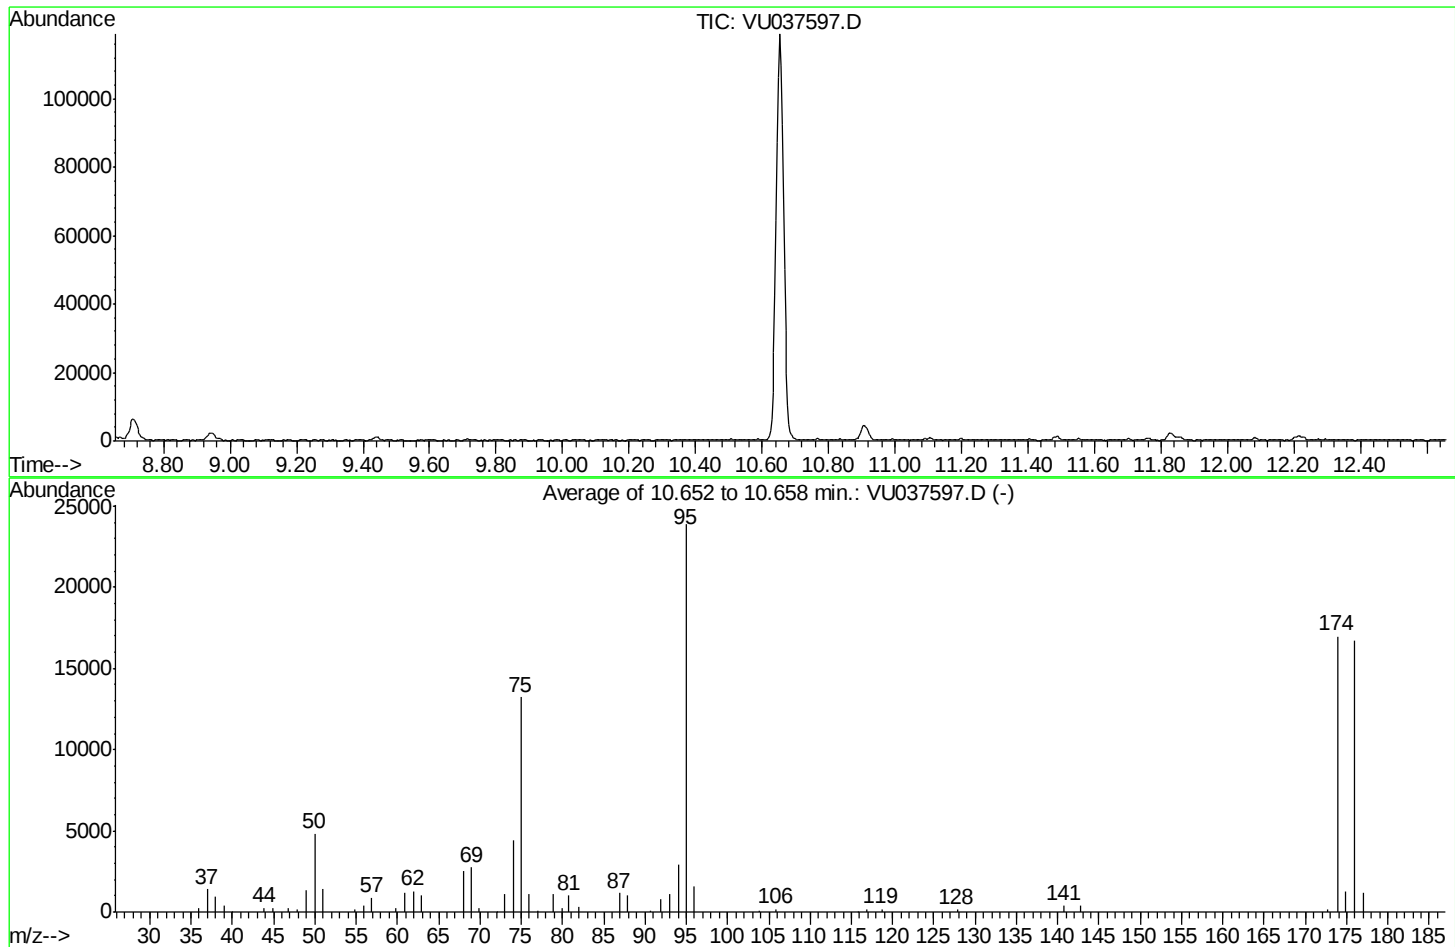

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	4831	PASS
75	95	30	80	55.3	13212	PASS
95	95	100	100	100.0	23882	PASS
96	95	5	9	6.7	1600	PASS
173	174	0.00	2	1.1	192	PASS
174	95	50	120	71.1	16979	PASS
175	174	5	9	7.2	1230	PASS
176	174	95	101	98.3	16695	PASS
177	176	5	9	7.0	1176	PASS

m/z	Abundance
35.90	390.0
37.00	1472.0
37.90	1095.0
39.00	415.0
43.90	420.0
44.90	205.0
46.80	226.0
47.90	131.0
48.90	1503.0
50.00	5079.0
51.00	1650.0
54.80	153.0
56.00	368.0
56.90	850.0
59.90	269.0
60.90	1175.0
61.90	1235.0
63.00	1057.0
67.90	2699.0
69.00	2949.0
69.90	239.0
72.00	107.0
72.90	1132.0
74.00	4690.0
75.00	13661.0
75.90	1138.0
77.00	147.0
78.80	1125.0
79.90	266.0
80.80	1004.0
81.90	340.0
86.90	1117.0
87.90	963.0
90.70	135.0
91.90	799.0
93.00	1179.0
94.00	2751.0
95.00	24128.0
96.00	1606.0
103.90	130.0
105.90	189.0
116.80	116.0
118.70	175.0
127.80	125.0
140.80	381.0
142.80	404.0
172.70	159.0
173.90	16992.0
174.90	1292.0
175.90	16808.0
177.00	1159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
35.90	420.0
37.00	1451.0
37.90	971.0
39.00	401.0
43.90	415.0
45.00	250.0
46.90	200.0
47.90	159.0
48.90	1404.0
50.00	5008.0
51.00	1424.0
54.90	154.0
55.90	387.0
56.90	914.0
59.90	257.0
61.00	1228.0
62.00	1326.0
62.90	1057.0
68.00	2578.0
69.00	2805.0
70.00	217.0
72.90	1100.0
74.00	4563.0
75.00	13612.0
75.90	1119.0
77.00	106.0
78.90	1073.0
79.90	262.0
80.80	1046.0
81.90	325.0
86.90	1228.0
87.90	1009.0
91.90	784.0
92.90	1155.0
94.00	3069.0
95.00	24544.0
96.00	1593.0
103.90	112.0
105.90	211.0
115.80	102.0
116.80	150.0
118.70	178.0
127.90	156.0
140.80	374.0
142.80	370.0
172.70	206.0
173.90	17656.0
174.90	1263.0
175.90	17296.0
176.90	1222.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
35.90	390.0
37.00	1295.0
37.90	855.0
39.00	405.0
39.90	120.0
43.90	387.0
45.00	259.0
46.80	266.0
47.90	174.0
48.90	1155.0
50.00	4406.0
51.00	1229.0
54.90	172.0
55.90	426.0
56.90	878.0
59.80	198.0
61.00	1165.0
62.00	1255.0
62.90	934.0
68.00	2394.0
69.00	2454.0
70.00	185.0
73.00	1109.0
74.00	4053.0
75.00	12364.0
75.90	1061.0
78.90	1065.0
79.90	256.0
80.80	997.0
81.90	268.0
86.90	1120.0
87.90	1001.0
91.90	725.0
92.90	1033.0
94.00	2934.0
95.00	22976.0
96.00	1602.0
105.90	193.0
116.80	164.0
118.70	154.0
127.90	159.0
140.80	326.0
142.80	303.0
172.70	213.0
173.90	16289.0
174.90	1137.0
175.90	15982.0
176.90	1149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

Scan 2884 (10.613 min): VU037597.D
BFB37

m/z	Abundance
35.80	176.0
44.00	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37