

m/z	Abundance
35.90	479.0
37.00	1911.0
38.00	1747.0
38.90	746.0
44.00	470.0
45.00	313.0
46.90	191.0
48.00	228.0
48.90	1539.0
50.00	6978.0
51.00	1978.0
55.90	602.0
57.00	1210.0
60.00	320.0
61.00	1833.0
62.00	1726.0
63.00	1233.0
64.00	160.0
65.00	154.0
66.70	104.0
68.00	3575.0
69.00	3636.0
69.90	329.0
72.00	191.0
72.90	1802.0
74.00	5973.0
75.00	16237.0
76.00	1235.0
76.80	145.0
78.80	1293.0
79.90	425.0
80.90	1517.0
81.80	373.0
86.90	1114.0
87.90	951.0
90.90	166.0
92.00	1034.0
93.00	1537.0
94.00	3853.0
95.00	28880.0
96.00	1817.0
103.70	156.0
105.70	123.0
115.80	153.0
116.90	260.0
117.70	110.0
118.90	194.0
127.90	115.0
129.70	130.0
140.80	465.0
142.80	416.0
171.90	264.0
173.90	25824.0
174.90	2174.0
175.90	25088.0
176.90	1536.0

Instrument :
MSVOA_U
ClientSampleId :
BFB631

m/z	Abundance
43.80	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB631

m/z	Abundance
35.90	454.0
37.00	2090.0
38.00	1894.0
39.00	760.0
40.00	116.0
44.00	418.0
44.90	340.0
47.10	230.0
47.90	255.0
48.90	1499.0
50.00	7219.0
51.00	1971.0
51.90	105.0
55.90	562.0
57.00	996.0
59.90	335.0
60.90	1814.0
62.00	1720.0
63.00	1291.0
63.90	142.0
65.00	118.0
68.00	3475.0
69.00	3802.0
70.00	366.0
71.90	158.0
72.90	1779.0
74.00	5553.0
75.00	16488.0
76.00	1379.0
76.90	180.0
77.70	105.0
78.90	1422.0
79.90	453.0
80.90	1594.0
81.80	321.0
86.90	1002.0
87.90	914.0
91.00	142.0
92.00	1174.0
93.00	1431.0
94.00	4064.0
95.00	29568.0
96.00	1899.0
103.80	170.0
104.80	106.0
105.80	140.0
115.80	137.0
116.90	237.0
117.70	122.0
118.90	159.0
127.90	118.0
129.80	144.0
140.80	453.0
142.80	502.0
171.90	199.0
173.90	25296.0
174.90	2218.0
175.90	24528.0
176.90	1636.0

Instrument :
MSVOA_U
ClientSampleId :
BFB631

m/z	Abundance
35.90	494.0
37.00	2111.0
38.00	1948.0
38.90	798.0
44.00	453.0
44.90	350.0
46.90	199.0
48.00	253.0
48.90	1594.0
50.00	7456.0
51.00	2110.0
55.00	101.0
56.00	607.0
57.00	1178.0
59.90	313.0
61.00	1864.0
62.00	1825.0
63.00	1302.0
64.00	150.0
65.00	142.0
68.00	3704.0
69.00	3903.0
69.90	376.0
71.90	176.0
72.90	1914.0
74.00	5934.0
75.00	17152.0
76.00	1333.0
76.90	175.0
78.80	1411.0
79.90	471.0
80.90	1707.0
81.80	352.0
86.90	1052.0
87.90	973.0
90.90	168.0
92.00	1190.0
93.00	1591.0
94.00	4150.0
95.00	30544.0
96.00	1953.0
103.70	171.0
104.70	125.0
105.70	124.0
115.80	144.0
116.90	262.0
117.70	126.0
118.90	184.0
127.90	140.0
129.80	151.0
140.80	488.0
142.80	490.0
171.90	248.0
173.90	26584.0
174.90	2346.0
175.90	26048.0
176.90	1649.0



Instrument :
MSVOA_U
ClientSampleId :
BFB631

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040721\
 Data File : VU042970.D
 Acq On : 07 Apr 2021 08:59
 Operator : SY/MD
 Sample : BFB63
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB631

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM040721WMA.M
 Title : VOC Analysis
 Last Update : Thu Apr 08 08:47:10 2021

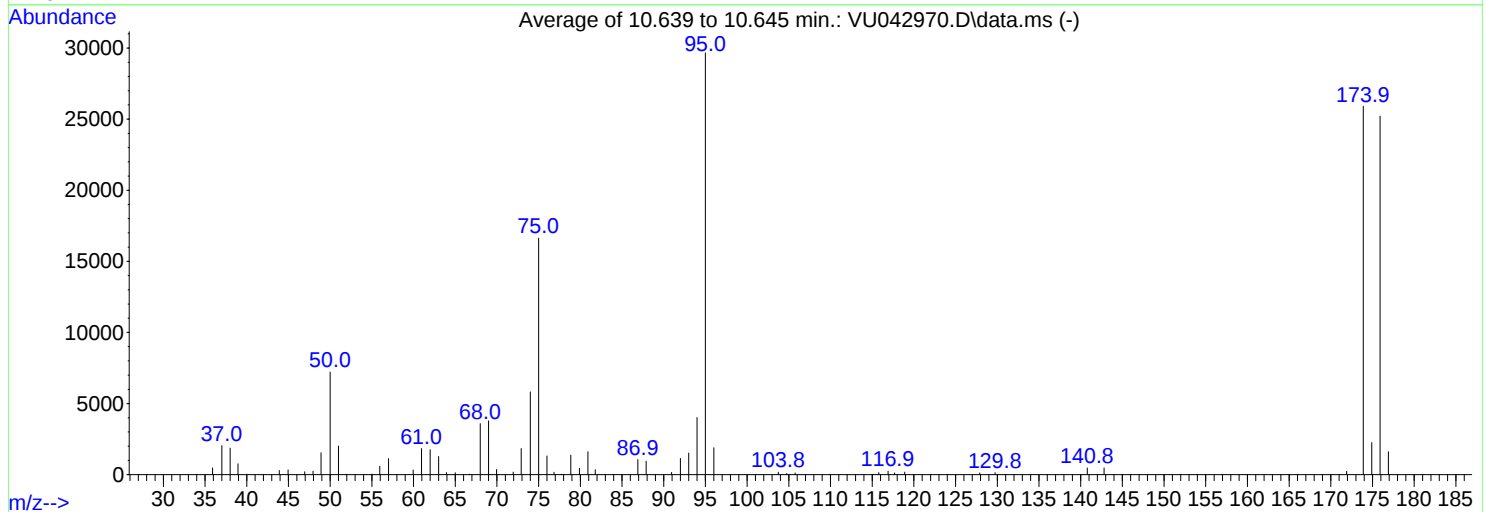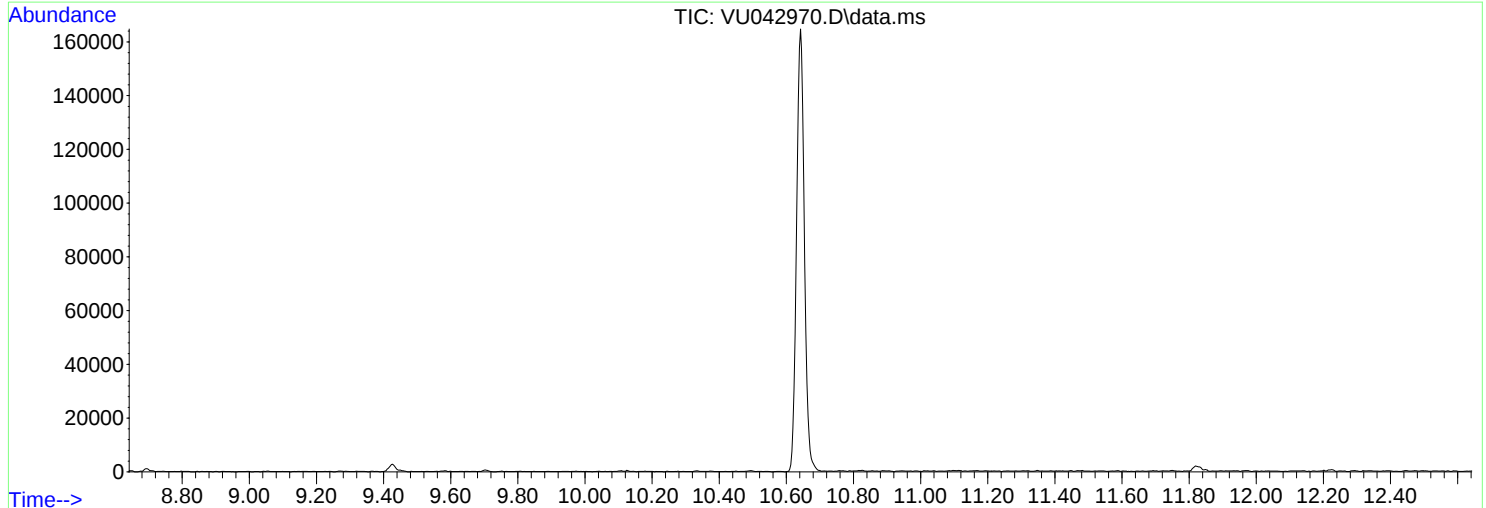

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.3	7218	PASS
75	95	30	80	56.0	16626	PASS
95	95	100	100	100.0	29664	PASS
96	95	5	9	6.4	1890	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.3	25901	PASS
175	174	5	9	8.7	2246	PASS
176	174	95	101	97.4	25221	PASS
177	176	5	9	6.4	1607	PASS