

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
 Data File : VU053599.D
 Acq On : 07 Apr 2023 17:05
 Operator : JC/MD
 Sample : 02251-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CMD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	119784	139352	16.26%	2.053%
2	1.909	169	177	199	rVB	96262	134385	15.68%	1.980%
3	2.565	368	381	394	rBV	186440	302416	35.28%	4.455%
4	2.954	498	502	507	rVB	378	271	0.03%	0.004%
5	3.038	523	528	531	rBV4	1259	1455	0.17%	0.021%
6	3.337	618	621	624	rBV2	264	170	0.02%	0.003%
7	3.408	640	643	648	rBV2	261	290	0.03%	0.004%
8	3.787	758	761	765	rVB2	311	231	0.03%	0.003%
9	3.826	770	773	776	rVB2	279	199	0.02%	0.003%
10	3.919	800	802	806	rBB2	221	138	0.02%	0.002%
11	4.070	846	849	854	rVB2	262	246	0.03%	0.004%
12	4.141	869	871	876	rVB	255	156	0.02%	0.002%
13	4.215	891	894	898	rVV	341	233	0.03%	0.003%
14	4.433	958	962	965	rBV2	278	249	0.03%	0.004%
15	4.571	1003	1005	1007	rBV2	224	148	0.02%	0.002%
16	4.613	1007	1018	1045	rBV2	71512	168729	19.69%	2.485%
17	4.825	1078	1084	1086	rBV3	488	485	0.06%	0.007%
18	4.896	1103	1106	1112	rBV3	341	372	0.04%	0.005%
19	5.057	1138	1156	1179	rBV	161664	354798	41.39%	5.226%
20	5.272	1220	1223	1225	rBV	221	157	0.02%	0.002%
21	5.295	1228	1230	1234	rBV2	383	189	0.02%	0.003%
22	5.440	1272	1275	1279	rBV	245	165	0.02%	0.002%
23	5.459	1279	1281	1284	rBV2	187	139	0.02%	0.002%
24	5.581	1311	1319	1322	rBV	270	270	0.03%	0.004%
25	5.613	1325	1329	1332	rBV	215	215	0.03%	0.003%
26	5.719	1341	1362	1382	rBV2	312496	857134	100.00%	12.626%
27	5.970	1438	1440	1443	rVB2	273	169	0.02%	0.002%
28	5.986	1443	1445	1450	rBV	208	194	0.02%	0.003%
29	6.096	1472	1479	1483	rBV2	272	279	0.03%	0.004%
30	6.118	1483	1486	1489	rBV	223	189	0.02%	0.003%
31	6.192	1505	1509	1512	rBV2	229	219	0.03%	0.003%
32	6.243	1512	1525	1549	rBV	280436	536194	62.56%	7.898%
33	6.526	1604	1613	1623	rVB7	4547	8506	0.99%	0.125%
34	6.565	1623	1625	1629	rVB2	219	167	0.02%	0.002%
35	6.636	1644	1647	1648	rBV	358	174	0.02%	0.003%
36	6.684	1648	1662	1682	rBV	197480	381585	44.52%	5.621%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
 Data File : VU053599.D
 Acq On : 07 Apr 2023 17:05
 Operator : JC/MD
 Sample : 02251-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CMD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.880	1720	1723	1726	rBV	199	139	0.02%	0.002%
38	6.977	1749	1753	1757	rVB	380	292	0.03%	0.004%
39	7.002	1757	1761	1763	rBV	257	212	0.02%	0.003%
40	7.115	1792	1796	1799	rBV2	352	306	0.04%	0.005%
41	7.147	1802	1806	1809	rBV	195	215	0.03%	0.003%
42	7.185	1813	1818	1820	rBV3	797	804	0.09%	0.012%
43	7.311	1854	1857	1861	rBV2	231	170	0.02%	0.003%
44	7.333	1861	1864	1868	rBV	179	160	0.02%	0.002%
45	7.501	1914	1916	1921	rBV	240	151	0.02%	0.002%
46	7.562	1923	1935	1955	rVV	112807	195923	22.86%	2.886%
47	7.751	1992	1994	2000	rVB2	270	238	0.03%	0.004%
48	7.803	2007	2010	2014	rVB	222	179	0.02%	0.003%
49	7.825	2014	2017	2020	rBV	211	181	0.02%	0.003%
50	7.893	2025	2038	2070	rBV	409659	718020	83.77%	10.576%
51	8.054	2086	2088	2092	rBV	336	151	0.02%	0.002%
52	8.176	2114	2126	2146	rBV2	80108	135803	15.84%	2.000%
53	8.375	2185	2188	2191	rVB	257	166	0.02%	0.002%
54	8.510	2228	2230	2235	rVB	223	161	0.02%	0.002%
55	8.549	2236	2242	2246	rBV4	545	608	0.07%	0.009%
56	8.626	2255	2266	2304	rBV	212534	388873	45.37%	5.728%
57	8.784	2312	2315	2319	rVB4	516	358	0.04%	0.005%
58	8.832	2327	2330	2333	rBV	284	193	0.02%	0.003%
59	8.870	2338	2342	2344	rBV2	172	148	0.02%	0.002%
60	8.941	2360	2364	2368	rVB2	291	273	0.03%	0.004%
61	8.970	2368	2373	2378	rBV	123	148	0.02%	0.002%
62	8.996	2378	2381	2383	rBV	357	266	0.03%	0.004%
63	9.173	2431	2436	2442	rBV2	266	288	0.03%	0.004%
64	9.227	2450	2453	2457	rBV2	290	271	0.03%	0.004%
65	9.288	2469	2472	2476	rBV2	222	139	0.02%	0.002%
66	9.311	2476	2479	2481	rBV	313	249	0.03%	0.004%
67	9.414	2498	2511	2540	rBV	385815	647370	75.53%	9.536%
68	9.693	2593	2598	2603	rBV2	521	518	0.06%	0.008%
69	9.793	2627	2629	2633	rVB2	260	177	0.02%	0.003%
70	9.816	2633	2636	2640	rBV2	313	233	0.03%	0.003%
71	9.848	2640	2646	2650	rBV2	309	400	0.05%	0.006%
72	9.935	2670	2673	2676	rBV2	186	132	0.02%	0.002%
73	9.954	2676	2679	2682	rVB2	239	175	0.02%	0.003%
74	9.980	2683	2687	2690	rVB2	325	250	0.03%	0.004%
75	10.005	2690	2695	2697	rBV	259	213	0.02%	0.003%
76	10.115	2725	2729	2734	rBV4	814	708	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
 Data File : VU053599.D
 Acq On : 07 Apr 2023 17:05
 Operator : JC/MD
 Sample : 02251-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.176	2746	2748	2754	rVB2	242	214	0.02%	0.003%
78	10.288	2781	2783	2785	rBV	271	162	0.02%	0.002%
79	10.484	2838	2844	2848	rVB2	304	406	0.05%	0.006%
80	10.751	2914	2927	2948	rBV	275708	446997	52.15%	6.584%
81	10.893	2959	2971	2976	rBV4	1217	1741	0.20%	0.026%
82	10.989	2998	3001	3004	rBV2	257	179	0.02%	0.003%
83	11.082	3027	3030	3033	rVV3	480	318	0.04%	0.005%
84	11.562	3176	3179	3181	rBV2	218	128	0.01%	0.002%
85	11.745	3233	3236	3239	rBV2	809	527	0.06%	0.008%
86	11.809	3243	3256	3278	rBV	418398	668643	78.01%	9.849%
87	11.941	3294	3297	3301	rBV3	537	465	0.05%	0.007%
88	12.037	3325	3327	3331	rVB2	350	205	0.02%	0.003%
89	12.086	3336	3342	3343	rBV3	668	635	0.07%	0.009%
90	12.189	3362	3374	3393	rBV	416277	675556	78.82%	9.951%
91	12.446	3452	3454	3456	rBV	282	147	0.02%	0.002%
92	12.655	3516	3519	3521	rBV	329	238	0.03%	0.004%
93	12.729	3539	3542	3545	rBV2	326	230	0.03%	0.003%
94	12.889	3588	3592	3599	rBV6	1202	1295	0.15%	0.019%
95	13.150	3670	3673	3675	rBV	235	163	0.02%	0.002%
96	13.452	3764	3767	3768	rBV2	344	214	0.02%	0.003%
97	13.500	3779	3782	3783	rBV	284	163	0.02%	0.002%
98	13.581	3804	3807	3811	rVB	546	289	0.03%	0.004%
99	13.787	3869	3871	3877	rBV2	359	361	0.04%	0.005%
100	13.841	3881	3888	3897	rVV5	2615	4026	0.47%	0.059%



Sum of corrected areas: 6788831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
Data File : VU053599.D
Acq On : 07 Apr 2023 17:05
Operator : JC/MD
Sample : 02251-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

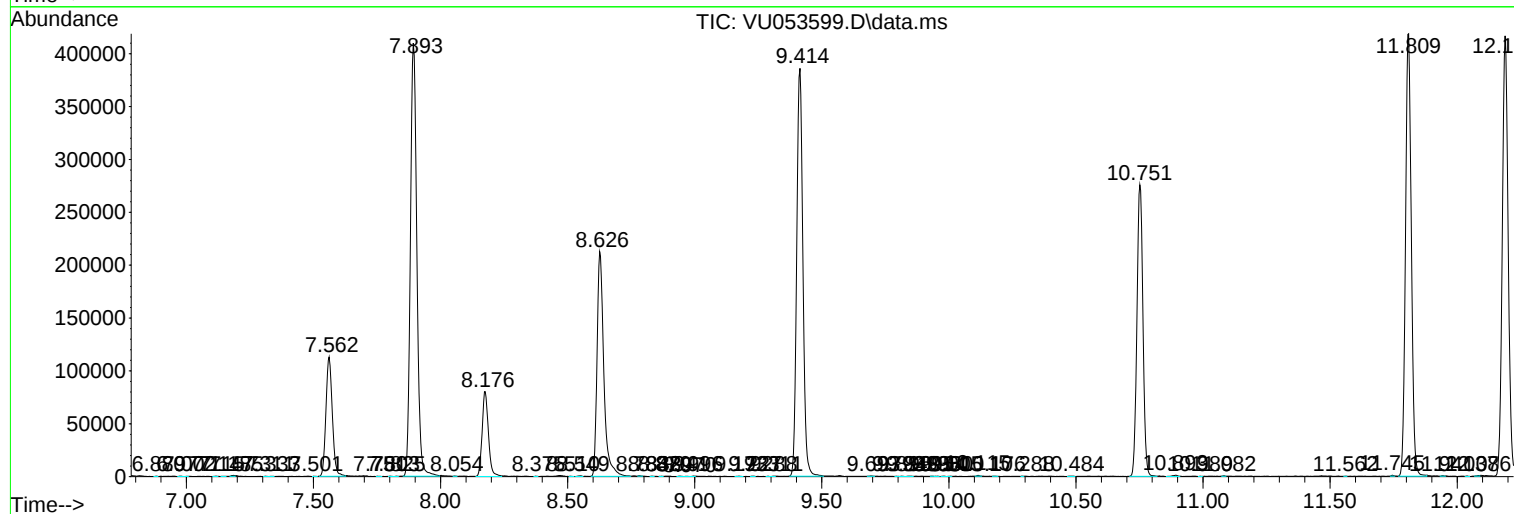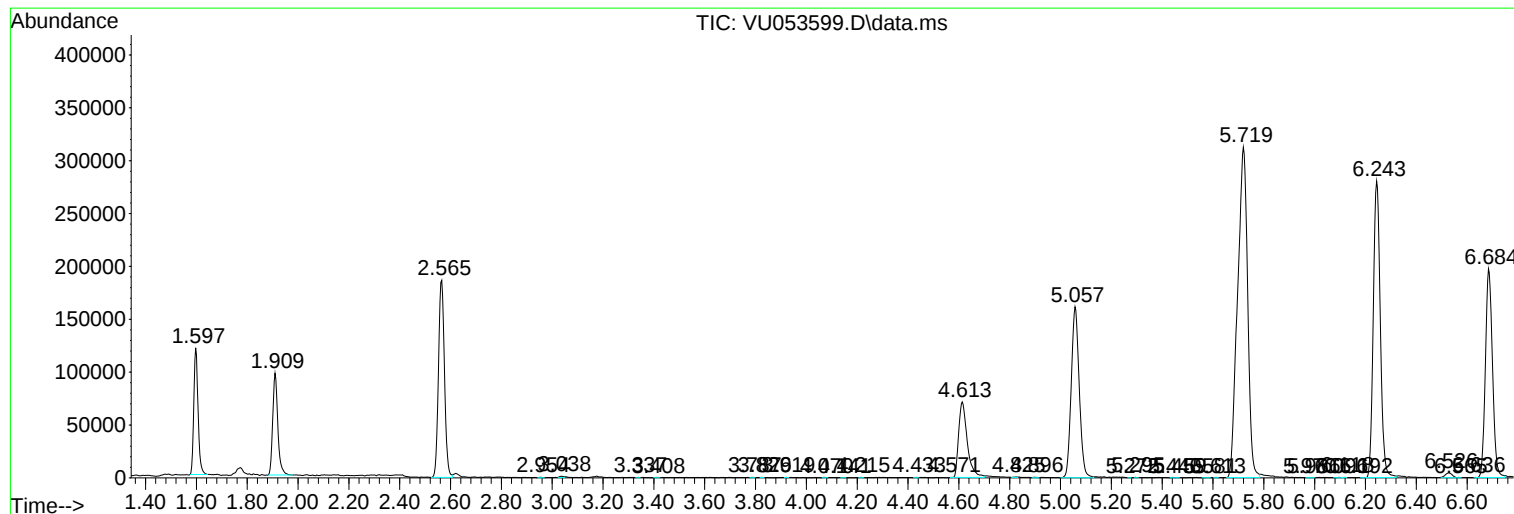

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
Data File : VU053599.D
Acq On : 07 Apr 2023 17:05
Operator : JC/MD
Sample : 02251-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
Data File : VU053599.D
Acq On : 07 Apr 2023 17:05
Operator : JC/MD
Sample : 02251-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------