

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
 Data File : VU053601.D
 Acq On : 07 Apr 2023 17:52
 Operator : JC/MD
 Sample : 02251-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	123464	143158	17.17%	2.173%
2	1.909	170	177	194	rVB	96402	134405	16.12%	2.041%
3	2.565	369	381	398	rBV	181406	297692	35.69%	4.520%
4	2.719	425	429	434	rVB3	683	687	0.08%	0.010%
5	2.761	438	442	444	rBV2	314	230	0.03%	0.003%
6	2.858	470	472	475	rBV	206	140	0.02%	0.002%
7	2.935	494	496	500	rBV2	267	166	0.02%	0.003%
8	3.176	563	571	576	rBV2	788	1336	0.16%	0.020%
9	3.372	628	632	636	rBV	262	193	0.02%	0.003%
10	3.501	669	672	674	rVB	240	144	0.02%	0.002%
11	3.848	765	780	797	rBV2	14558	33360	4.00%	0.506%
12	3.996	821	826	833	rBV	217	276	0.03%	0.004%
13	4.173	877	881	884	rBV	186	161	0.02%	0.002%
14	4.205	889	891	894	rVB2	230	129	0.02%	0.002%
15	4.314	921	925	932	rBV2	282	292	0.04%	0.004%
16	4.459	968	970	975	rVB	264	177	0.02%	0.003%
17	4.510	980	986	992	rBV2	303	423	0.05%	0.006%
18	4.613	1006	1018	1041	rBV	66870	158964	19.06%	2.413%
19	4.912	1105	1111	1117	rVB2	397	542	0.06%	0.008%
20	5.057	1140	1156	1178	rBV	156772	346707	41.57%	5.264%
21	5.263	1217	1220	1222	rBV	317	202	0.02%	0.003%
22	5.327	1237	1240	1245	rVB	389	290	0.03%	0.004%
23	5.420	1264	1269	1270	rBV	124	118	0.01%	0.002%
24	5.510	1291	1297	1300	rBV2	259	249	0.03%	0.004%
25	5.719	1341	1362	1382	rBV2	302579	834011	100.00%	12.662%
26	5.938	1428	1430	1437	rVB2	423	377	0.05%	0.006%
27	6.034	1456	1460	1461	rBV2	227	158	0.02%	0.002%
28	6.118	1484	1486	1491	rVB2	334	259	0.03%	0.004%
29	6.163	1497	1500	1503	rBV	276	178	0.02%	0.003%
30	6.243	1508	1525	1547	rBV	264007	506342	60.71%	7.687%
31	6.388	1566	1570	1572	rBV2	449	367	0.04%	0.006%
32	6.481	1596	1599	1601	rBV2	187	133	0.02%	0.002%
33	6.520	1607	1611	1621	rVB5	1259	1919	0.23%	0.029%
34	6.687	1649	1663	1685	rBV	192690	375183	44.99%	5.696%
35	6.848	1709	1713	1716	rBV2	314	280	0.03%	0.004%
36	6.864	1716	1718	1721	rVB	247	125	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
 Data File : VU053601.D
 Acq On : 07 Apr 2023 17:52
 Operator : JC/MD
 Sample : 02251-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.999	1758	1760	1763	rVB	275	174	0.02%	0.003%
38	7.021	1763	1767	1768	rBV	198	119	0.01%	0.002%
39	7.118	1793	1797	1800	rVB2	216	179	0.02%	0.003%
40	7.137	1800	1803	1807	rBV	149	126	0.02%	0.002%
41	7.176	1810	1815	1816	rBV	762	508	0.06%	0.008%
42	7.497	1911	1915	1922	rVB2	304	363	0.04%	0.006%
43	7.562	1922	1935	1955	rBV	108717	192968	23.14%	2.930%
44	7.722	1982	1985	1988	rVB2	385	220	0.03%	0.003%
45	7.783	1999	2004	2005	rBV	255	190	0.02%	0.003%
46	7.793	2005	2007	2014	rVB2	447	302	0.04%	0.005%
47	7.828	2014	2018	2019	rBV	176	114	0.01%	0.002%
48	7.893	2025	2038	2068	rBV	393012	689710	82.70%	10.471%
49	8.127	2108	2111	2113	rBV2	232	132	0.02%	0.002%
50	8.176	2115	2126	2142	rBV	77457	128871	15.45%	1.956%
51	8.343	2175	2178	2181	rBV	171	136	0.02%	0.002%
52	8.465	2207	2216	2220	rBV2	1032	1393	0.17%	0.021%
53	8.555	2239	2244	2246	rBV2	394	327	0.04%	0.005%
54	8.626	2255	2266	2292	rBV2	191012	364584	43.71%	5.535%
55	8.822	2325	2327	2331	rVB2	204	140	0.02%	0.002%
56	8.848	2331	2335	2337	rBV	333	232	0.03%	0.004%
57	8.890	2345	2348	2353	rVB2	169	114	0.01%	0.002%
58	8.992	2378	2380	2383	rBV2	212	159	0.02%	0.002%
59	9.012	2383	2386	2389	rVV	187	131	0.02%	0.002%
60	9.031	2390	2392	2395	rVB2	187	112	0.01%	0.002%
61	9.166	2431	2434	2438	rVB	255	153	0.02%	0.002%
62	9.275	2463	2468	2470	rBV	175	167	0.02%	0.003%
63	9.362	2491	2495	2498	rBV2	258	236	0.03%	0.004%
64	9.414	2498	2511	2532	rBV	368940	616212	73.89%	9.355%
65	9.632	2574	2579	2580	rBV2	175	146	0.02%	0.002%
66	9.697	2596	2599	2602	rVB3	446	274	0.03%	0.004%
67	9.819	2633	2637	2641	rBV	293	295	0.04%	0.004%
68	9.841	2641	2644	2648	rBV2	226	203	0.02%	0.003%
69	9.973	2682	2685	2687	rBV	230	119	0.01%	0.002%
70	10.044	2705	2707	2710	rBV	226	124	0.01%	0.002%
71	10.105	2719	2726	2728	rBV3	704	803	0.10%	0.012%
72	10.311	2788	2790	2793	rVB2	312	176	0.02%	0.003%
73	10.327	2793	2795	2798	rVB	295	138	0.02%	0.002%
74	10.388	2811	2814	2815	rBV2	245	131	0.02%	0.002%
75	10.484	2838	2844	2847	rBV2	342	387	0.05%	0.006%
76	10.565	2866	2869	2874	rBV2	392	335	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
 Data File : VU053601.D
 Acq On : 07 Apr 2023 17:52
 Operator : JC/MD
 Sample : 02251-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMCO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.751	2912	2927	2945	rBV	279107	444180	53.26%	6.743%
78	10.925	2977	2981	2984	rBV	230	143	0.02%	0.002%
79	10.944	2984	2987	2990	rVV	286	203	0.02%	0.003%
80	11.092	3026	3033	3036	rBV2	342	376	0.05%	0.006%
81	11.115	3036	3040	3044	rBV	230	189	0.02%	0.003%
82	11.217	3069	3072	3073	rBV	297	116	0.01%	0.002%
83	11.352	3110	3114	3115	rBV	265	180	0.02%	0.003%
84	11.529	3164	3169	3173	rBV2	319	371	0.04%	0.006%
85	11.668	3210	3212	3216	rBV2	213	130	0.02%	0.002%
86	11.722	3226	3229	3231	rBV	254	150	0.02%	0.002%
87	11.742	3231	3235	3236	rBV2	576	459	0.06%	0.007%
88	11.809	3243	3256	3277	rBV	390166	632755	75.87%	9.606%
89	12.063	3331	3335	3336	rBV	299	201	0.02%	0.003%
90	12.089	3336	3343	3346	rBV4	1163	1365	0.16%	0.021%
91	12.188	3362	3374	3392	rBV	408708	662254	79.41%	10.054%
92	12.542	3482	3484	3489	rBV2	268	155	0.02%	0.002%
93	12.950	3608	3611	3614	rBV	477	274	0.03%	0.004%
94	13.031	3634	3636	3639	rBV2	399	207	0.02%	0.003%
95	13.311	3719	3723	3727	rVB	347	279	0.03%	0.004%
96	13.356	3736	3737	3740	rVB	381	168	0.02%	0.003%
97	13.629	3820	3822	3823	rBV	434	184	0.02%	0.003%
98	13.693	3838	3842	3843	rBV2	374	272	0.03%	0.004%
99	13.809	3876	3878	3880	rVB	324	133	0.02%	0.002%
100	13.838	3880	3887	3888	rBV2	1848	1496	0.18%	0.023%




Sum of corrected areas: 6586816

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
Data File : VU053601.D
Acq On : 07 Apr 2023 17:52
Operator : JC/MD
Sample : 02251-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

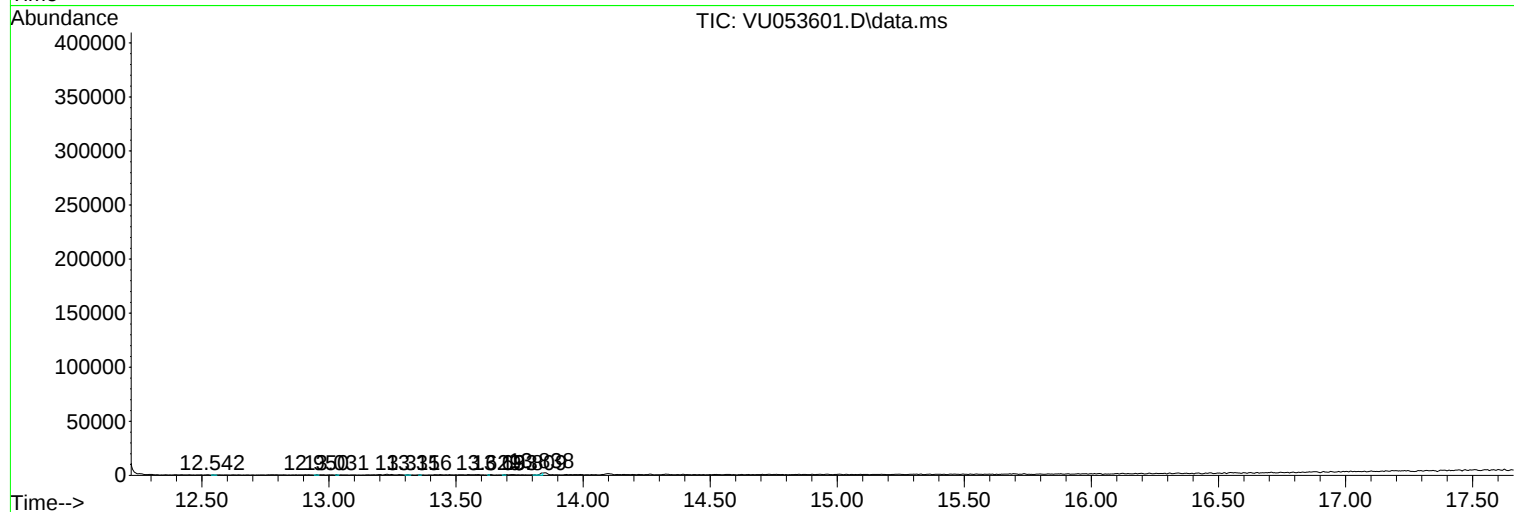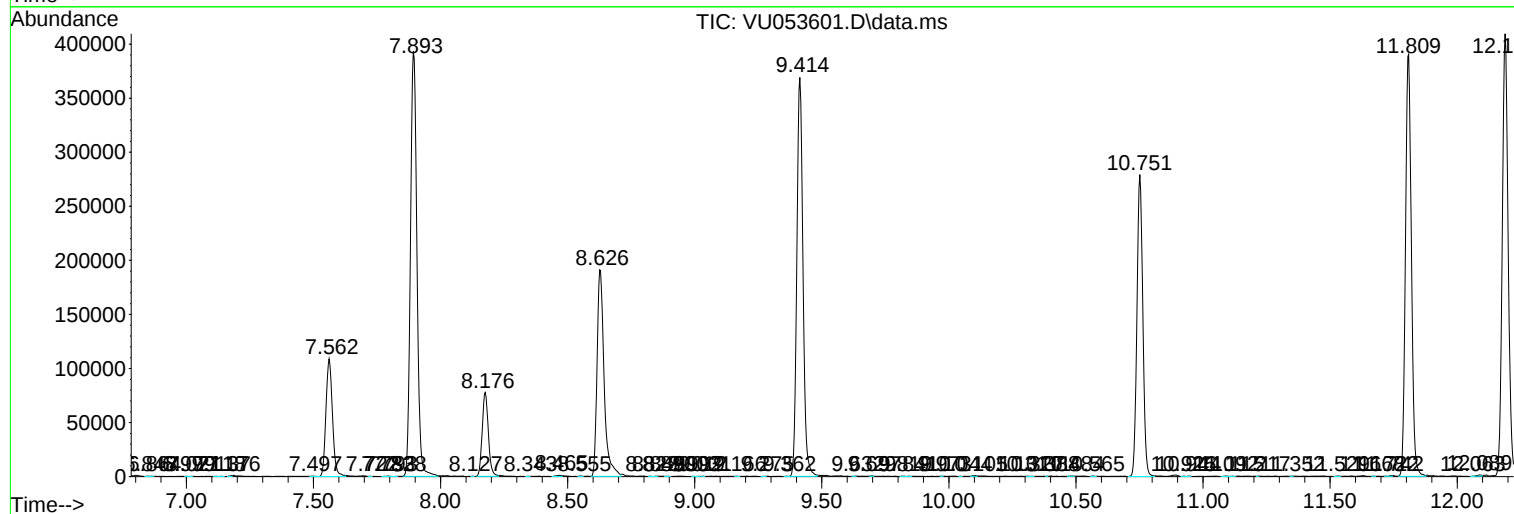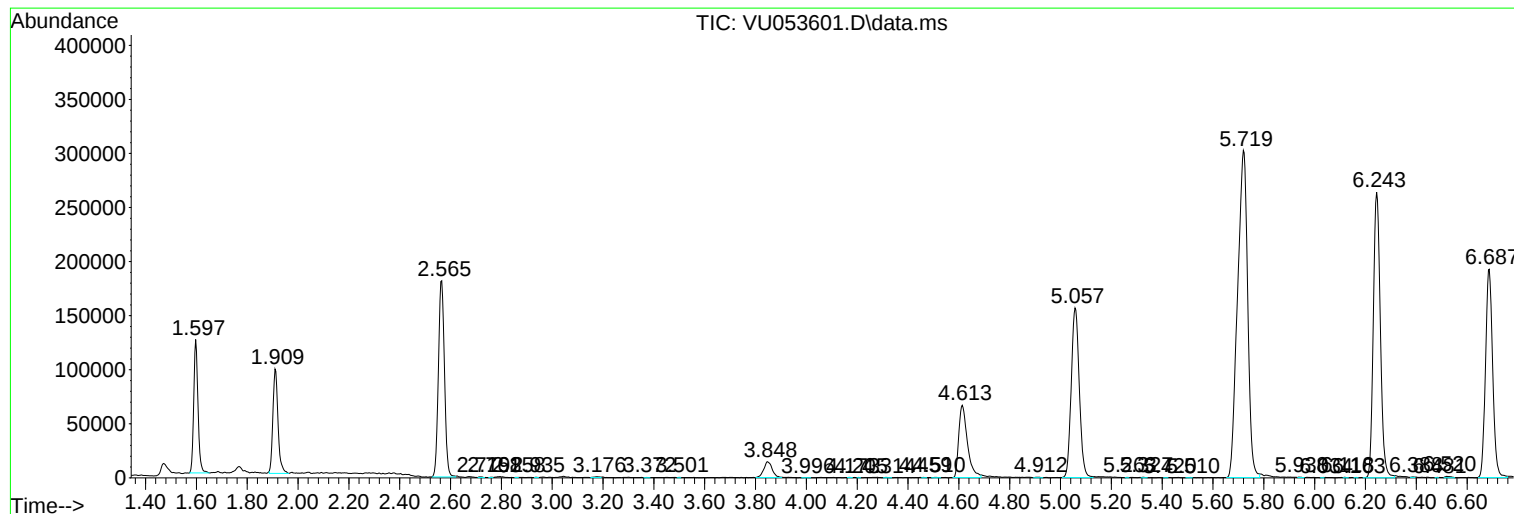

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
Data File : VU053601.D
Acq On : 07 Apr 2023 17:52
Operator : JC/MD
Sample : 02251-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
Data File : VU053601.D
Acq On : 07 Apr 2023 17:52
Operator : JC/MD
Sample : 02251-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------