
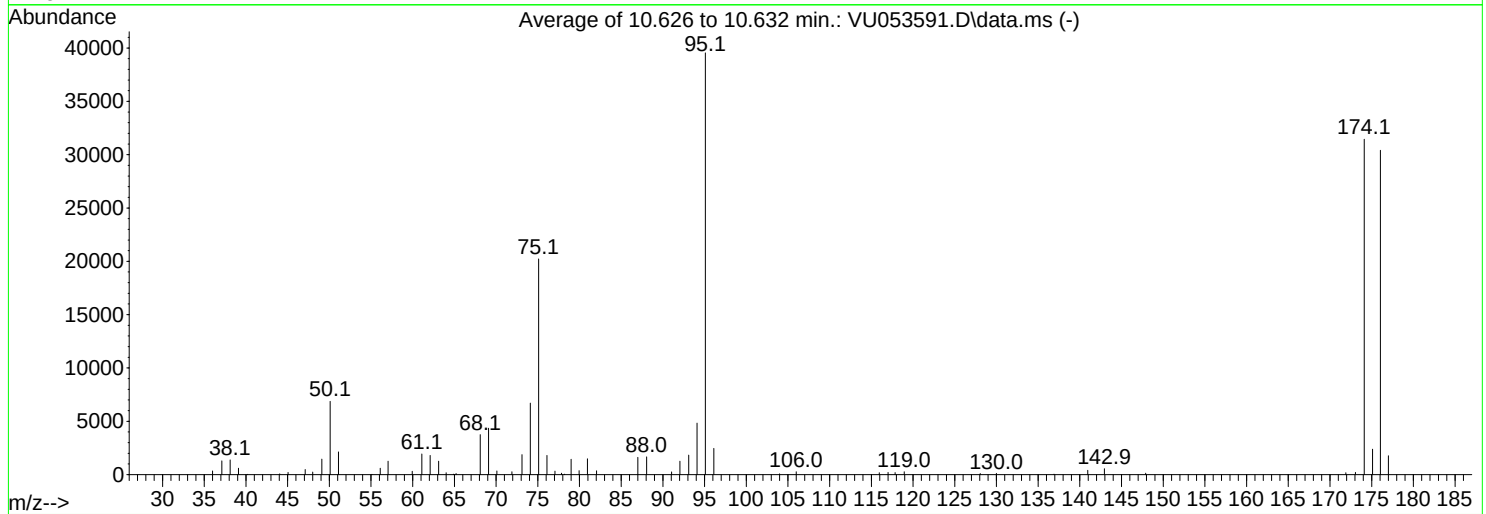


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040723\
 Data File : VU053591.D
 Acq On : 07 Apr 2023 09:40
 Operator : JC/MD
 Sample : BFB176
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB176

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 11 02:19:45 2023

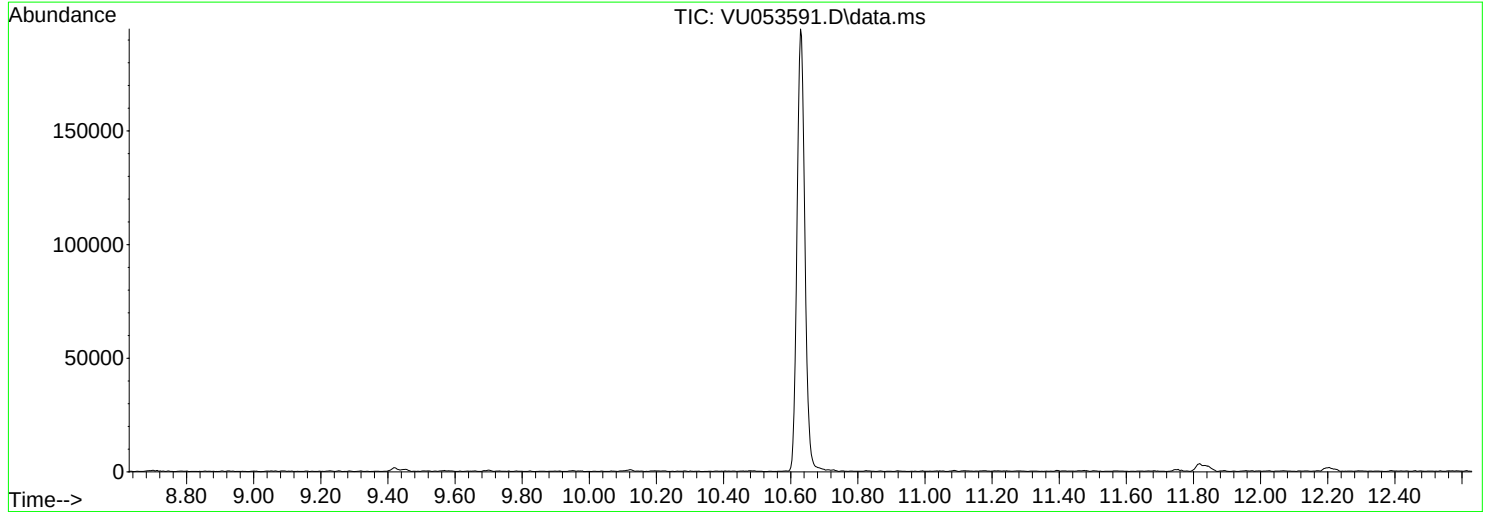

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	6879	PASS
75	95	30	80	51.1	20219	PASS
95	95	100	100	100.0	39547	PASS
96	95	5	9	6.2	2467	PASS
173	174	0.00	2	0.7	210	PASS
174	95	50	120	79.5	31440	PASS
175	174	5	9	7.6	2393	PASS
176	174	95	101	96.7	30413	PASS
177	176	5	9	5.8	1772	PASS

m/z	Abundance
44.10	365.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176

m/z	Abundance
36.00	377.0
37.10	1292.0
38.10	1242.0
39.10	584.0
40.20	112.0
44.00	522.0
45.00	201.0
47.10	425.0
48.00	245.0
49.10	1422.0
50.10	6608.0
51.10	2200.0
55.10	102.0
56.10	559.0
57.00	1102.0
60.00	350.0
61.10	1857.0
62.10	1695.0
63.10	1158.0
64.00	198.0
65.20	159.0
68.10	3526.0
69.10	4381.0
70.10	314.0
71.90	268.0
73.10	1673.0
74.10	6361.0
75.10	19408.0
76.10	1775.0
77.00	307.0
77.80	127.0
79.00	1324.0
80.10	371.0
81.00	1386.0
82.10	339.0
87.00	1543.0
88.10	1690.0
91.10	198.0
92.10	1315.0
93.10	1696.0
94.10	4872.0
95.10	38512.0
96.10	2448.0
106.00	244.0
116.00	149.0
117.00	233.0
117.80	149.0
118.90	250.0
130.10	124.0
136.90	115.0
141.00	424.0
142.90	538.0
147.80	118.0
171.90	199.0
173.00	218.0
174.10	29856.0
175.10	2370.0
176.10	27816.0
177.00	1593.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176

m/z	Abundance
36.00	360.0
37.10	1328.0
38.10	1431.0
39.10	645.0
44.10	436.0
45.00	215.0
47.10	509.0
48.00	248.0
49.10	1489.0
50.10	7040.0
51.10	2171.0
56.10	616.0
57.10	1315.0
59.90	311.0
61.10	1999.0
62.10	1871.0
63.10	1281.0
64.00	174.0
65.20	153.0
68.10	3916.0
69.10	4486.0
70.10	353.0
71.90	289.0
73.10	1974.0
74.10	6955.0
75.10	20880.0
76.10	1886.0
77.10	366.0
77.80	148.0
79.00	1452.0
79.90	383.0
81.00	1538.0
82.10	376.0
87.00	1688.0
88.00	1709.0
91.10	283.0
92.10	1299.0
93.10	1868.0
94.10	5011.0
95.10	40792.0
96.10	2505.0
104.00	105.0
106.00	304.0
115.90	187.0
117.00	208.0
117.90	200.0
118.90	271.0
128.00	141.0
130.00	127.0
140.90	426.0
143.00	570.0
147.90	152.0
171.90	176.0
173.10	217.0
174.10	32288.0
175.10	2486.0
176.00	31432.0
177.00	1793.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176

m/z	Abundance
36.00	295.0
37.10	1246.0
38.10	1476.0
39.10	586.0
44.10	375.0
45.10	227.0
47.10	492.0
48.00	213.0
49.10	1473.0
50.10	6990.0
51.10	2042.0
56.10	642.0
57.10	1364.0
59.90	291.0
61.10	1944.0
62.10	1859.0
63.10	1366.0
64.00	161.0
64.90	150.0
68.10	3812.0
69.10	4202.0
70.10	371.0
71.90	273.0
73.10	1992.0
74.10	6806.0
75.10	20368.0
76.10	1752.0
77.10	345.0
77.90	140.0
78.20	152.0
79.00	1529.0
79.90	390.0
80.90	1519.0
82.00	376.0
87.00	1632.0
88.00	1618.0
91.00	277.0
92.00	1177.0
93.10	1928.0
94.10	4608.0
95.10	39336.0
96.10	2448.0
104.00	121.0
106.00	284.0
115.90	212.0
117.00	191.0
117.90	214.0
119.00	288.0
128.10	161.0
129.90	112.0
141.00	350.0
143.00	550.0
148.00	137.0
171.90	147.0
173.00	194.0
174.10	32176.0
175.10	2324.0
176.00	31992.0
177.00	1931.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176