

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040819\
 Data File : VU030847.D
 Acq On : 07 Apr 2019 11:20
 Operator : JC/SP
 Sample : K2283-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZ80

Quant Time: Apr 08 03:56:15 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Apr 08 03:35:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	236852	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	235488	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	99967	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	106850	5.90	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	118.00%
7) Chloroethane-d5	1.68	69	86539	5.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.60%
11) 1,1-Dichloroethene-d2	2.27	63	156889	4.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.60%
20) 2-Butanone-d5	4.19	46	298116	63.92	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	127.84%
24) Chloroform-d	4.64	84	170714	5.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.20%
26) 1,2-Dichloroethane-d4	5.31	65	101605	6.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	124.80%
32) Benzene-d6	5.33	84	339561	5.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.40%
36) 1,2-Dichloropropane-d6	6.32	67	120492	5.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	115.80%
41) Toluene-d8	7.56	98	280822	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.40%
43) trans-1,3-Dichloropropene-	7.85	79	40711	5.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	105.40%
46) 2-Hexanone-d5	8.31	63	202721	60.36	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	120.72%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	93234	6.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	125.20%#
64) 1,2-Dichlorobenzene-d4	11.86	152	99070	5.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.40%


Target Compounds					Qvalue
13) Acetone	2.32	43	7979	2.213 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040819\
Data File : VU030847.D
Acq On : 07 Apr 2019 11:20
Operator : JC/SP
Sample : K2283-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZ80

Quant Time: Apr 08 03:56:15 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Apr 08 03:35:14 2019
Response via : Initial Calibration

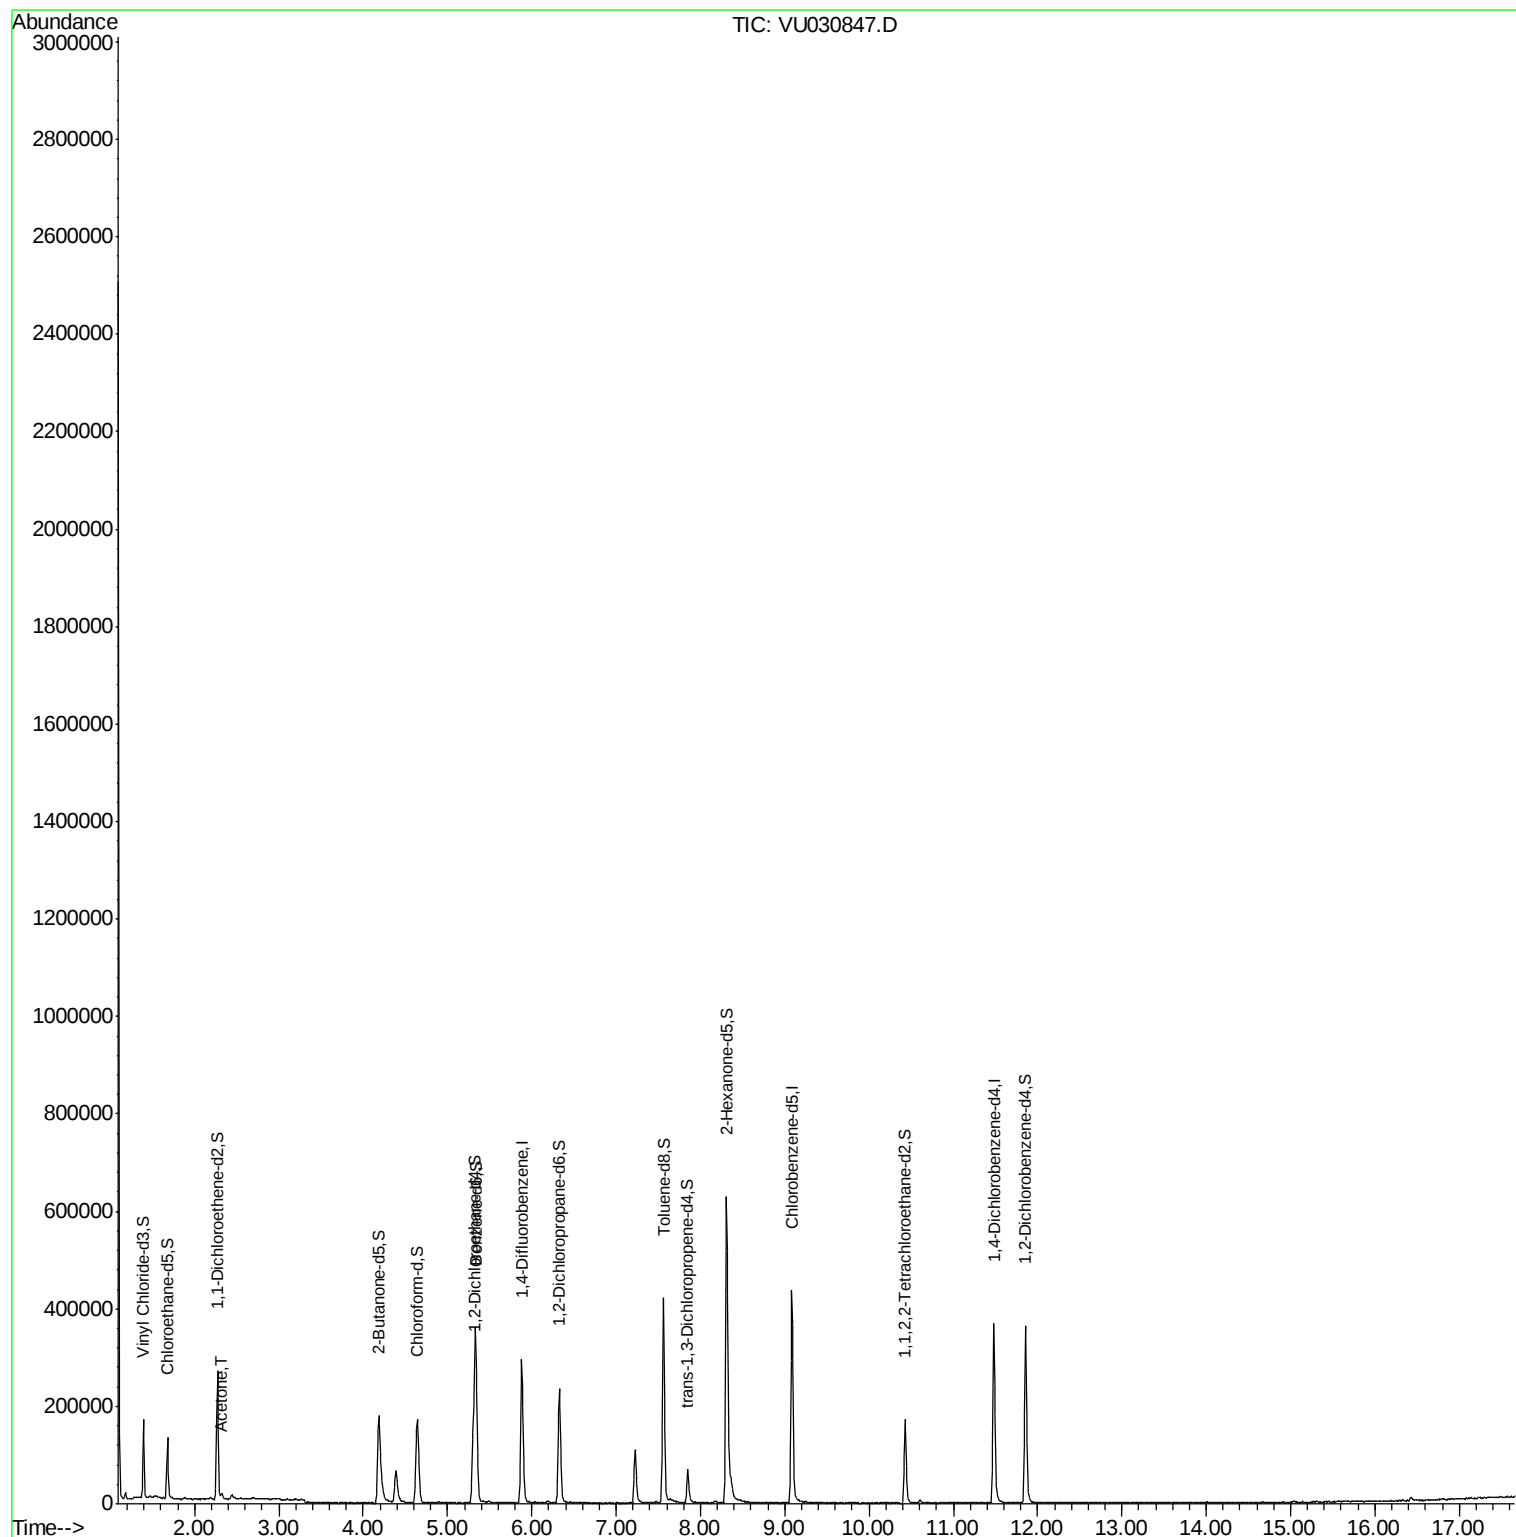

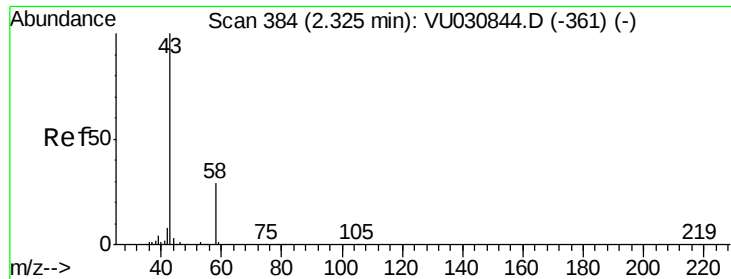

#13

Acetone

Concen: 2.213 ug/L

RT: 2.32 min Scan# 382

Delta R.T. -0.04 min

Lab File: VU030847.D

Acq: 07 Apr 2019 11:20

Instrument :

MSVOA_U

ClientSampleId :

BEZ80

Tgt Ion: 43 Resp: 7979

Ion Ratio Lower Upper

43 100

58 28.4 0.0 62.8

