

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040819\
 Data File : VU030862.D
 Acq On : 07 Apr 2019 17:21
 Operator : JC/SP
 Sample : K2283-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZ95

Quant Time: Apr 08 04:52:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Apr 08 03:35:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	237099	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	242118	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	94771	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	113077	6.24	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	124.80%
7) Chloroethane-d5	1.68	69	92819	6.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	127.00%
11) 1,1-Dichloroethene-d2	2.27	63	163382	4.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.00%
20) 2-Butanone-d5	4.19	46	301241	64.52	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	129.04%
24) Chloroform-d	4.64	84	166952	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.60%
26) 1,2-Dichloroethane-d4	5.31	65	105301	6.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	129.20%
32) Benzene-d6	5.33	84	364297	5.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.20%
36) 1,2-Dichloropropane-d6	6.33	67	125063	5.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	117.00%
41) Toluene-d8	7.56	98	291007	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.20%
43) trans-1,3-Dichloropropene-	7.85	79	40671	5.12	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.40%
46) 2-Hexanone-d5	8.31	63	194570	56.34	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	112.68%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	98243	6.41	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	128.20%#
64) 1,2-Dichlorobenzene-d4	11.86	152	103107	6.50	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	130.00%#


Target Compounds					Qvalue
13) Acetone	2.32	43	8993	2.491 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040819\
Data File : VU030862.D
Acq On : 07 Apr 2019 17:21
Operator : JC/SP
Sample : K2283-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZ95

Quant Time: Apr 08 04:52:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Apr 08 03:35:14 2019
Response via : Initial Calibration

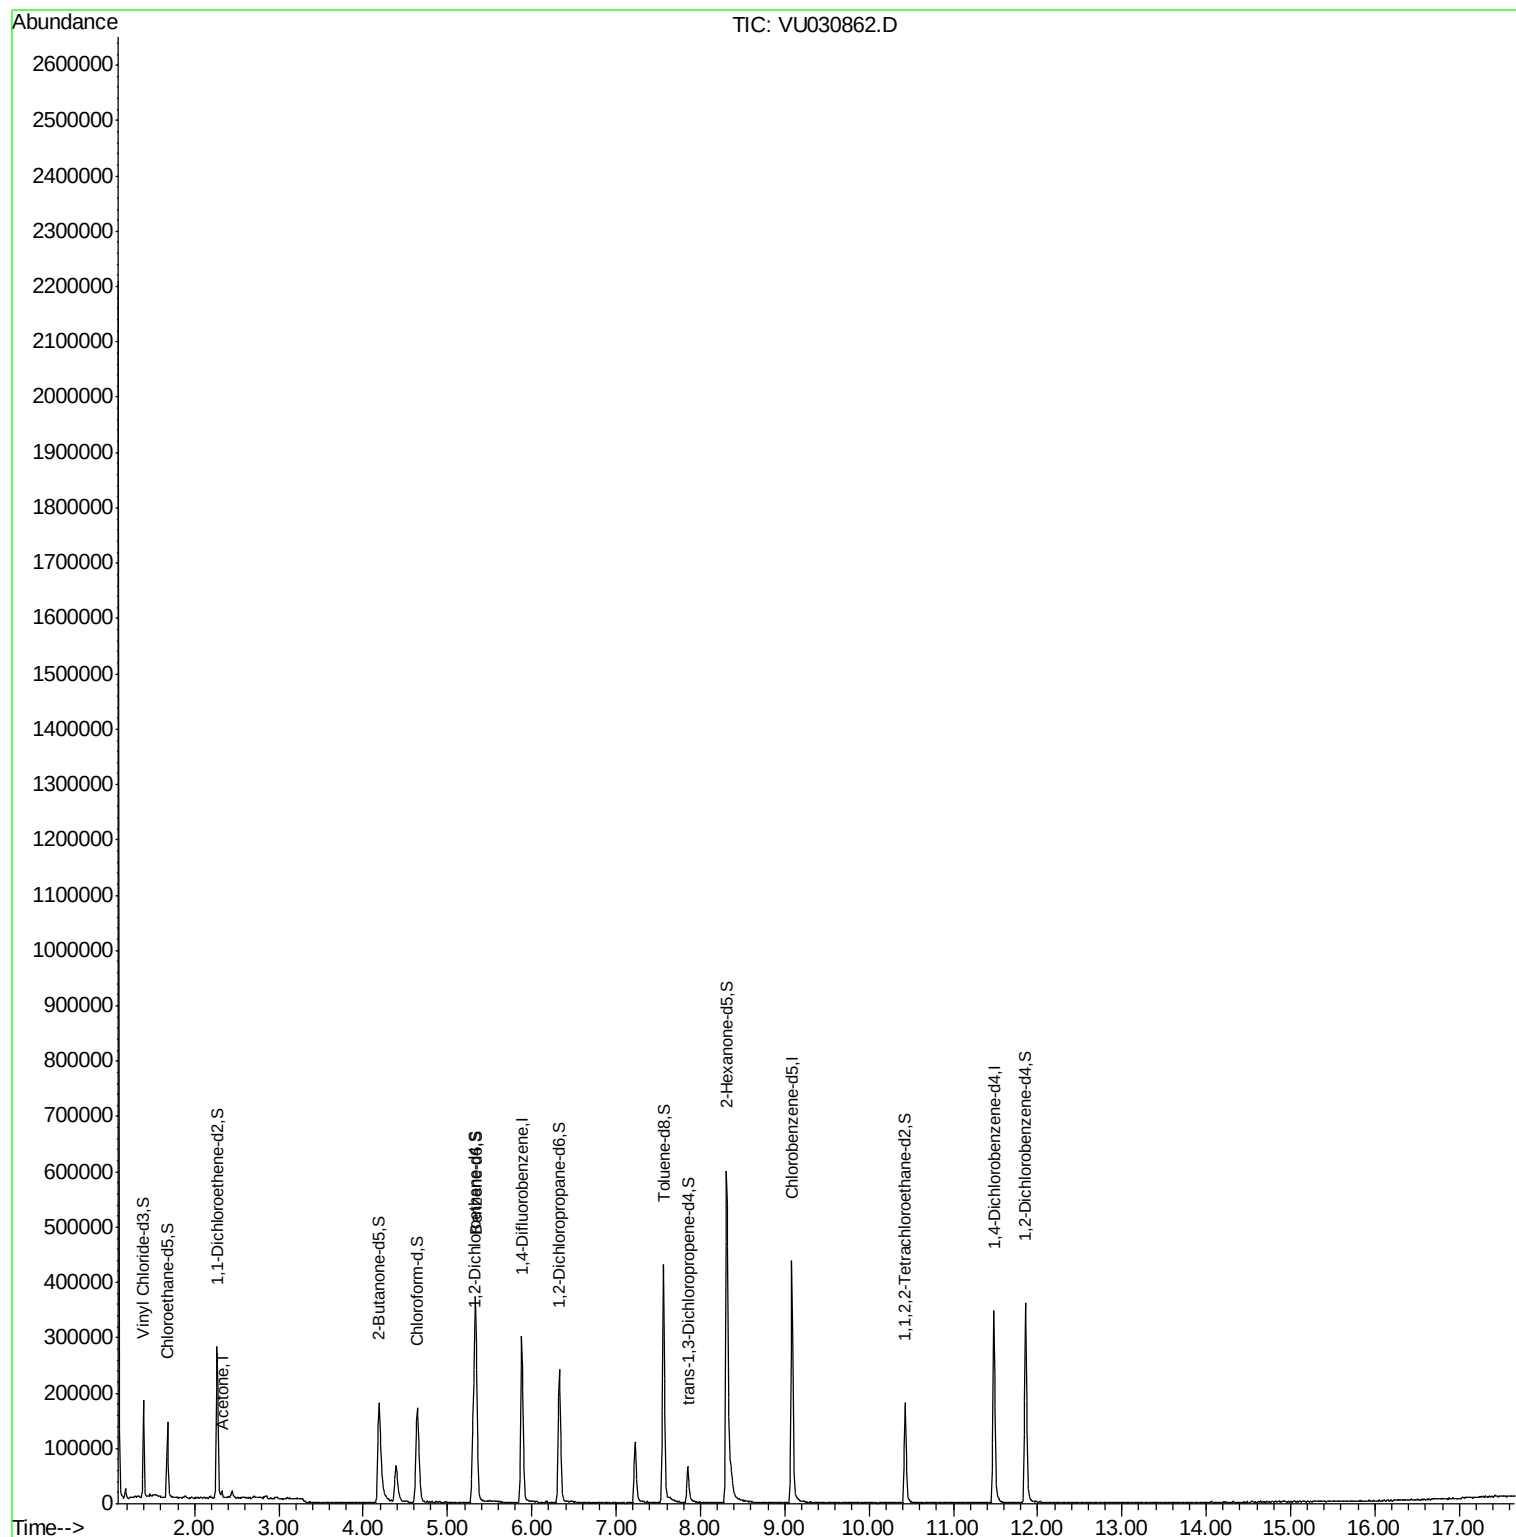

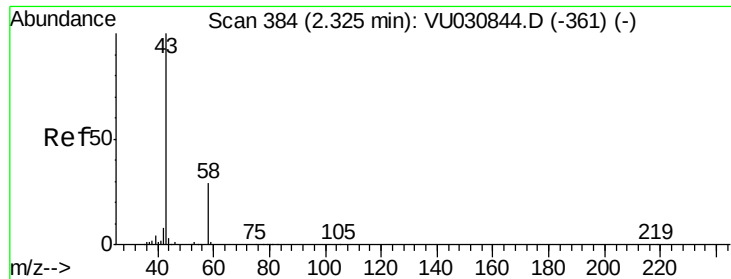

#13

Acetone

Concen: 2.491 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.04 min

Lab File: VU030862.D

Acq: 07 Apr 2019 17:21

Instrument :

MSVOA_U

ClientSampleId :

BEZ95

Tgt Ion: 43 Resp: 8993

Ion Ratio Lower Upper

43 100

58 29.3 0.0 62.8

