

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040819\
 Data File : VU030881.D
 Acq On : 08 Apr 2019 01:25
 Operator : JC/SP
 Sample : K2284-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZB2

Quant Time: Apr 08 05:59:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Apr 08 04:40:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	240693	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	248171	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	94629	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	110705	6.02	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	120.40%
7) Chloroethane-d5	1.68	69	96183	6.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	129.80%
11) 1,1-Dichloroethene-d2	2.27	63	162549	4.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.40%
20) 2-Butanone-d5	4.19	46	312709	65.98	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	131.96%#
24) Chloroform-d	4.64	84	165304	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.00%
26) 1,2-Dichloroethane-d4	5.31	65	108687	6.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	131.40%#
32) Benzene-d6	5.33	84	356317	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.00%
36) 1,2-Dichloropropane-d6	6.33	67	121262	5.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.60%
41) Toluene-d8	7.56	98	280502	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
43) trans-1,3-Dichloropropene-	7.85	79	40538	4.98	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.60%
46) 2-Hexanone-d5	8.31	63	191565	54.12	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.24%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	98937	6.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	126.00%#
64) 1,2-Dichlorobenzene-d4	11.86	152	100715	6.36	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	127.20%#


Target Compounds					Qvalue
13) Acetone	2.32	43	9652	2.634 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040819\
Data File : VU030881.D
Acq On : 08 Apr 2019 01:25
Operator : JC/SP
Sample : K2284-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZB2

Quant Time: Apr 08 05:59:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Apr 08 04:40:32 2019
Response via : Initial Calibration

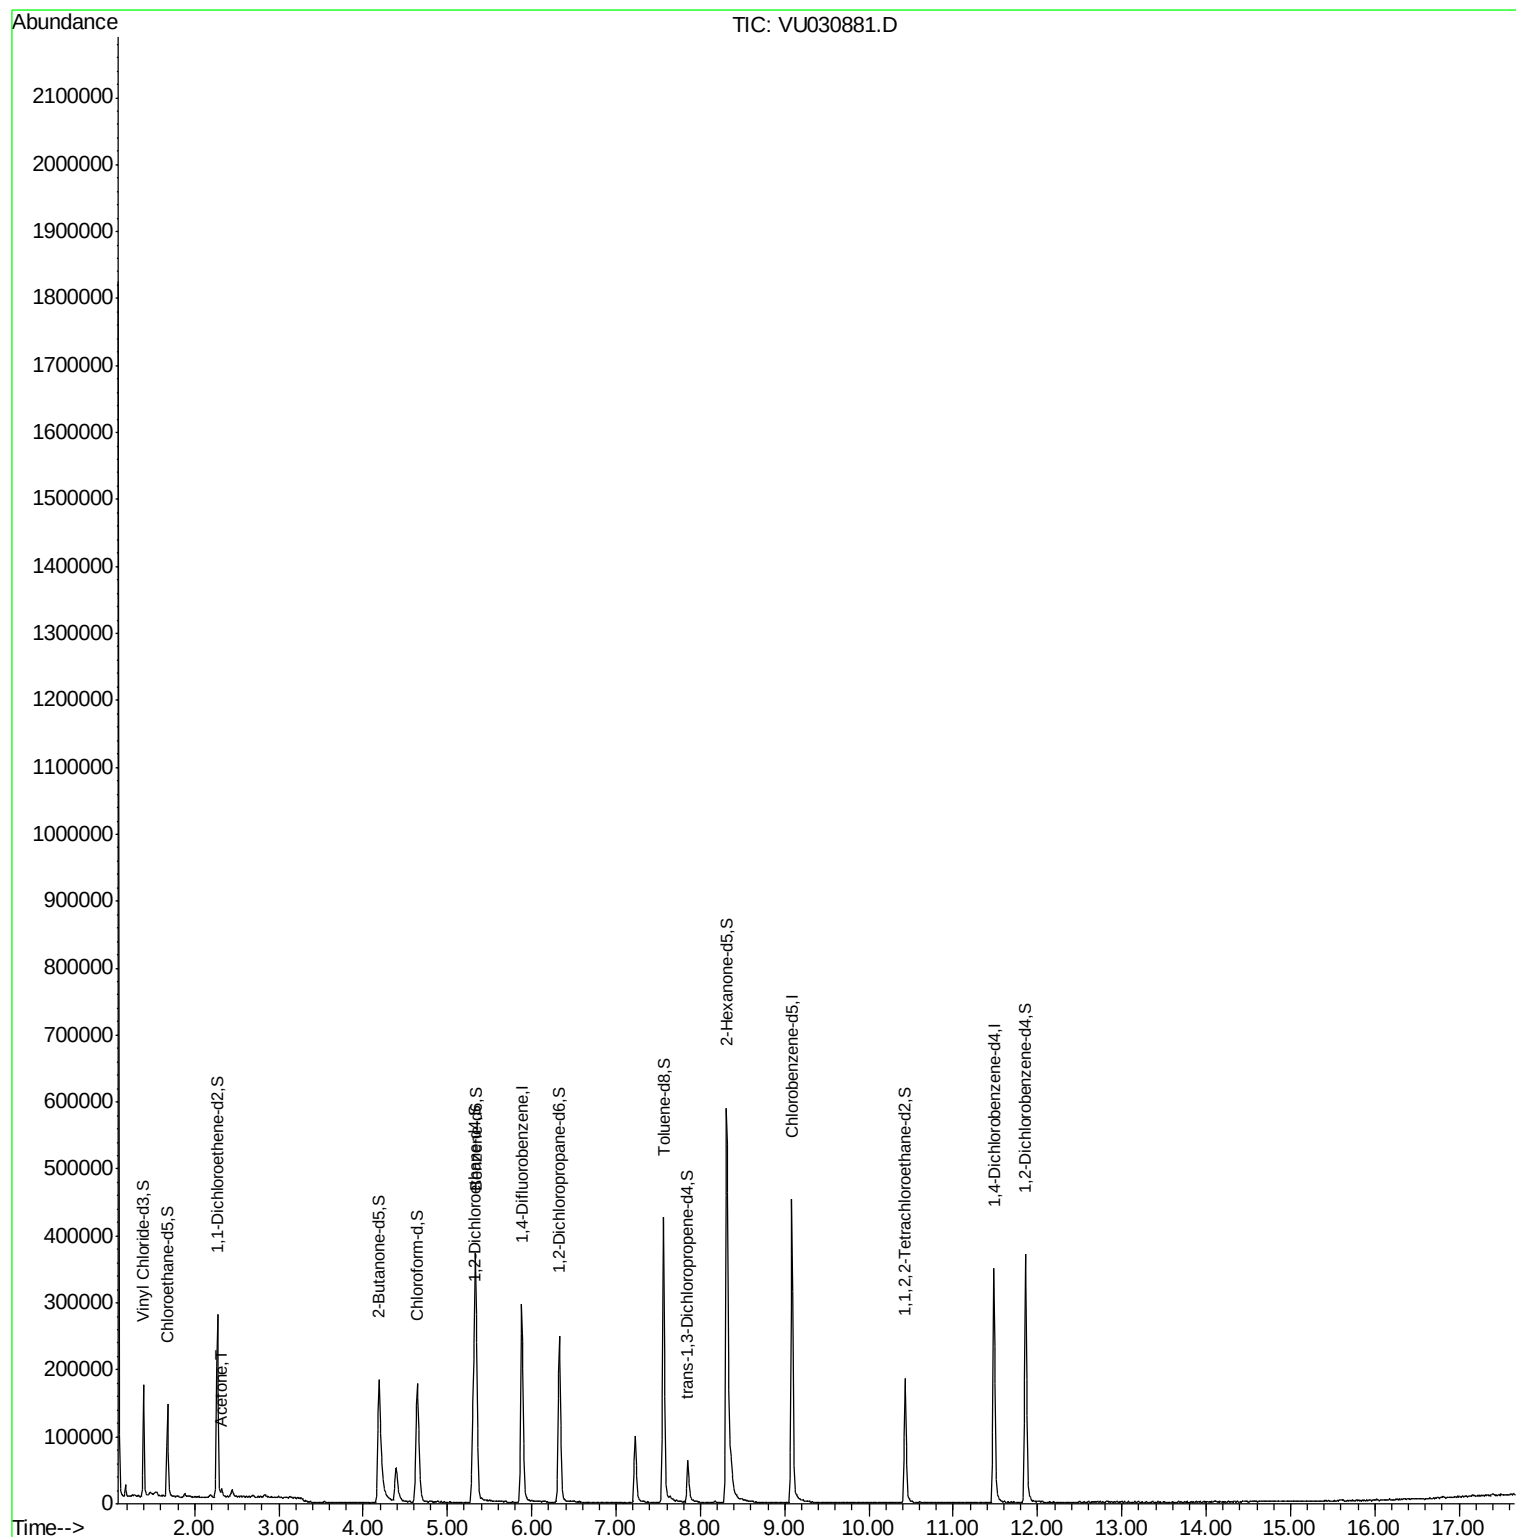

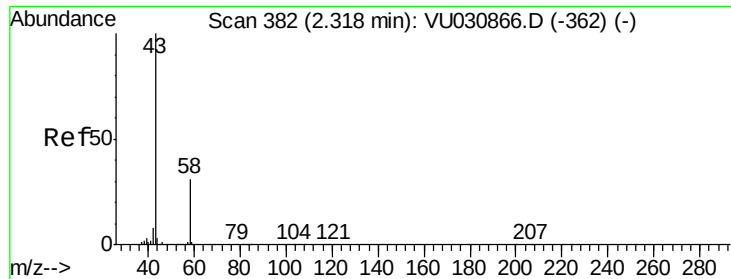

#13
 Acetone
 Concen: 2.634 ug/L
 RT: 2.32 min Scan# 382
 Delta R.T. -0.04 min
 Lab File: VU030881.D
 Acq: 08 Apr 2019 01:25

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZB2

Tgt Ion: 43 Resp: 9652
 Ion Ratio Lower Upper
 43 100
 58 29.2 0.0 62.8

