

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040819\
 Data File : VU030873.D
 Acq On : 07 Apr 2019 22:11
 Operator : JC/SP
 Sample : K2284-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZA4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	36	rVB	18979	19003	1.19%	0.190%
2	1.395	88	95	106	rBV	164312	171114	10.69%	1.712%
3	1.678	174	183	194	rVB	134112	169310	10.57%	1.694%
4	2.270	355	367	378	rBV	261756	407272	25.43%	4.076%
5	4.190	947	964	993	rBV	170909	488361	30.50%	4.887%
6	4.399	1017	1029	1054	rVB3	19379	51100	3.19%	0.511%
7	4.643	1088	1105	1128	rBV3	163940	431389	26.94%	4.317%
8	4.907	1170	1187	1200	rVB7	12811	32519	2.03%	0.325%
9	5.331	1296	1319	1347	rBV4	361578	1013814	63.31%	10.145%
10	5.881	1475	1490	1513	rBV	288303	583558	36.44%	5.840%
11	6.180	1567	1583	1611	rBV	808280	1601395	100.00%	16.025%
12	6.328	1616	1629	1649	rVV	241855	488211	30.49%	4.886%
13	7.225	1897	1908	1928	rBV	101497	191148	11.94%	1.913%
14	7.562	1999	2013	2031	rBV	409642	742706	46.38%	7.432%
15	7.852	2092	2103	2118	rBV	62264	113570	7.09%	1.137%
16	8.312	2235	2246	2293	rBV2	564316	1232580	76.97%	12.335%
17	9.086	2473	2487	2516	rBV	429157	755487	47.18%	7.560%
18	10.430	2892	2905	2924	rBV	176157	296291	18.50%	2.965%
19	11.482	3221	3232	3261	rBV	343150	595631	37.19%	5.961%
20	11.858	3331	3349	3369	rBV	343738	608450	37.99%	6.089%


Sum of corrected areas: 9992909

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040819\
Data File : VU030873.D
Acq On : 07 Apr 2019 22:11
Operator : JC/SP
Sample : K2284-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BEZA4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

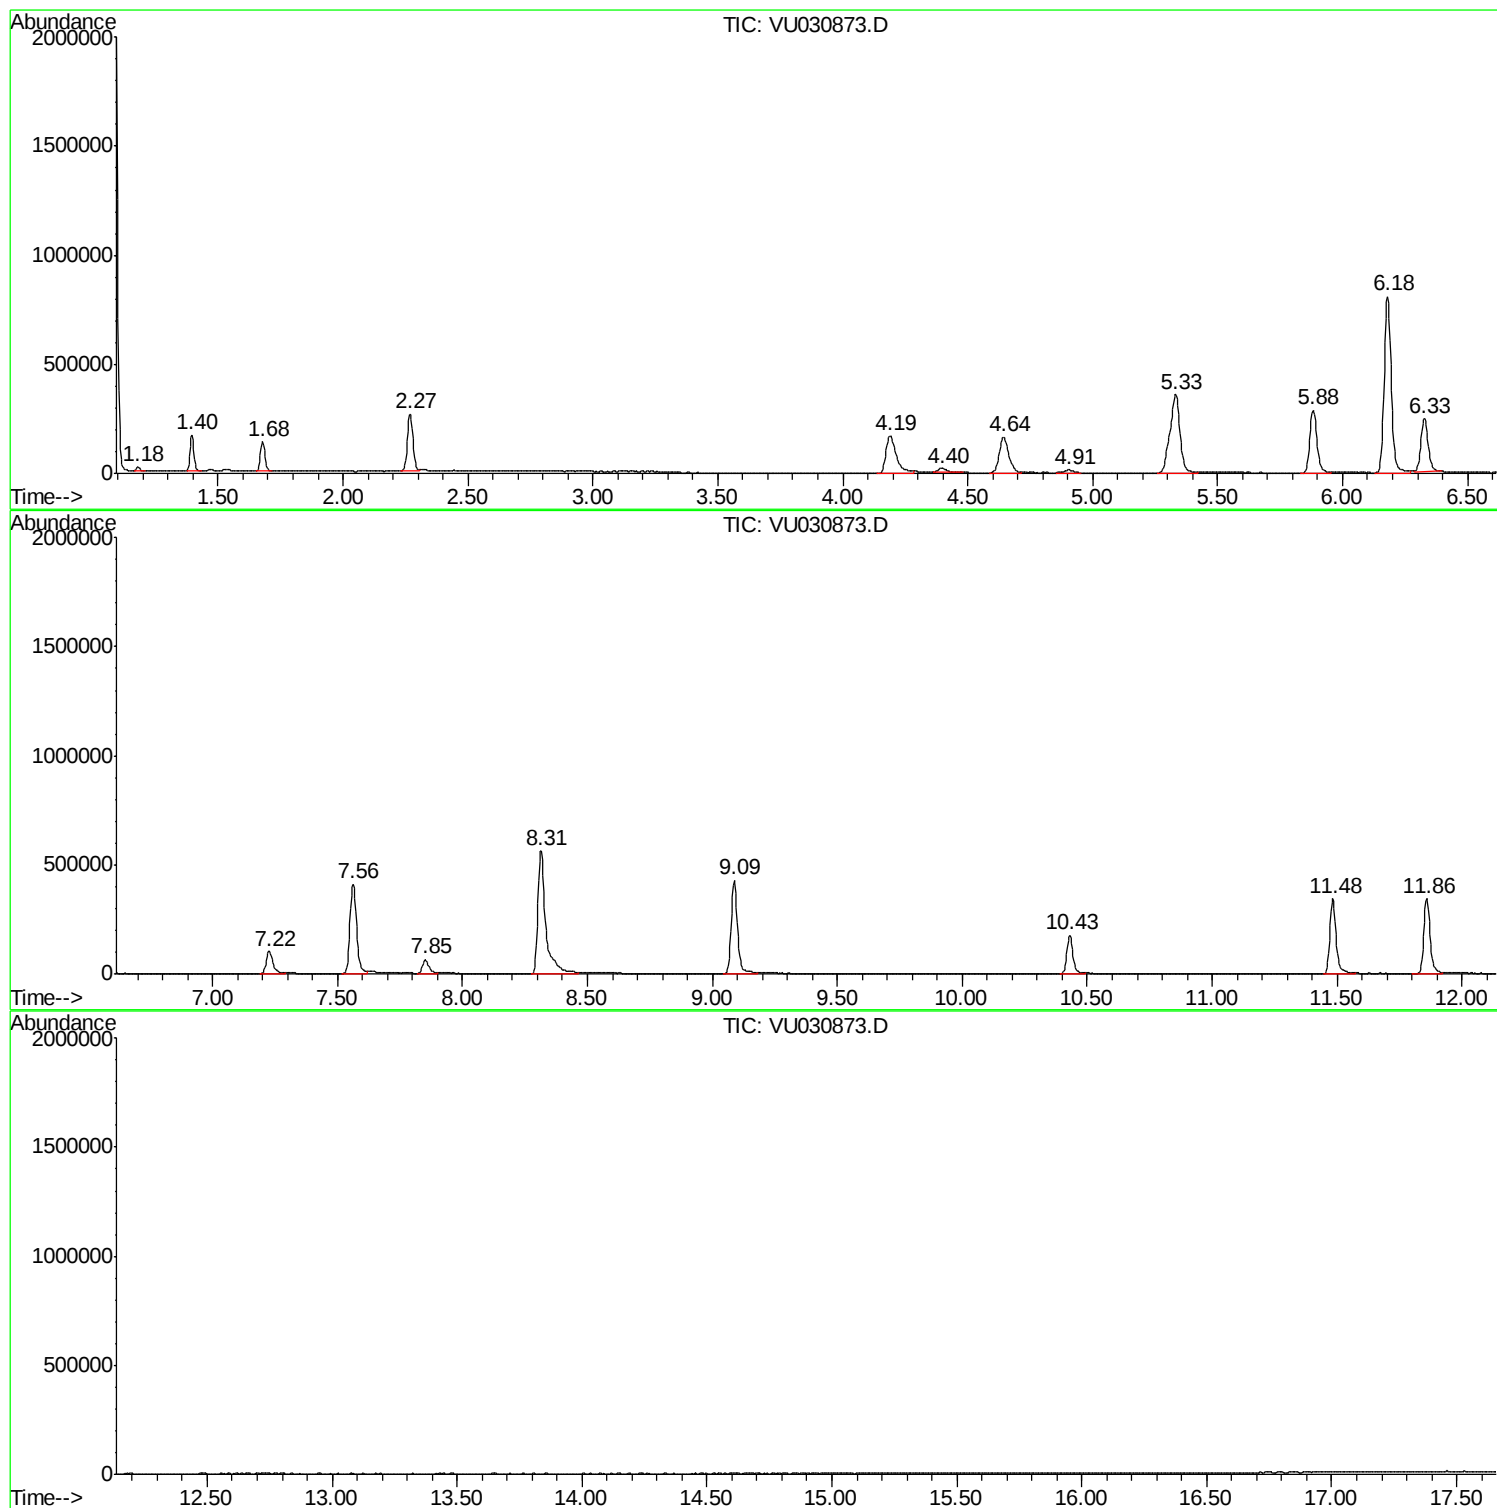

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040819\
Data File : VU030873.D
Acq On : 07 Apr 2019 22:11
Operator : JC/SP
Sample : K2284-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZA4










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.22	1.64 ug/L	191148	1,4-Difluorobenzene	5.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	37
2		Thiophosgene	114	CCl2S	000463-71-8	35
3		3-Thiatricyclo[3.1.1.0(2,4)]heptane	112	C6H8S	1000221-37-0	9
4		2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9
5		2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9

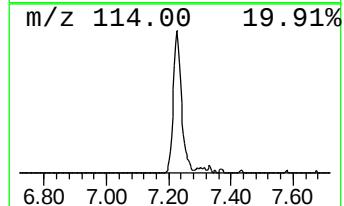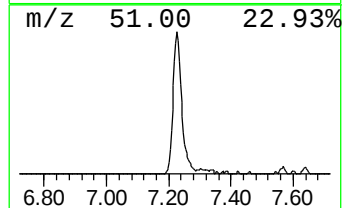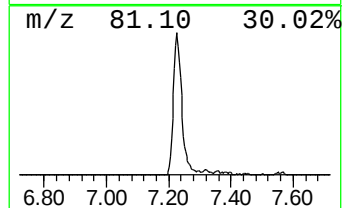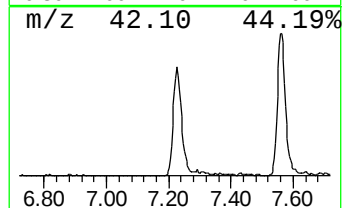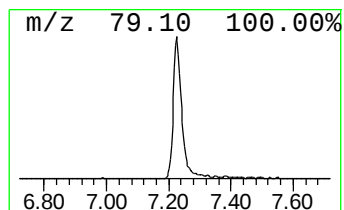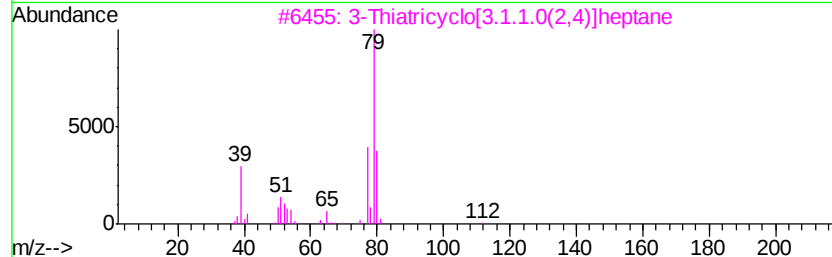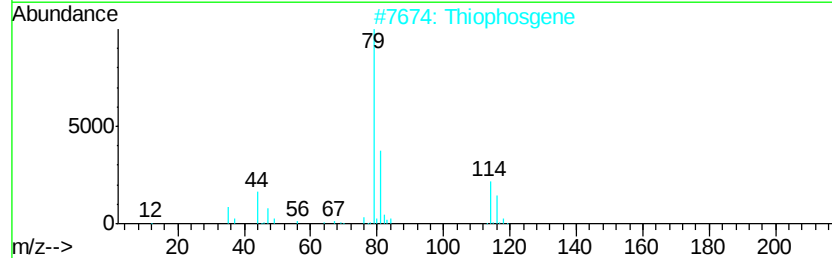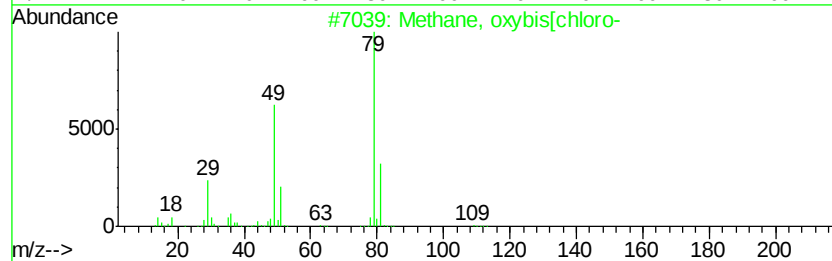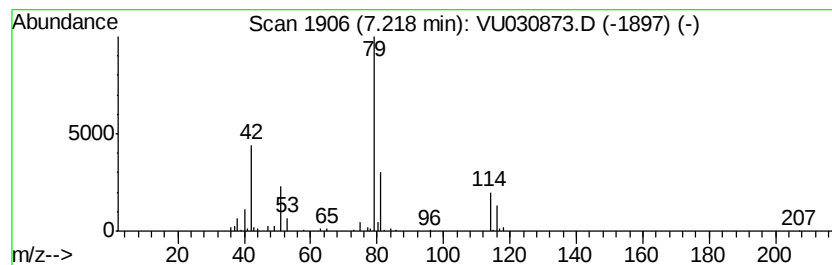

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040819\
Data File : VU030873.D
Acq On : 07 Apr 2019 22:11
Operator : JC/SP
Sample : K2284-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZA4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.22	1.6	ug/L	191148	1	5.88	583558	5.0