


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040821\
Data File : VU042982.D
Acq On : 08 Apr 2021 09:42
Operator : SY/MD
Sample : BFB64
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB641

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM040821WMA.M
Title : VOC Analysis
Last Update : Fri Apr 09 02:13:24 2021

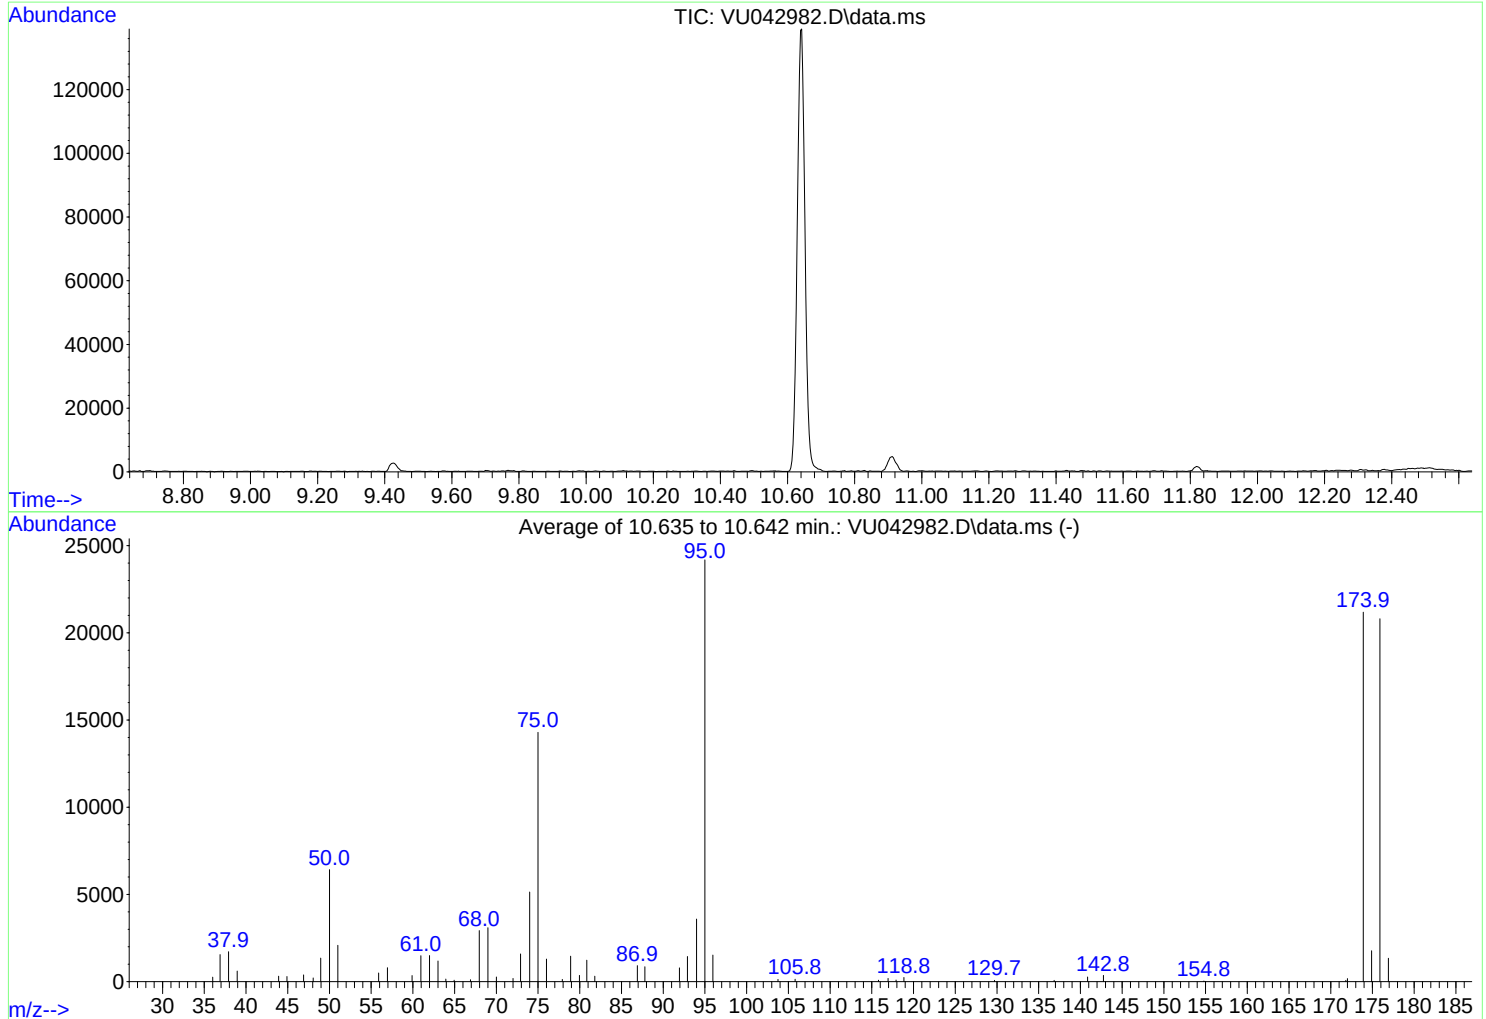

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2880

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	26.6	6426	PASS
75	95	30	80	59.1	14299	PASS
95	95	100	100	100.0	24187	PASS
96	95	5	9	6.3	1523	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.6	21187	PASS
175	174	5	9	8.4	1773	PASS
176	174	95	101	98.2	20811	PASS
177	176	5	9	6.4	1339	PASS

m/z	Abundance
43.90	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB641

m/z	Abundance
36.00	240.0
36.90	1456.0
37.90	1806.0
39.00	665.0
43.90	484.0
44.90	232.0
46.90	455.0
48.00	216.0
49.00	1410.0
50.00	6591.0
51.00	2120.0
55.90	479.0
57.00	719.0
59.90	357.0
61.00	1460.0
62.00	1511.0
63.00	1244.0
63.90	166.0
65.00	137.0
66.90	166.0
68.00	2924.0
69.00	3230.0
70.00	255.0
72.00	196.0
72.90	1614.0
74.00	5207.0
75.00	14769.0
76.00	1244.0
77.90	138.0
78.90	1501.0
79.90	388.0
80.90	1339.0
81.80	330.0
86.90	973.0
87.80	861.0
92.00	777.0
92.90	1507.0
94.00	3678.0
95.00	24680.0
95.90	1514.0
103.70	127.0
105.80	116.0
116.90	180.0
117.90	156.0
118.80	251.0
129.70	119.0
136.80	124.0
140.80	234.0
142.80	409.0
154.80	119.0
172.00	281.0
173.90	22496.0
174.90	1779.0
175.90	22200.0
176.90	1354.0

Instrument :
MSVOA_U
ClientSampleId :
BFB641

m/z	Abundance
36.00	270.0
36.90	1593.0
37.90	1748.0
38.90	617.0
43.90	495.0
44.90	314.0
46.90	400.0
48.00	223.0
49.00	1372.0
50.00	6619.0
51.00	2177.0
55.90	508.0
57.00	808.0
59.90	366.0
61.00	1523.0
62.00	1573.0
63.00	1210.0
63.90	149.0
64.90	121.0
66.90	151.0
68.00	3032.0
69.00	3199.0
70.00	294.0
72.00	194.0
72.90	1673.0
74.00	5238.0
75.00	14830.0
76.00	1359.0
77.90	150.0
78.90	1527.0
79.90	357.0
80.90	1257.0
81.80	306.0
86.90	933.0
87.80	912.0
92.00	828.0
92.90	1479.0
94.00	3661.0
95.00	24912.0
96.00	1566.0
103.80	131.0
105.80	143.0
115.80	130.0
117.00	186.0
117.90	120.0
118.90	251.0
129.70	104.0
136.90	104.0
140.80	277.0
142.70	372.0
172.00	242.0
173.90	21776.0
174.90	1798.0
175.90	21624.0
176.90	1405.0

Instrument :
MSVOA_U
ClientSampleId :
BFB641

m/z	Abundance
36.00	249.0
36.90	1612.0
37.90	1584.0
38.90	536.0
43.90	418.0
44.90	340.0
46.90	315.0
48.10	192.0
48.90	1261.0
50.00	6068.0
51.00	1943.0
55.90	504.0
56.90	854.0
59.90	315.0
60.90	1467.0
62.00	1410.0
63.00	1088.0
64.00	115.0
67.90	2817.0
69.00	2842.0
70.00	253.0
72.00	165.0
72.90	1487.0
74.00	4976.0
75.00	13298.0
76.00	1291.0
77.90	104.0
78.90	1345.0
80.00	338.0
80.80	1090.0
81.80	307.0
86.90	852.0
87.80	790.0
91.90	750.0
92.90	1325.0
94.00	3429.0
95.00	22968.0
96.00	1488.0
103.80	132.0
105.80	146.0
115.80	111.0
117.00	189.0
118.90	218.0
140.90	288.0
142.70	283.0
171.80	215.0
173.90	19288.0
174.90	1742.0
175.90	18608.0
176.90	1257.0

Instrument :
MSVOA_U
ClientSampleId :
BFB641