


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040919\
 Data File : VU030889.D
 Acq On : 08 Apr 2019 08:36
 Operator : JC/SP
 Sample : BFB53
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB53

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 09 02:16:31 2019

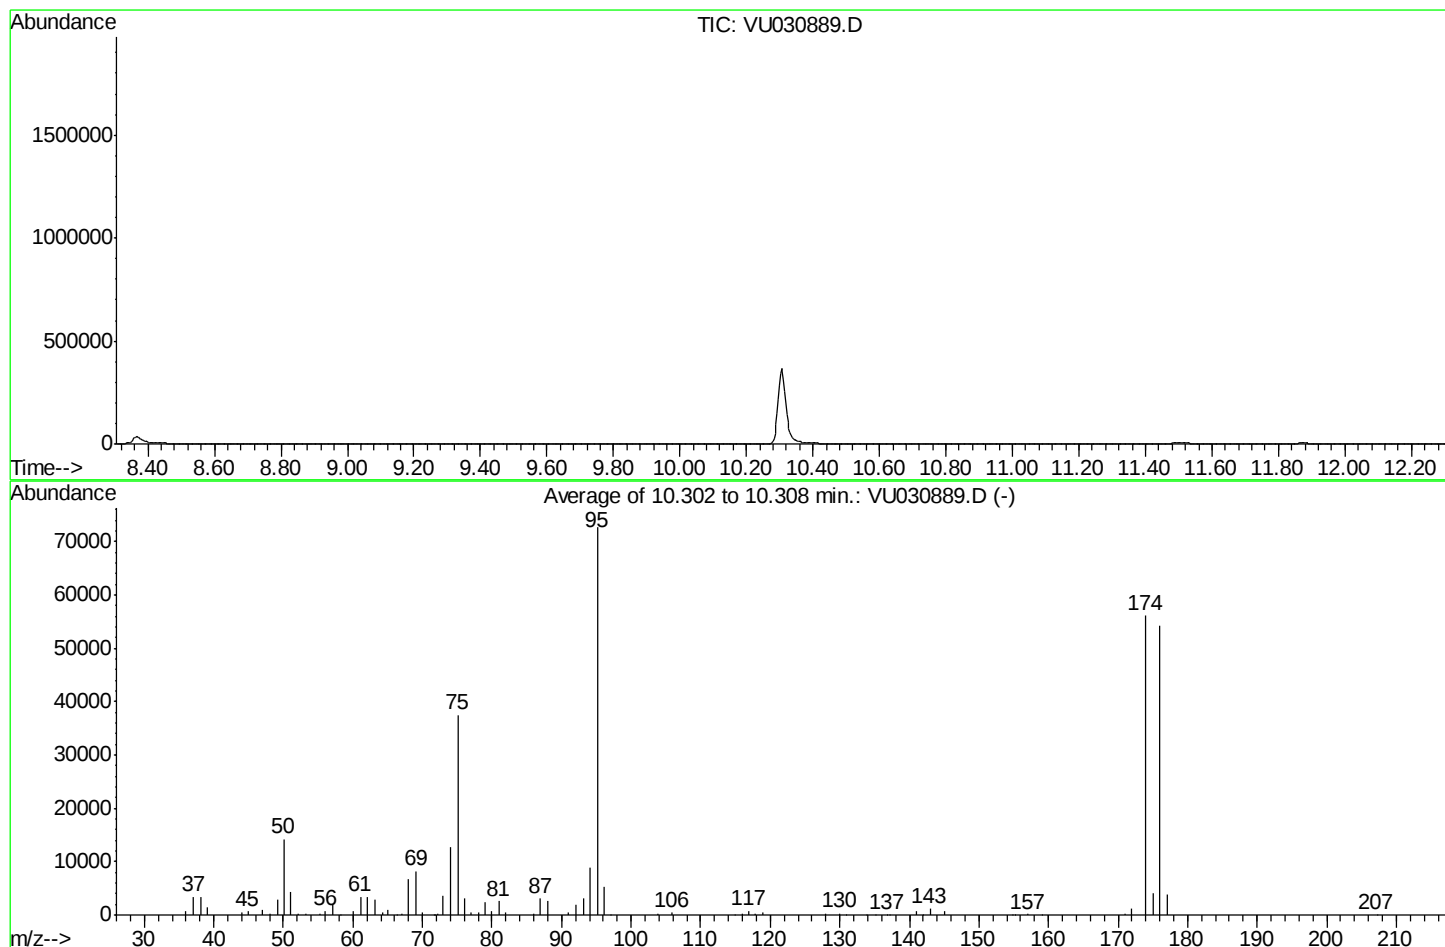

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	14221	PASS
75	95	30	80	51.7	37549	PASS
95	95	100	100	100.0	72688	PASS
96	95	5	9	7.3	5306	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.2	56130	PASS
175	174	5	9	7.4	4166	PASS
176	174	95	101	96.5	54157	PASS
177	176	5	9	7.1	3825	PASS

Scan 2853 (10.263 min): VU030889.D
BFB53

m/z	Abundance
40.00	655.0
43.90	916.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	546.0
37.10	3505.0
38.10	3376.0
39.10	1437.0
40.00	659.0
44.00	1536.0
44.90	594.0
46.90	832.0
48.10	417.0
49.10	2619.0
50.10	14432.0
51.10	4124.0
52.00	261.0
53.10	207.0
55.30	202.0
56.00	710.0
57.10	1956.0
60.10	698.0
61.10	3437.0
62.00	3556.0
63.10	3191.0
64.20	463.0
65.10	914.0
67.10	129.0
68.00	6613.0
69.10	7955.0
70.00	540.0
71.60	174.0
72.20	210.0
73.00	3554.0
74.10	12975.0
75.10	36048.0
76.00	2979.0
77.00	568.0
78.10	457.0
79.00	2388.0
79.90	634.0
81.00	2375.0
81.90	481.0
86.00	118.0
87.00	3108.0
88.00	2625.0
91.00	330.0
92.00	1566.0
93.10	3222.0
94.10	8619.0
95.10	70968.0
96.10	5390.0
103.90	205.0
105.90	253.0
114.90	130.0
115.90	243.0
116.90	747.0
117.80	275.0
118.90	438.0
127.90	214.0
130.00	233.0
136.80	264.0
140.90	841.0
143.00	1009.0
145.00	529.0
157.10	168.0
159.10	139.0
171.10	165.0
172.00	1095.0
174.00	52944.0
175.10	4125.0
176.00	50576.0
177.10	3824.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	655.0
37.10	3548.0
38.10	3477.0
39.10	1520.0
40.00	627.0
44.00	1514.0
45.00	618.0
46.90	1065.0
48.00	316.0
49.10	3169.0
50.10	14489.0
51.10	4382.0
52.10	205.0
53.20	221.0
55.30	206.0
56.00	795.0
57.10	1933.0
58.20	116.0
60.10	769.0
61.10	3623.0
62.00	3542.0
63.10	2921.0
64.20	455.0
65.00	1057.0
67.10	161.0
68.00	6937.0
69.10	8583.0
70.00	563.0
71.80	211.0
72.10	248.0
73.00	3786.0
74.10	13156.0
75.10	38872.0
76.10	3065.0
77.10	592.0
78.20	486.0
79.00	2536.0
79.90	697.0
80.90	2706.0
81.90	548.0
86.00	182.0
86.90	3174.0
88.00	2691.0
91.00	406.0
92.00	1906.0
93.10	3268.0
94.10	9243.0
95.10	75248.0
96.10	5367.0
103.90	240.0
106.00	394.0
115.90	307.0
117.00	785.0
117.80	218.0
118.90	585.0
127.90	228.0
130.00	293.0
136.80	112.0
137.10	160.0
140.90	790.0
143.00	1107.0
145.00	670.0
154.90	108.0
157.10	214.0
159.10	123.0
171.00	157.0
172.00	1192.0
174.00	58152.0
175.10	4291.0
176.00	56296.0
177.10	3997.0
207.20	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	698.0
37.10	3195.0
38.10	3330.0
39.10	1407.0
40.00	556.0
44.00	1335.0
45.00	672.0
46.90	1163.0
49.10	3203.0
50.10	13744.0
51.10	4276.0
52.10	210.0
53.20	160.0
55.20	199.0
56.00	895.0
57.10	1688.0
58.20	113.0
60.10	733.0
61.10	3373.0
62.00	3314.0
63.10	2545.0
64.20	371.0
65.00	1132.0
66.30	101.0
67.10	236.0
68.00	6871.0
69.10	8208.0
70.00	453.0
72.00	298.0
73.00	3706.0
74.10	11752.0
75.10	37728.0
76.10	2988.0
77.10	521.0
78.20	464.0
79.00	2465.0
79.90	722.0
80.90	2848.0
81.90	548.0
86.00	199.0
86.90	2816.0
88.00	2665.0
90.90	373.0
92.00	2024.0
93.10	2991.0
94.10	9049.0
95.10	71848.0
96.10	5161.0
97.10	201.0
103.90	292.0
106.00	483.0
115.90	350.0
117.00	719.0
117.70	196.0
118.90	706.0
127.90	224.0
130.00	317.0
130.90	104.0
133.90	130.0
135.10	102.0
137.10	112.0
141.00	758.0
142.00	121.0
142.90	1227.0
145.00	694.0
155.20	140.0
157.10	168.0
171.00	152.0
172.00	1097.0
174.00	57296.0
175.10	4082.0
176.00	55600.0
177.10	3656.0
207.20	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53