

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040920\
 Data File : VU037621.D
 Acq On : 09 Apr 2020 16:29
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	97	rVB	344488	361207	15.94%	2.032%
2	1.932	177	184	196	rVB	256167	330087	14.57%	1.857%
3	2.591	378	389	405	rVB	470272	770337	34.00%	4.333%
4	3.433	648	651	653	rBV2	1015	593	0.03%	0.003%
5	3.674	724	726	729	rBV2	607	287	0.01%	0.002%
6	3.932	804	806	809	rBV3	521	390	0.02%	0.002%
7	3.980	815	821	824	rBV6	896	1005	0.04%	0.006%
8	4.006	827	829	832	rVV3	450	224	0.01%	0.001%
9	4.080	849	852	856	rBV3	449	396	0.02%	0.002%
10	4.482	974	977	984	rVB6	894	1046	0.05%	0.006%
11	4.520	984	989	990	rBV3	555	440	0.02%	0.002%
12	4.543	993	996	998	rBV4	474	274	0.01%	0.002%
13	4.575	1003	1006	1007	rBV3	525	296	0.01%	0.002%
14	4.665	1018	1034	1066	rBV	269711	642545	28.36%	3.614%
15	4.938	1116	1119	1122	rBV4	677	658	0.03%	0.004%
16	4.983	1131	1133	1134	rBV2	207	71	0.00%	0.000%
17	5.028	1145	1147	1148	rBV2	474	203	0.01%	0.001%
18	5.102	1153	1170	1195	rVV	377771	842063	37.16%	4.737%
19	5.282	1221	1226	1230	rBV5	953	1100	0.05%	0.006%
20	5.340	1234	1244	1248	rBV8	2105	3730	0.16%	0.021%
21	5.408	1261	1265	1268	rBV4	1040	945	0.04%	0.005%
22	5.546	1306	1308	1311	rBV3	560	233	0.01%	0.001%
23	5.620	1327	1331	1333	rBV4	607	456	0.02%	0.003%
24	5.761	1348	1375	1393	rBV2	862681	2265793	100.00%	12.745%
25	6.073	1464	1472	1473	rBV6	1905	1982	0.09%	0.011%
26	6.224	1516	1519	1522	rBV4	547	536	0.02%	0.003%
27	6.282	1522	1537	1555	rVV	689038	1292156	57.03%	7.268%
28	6.562	1613	1624	1635	rBV9	5250	11594	0.51%	0.065%
29	6.636	1645	1647	1649	rBV3	478	189	0.01%	0.001%
30	6.662	1653	1655	1656	rBV	341	126	0.01%	0.001%
31	6.723	1659	1674	1693	rBV	535931	1039833	45.89%	5.849%
32	7.015	1763	1765	1767	rBV3	569	320	0.01%	0.002%
33	7.044	1772	1774	1775	rBV2	500	276	0.01%	0.002%
34	7.067	1778	1781	1785	rBV5	721	652	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040920\
 Data File : VU037621.D
 Acq On : 09 Apr 2020 16:29
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
 Title : VOC Analysis

35	7.118	1795	1797	1799	rBV	438	242	0.01%	0.001%
36	7.202	1810	1823	1826	rBV8	2792	4287	0.19%	0.024%
37	7.305	1854	1855	1856	rBV	399	116	0.01%	0.001%
38	7.346	1863	1868	1872	rBV6	623	619	0.03%	0.003%
39	7.366	1872	1874	1875	rBV	372	158	0.01%	0.001%
40	7.411	1886	1888	1891	rBV3	430	223	0.01%	0.001%
41	7.427	1891	1893	1898	rBV4	565	438	0.02%	0.002%
42	7.591	1931	1944	1958	rBV	346643	591842	26.12%	3.329%
43	7.819	2008	2015	2025	rVB4	3837	6403	0.28%	0.036%
44	7.861	2025	2028	2031	rBV3	838	506	0.02%	0.003%
45	7.922	2031	2047	2065	rBV	1104137	1870709	82.56%	10.523%
46	8.134	2111	2113	2116	rVB3	914	445	0.02%	0.003%
47	8.202	2122	2134	2151	rBV	245377	406875	17.96%	2.289%
48	8.481	2219	2221	2223	rBV2	941	502	0.02%	0.003%
49	8.523	2231	2234	2238	rVB3	768	540	0.02%	0.003%
50	8.655	2260	2275	2307	rBV	798222	1403451	61.94%	7.894%
51	8.935	2352	2362	2363	rBV7	3208	3404	0.15%	0.019%
52	9.050	2397	2398	2401	rBV2	326	172	0.01%	0.001%
53	9.166	2431	2434	2435	rBV2	799	491	0.02%	0.003%
54	9.218	2449	2450	2451	rBV	173	37	0.00%	0.000%
55	9.234	2451	2455	2456	rBV2	507	388	0.02%	0.002%
56	9.276	2464	2468	2472	rVB4	914	838	0.04%	0.005%
57	9.295	2472	2474	2479	rBV3	456	487	0.02%	0.003%
58	9.356	2491	2493	2496	rBV2	555	339	0.01%	0.002%
59	9.372	2496	2498	2502	rVB3	695	312	0.01%	0.002%
60	9.436	2505	2518	2539	rBV	972575	1585131	69.96%	8.916%
61	9.562	2552	2557	2561	rBV7	720	984	0.04%	0.006%
62	9.748	2613	2615	2616	rBV2	240	83	0.00%	0.000%
63	9.767	2616	2621	2623	rBV4	564	411	0.02%	0.002%
64	9.790	2624	2628	2629	rBV2	473	285	0.01%	0.002%
65	9.848	2643	2646	2649	rBV3	627	530	0.02%	0.003%
66	9.877	2653	2655	2656	rBV	412	166	0.01%	0.001%
67	9.960	2679	2681	2683	rBV3	519	272	0.01%	0.002%
68	10.160	2741	2743	2746	rVB3	774	450	0.02%	0.003%
69	10.176	2746	2748	2750	rBV2	374	199	0.01%	0.001%
70	10.253	2771	2772	2773	rBV2	526	171	0.01%	0.001%
71	10.337	2795	2798	2801	rVB3	239	163	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040920\
 Data File : VU037621.D
 Acq On : 09 Apr 2020 16:29
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
 Title : VOC Analysis

72	10.356	2801	2804	2807	rBV3	424	332	0.01%	0.002%
73	10.375	2807	2810	2813	rBV2	508	346	0.02%	0.002%
74	10.648	2893	2895	2900	rVB4	1262	966	0.04%	0.005%
75	10.677	2900	2904	2906	rBV2	1005	808	0.04%	0.005%
76	10.771	2918	2933	2952	rBV	679173	1103007	48.68%	6.204%
77	10.902	2970	2974	2983	rVB5	2526	3487	0.15%	0.020%
78	10.957	2989	2991	2992	rBV2	452	173	0.01%	0.001%
79	10.999	3001	3004	3008	rBV3	1066	686	0.03%	0.004%
80	11.189	3060	3063	3065	rBV2	423	310	0.01%	0.002%
81	11.385	3121	3124	3126	rBV3	506	250	0.01%	0.001%
82	11.430	3137	3138	3139	rBV	462	106	0.00%	0.001%
83	11.529	3166	3169	3171	rVB2	709	432	0.02%	0.002%
84	11.542	3171	3173	3174	rBV	491	139	0.01%	0.001%
85	11.587	3185	3187	3188	rBV3	439	172	0.01%	0.001%
86	11.597	3188	3190	3193	rBV3	502	308	0.01%	0.002%
87	11.825	3248	3261	3278	rBV	991639	1571059	69.34%	8.837%
88	12.156	3361	3364	3365	rBV	836	431	0.02%	0.002%
89	12.205	3366	3379	3397	rVB	1023450	1639128	72.34%	9.220%
90	12.330	3414	3418	3419	rBV3	1176	834	0.04%	0.005%


Sum of corrected areas: 17777686

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040920\
Data File : VU037621.D
Acq On : 09 Apr 2020 16:29
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

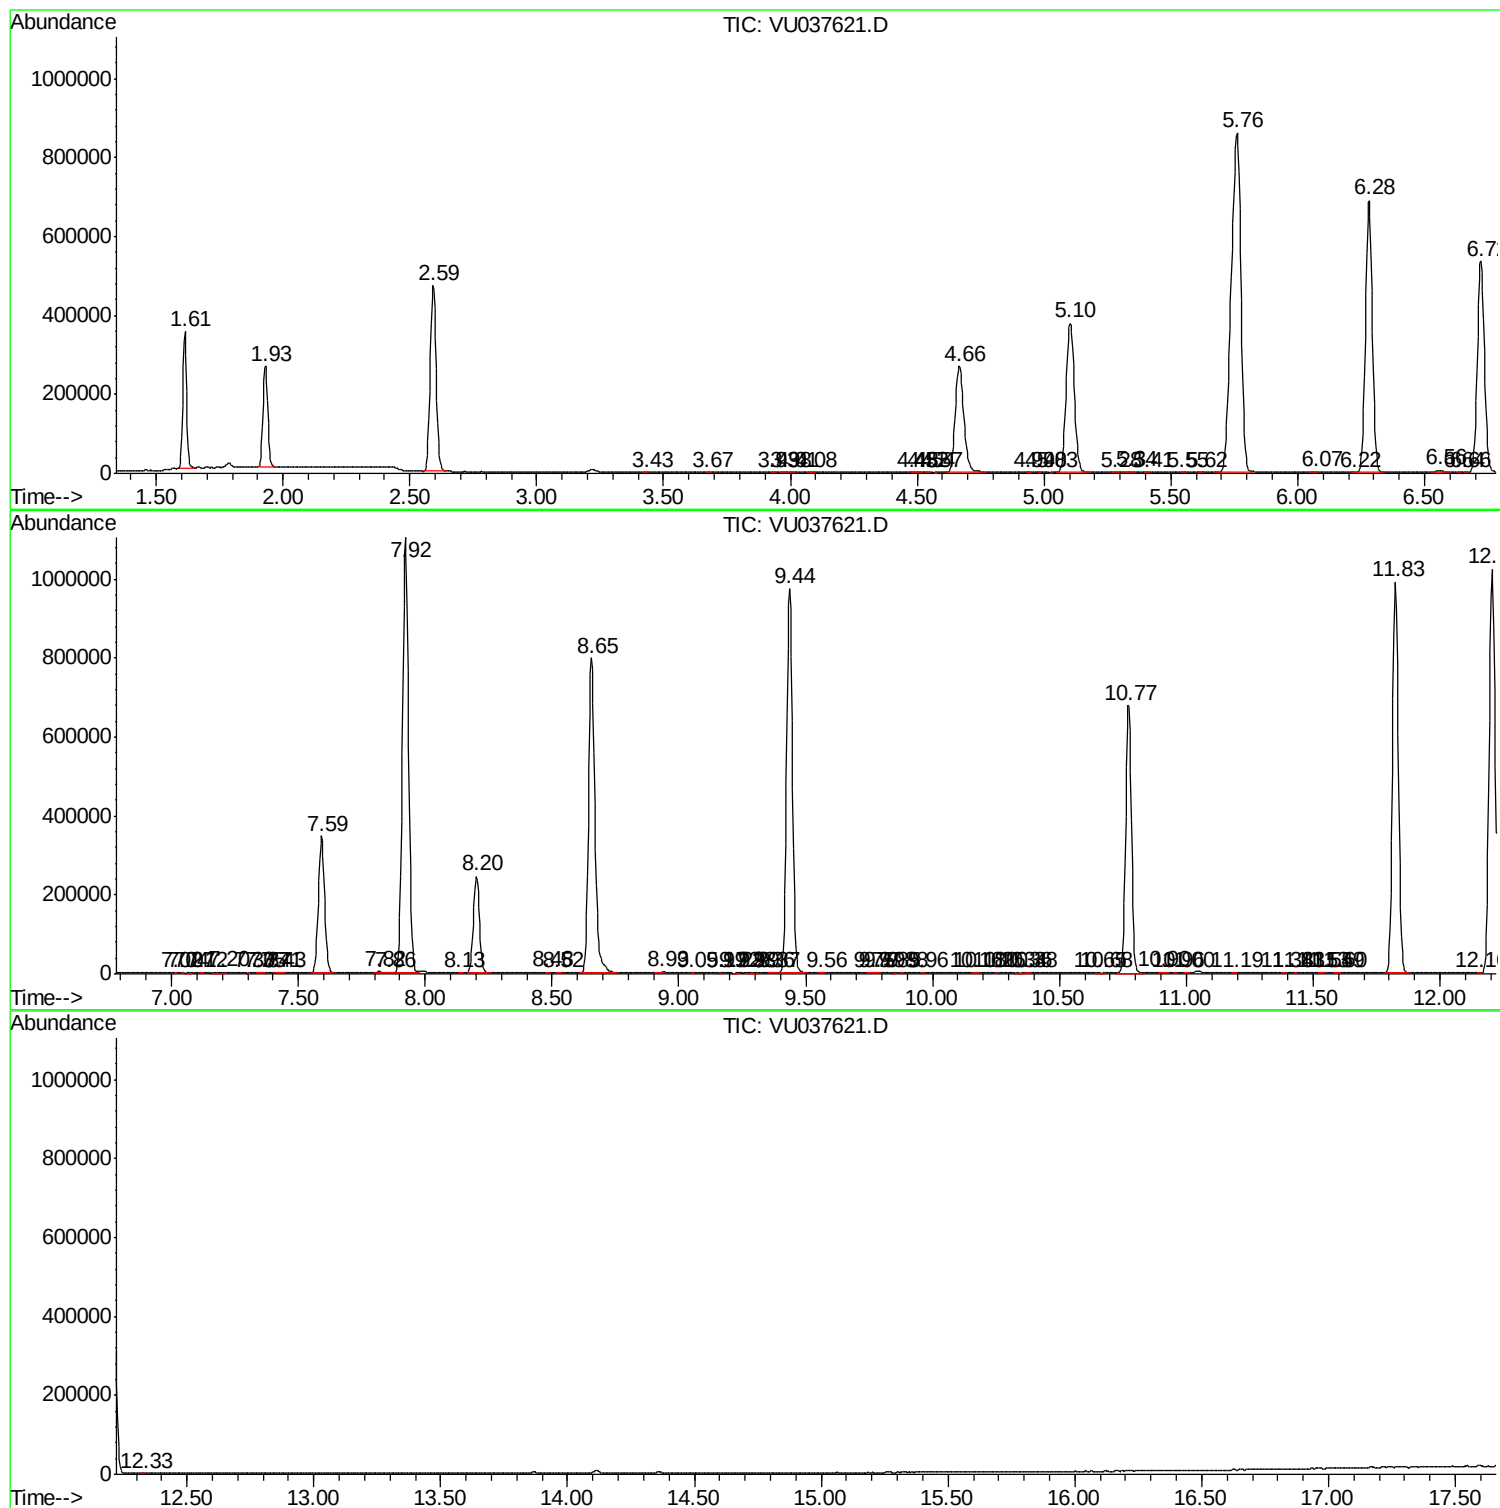

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040920\
Data File : VU037621.D
Acq On : 09 Apr 2020 16:29
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040920\
Data File : VU037621.D
Acq On : 09 Apr 2020 16:29
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc