


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040920\
 Data File : VU037606.D
 Acq On : 09 Apr 2020 08:55
 Operator : JC/MD
 Sample : BFB38
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB38

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
 Title : VOC Analysis
 Last Update : Thu Apr 09 10:11:14 2020

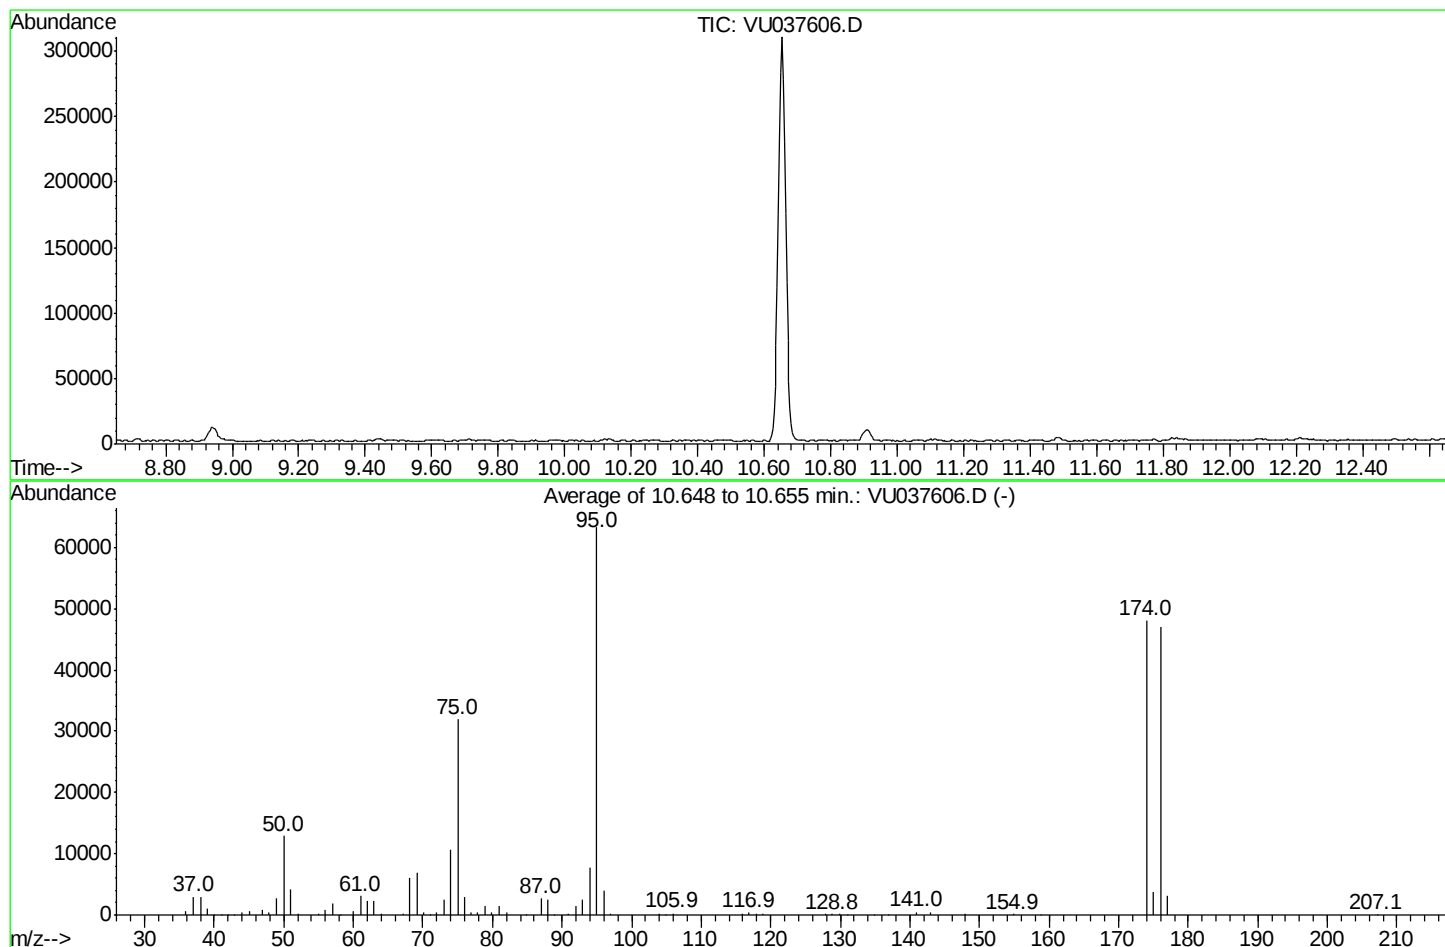

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	12920	PASS
75	95	30	80	50.4	31869	PASS
95	95	100	100	100.0	63261	PASS
96	95	5	9	6.2	3913	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.8	47968	PASS
175	174	5	9	7.8	3764	PASS
176	174	95	101	98.1	47053	PASS
177	176	5	9	6.5	3076	PASS

Scan 2883 (10.610 min): VU037606.D
BFB38

m/z	Abundance
38.90	121.0
39.90	226.0
41.10	149.0
42.90	239.0
44.00	884.0
55.10	209.0
56.00	103.0
68.00	126.0
98.00	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.90	526.0
37.00	2857.0
38.00	2781.0
39.00	1099.0
39.90	316.0
41.00	262.0
41.90	154.0
43.00	313.0
44.00	1213.0
45.00	669.0
46.90	753.0
47.90	361.0
49.00	2686.0
50.00	12600.0
51.00	3931.0
52.00	200.0
55.10	388.0
56.00	918.0
57.00	1684.0
59.90	553.0
61.00	2862.0
62.00	2236.0
63.00	2220.0
63.90	210.0
67.10	294.0
68.00	5845.0
69.10	6726.0
70.00	455.0
71.90	427.0
73.10	2450.0
74.00	10330.0
75.00	30240.0
76.00	3025.0
76.90	407.0
77.90	351.0
79.00	1485.0
79.80	459.0
81.00	1302.0
82.00	297.0
87.00	2347.0
88.00	2325.0
88.80	114.0
90.90	345.0
92.00	1444.0
93.00	2256.0
94.00	7510.0
95.00	60080.0
96.00	3631.0
97.00	181.0
104.00	200.0
104.90	100.0
105.90	249.0
115.80	151.0
116.90	384.0
117.80	147.0
118.90	260.0
127.90	148.0
128.80	166.0
129.90	204.0
130.90	125.0
136.90	152.0
141.00	473.0
142.90	377.0
147.90	146.0
154.80	136.0
174.00	44256.0
175.00	3551.0
176.00	43176.0
177.00	2740.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
36.00	566.0
37.00	3096.0
38.00	2996.0
39.00	1283.0
40.00	312.0
41.00	275.0
41.90	119.0
43.00	310.0
43.90	1182.0
45.00	752.0
47.00	773.0
47.90	426.0
49.00	2819.0
50.00	13373.0
51.00	4389.0
52.10	195.0
55.00	351.0
56.00	1030.0
57.00	1862.0
58.20	100.0
59.90	617.0
61.00	3202.0
62.10	2474.0
63.00	2418.0
64.00	227.0
67.10	306.0
68.00	6514.0
69.10	7199.0
70.10	545.0
71.90	404.0
73.00	2664.0
74.00	11025.0
75.00	32752.0
76.00	3058.0
76.90	485.0
77.90	389.0
78.90	1603.0
79.80	523.0
81.00	1486.0
82.00	369.0
84.80	100.0
87.00	2698.0
87.90	2701.0
90.90	328.0
92.00	1458.0
93.00	2512.0
94.00	7971.0
95.00	65440.0
96.00	3992.0
97.00	188.0
103.90	234.0
105.90	298.0
115.90	224.0
116.90	382.0
117.80	183.0
118.90	312.0
127.80	147.0
128.90	230.0
129.90	174.0
130.90	109.0
136.90	138.0
141.00	528.0
142.90	464.0
147.90	152.0
154.90	170.0
158.80	115.0
174.00	49520.0
175.00	3883.0
176.00	48632.0
177.00	3159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
36.00	514.0
37.00	2987.0
38.00	2907.0
39.00	1246.0
40.00	298.0
41.00	245.0
43.00	267.0
43.90	1221.0
45.00	657.0
47.10	771.0
47.90	435.0
49.00	2714.0
50.00	12787.0
51.00	4352.0
52.10	174.0
55.00	271.0
56.10	1067.0
57.00	1935.0
59.90	559.0
61.00	3154.0
62.10	2493.0
63.00	2389.0
64.10	209.0
67.10	258.0
68.00	6520.0
69.10	6865.0
70.10	526.0
71.00	116.0
71.90	326.0
73.00	2709.0
74.00	10671.0
75.00	32616.0
76.00	2844.0
76.90	469.0
77.80	377.0
78.90	1615.0
79.80	509.0
81.00	1556.0
82.00	397.0
86.90	2833.0
87.90	2671.0
90.90	282.0
92.00	1460.0
93.00	2494.0
94.00	7469.0
95.00	64264.0
96.00	4116.0
97.00	158.0
103.90	236.0
105.90	301.0
115.90	268.0
116.90	401.0
117.90	193.0
118.90	305.0
127.80	179.0
128.90	233.0
129.90	185.0
131.00	101.0
134.90	115.0
141.00	495.0
142.90	555.0
148.00	158.0
155.00	218.0
174.00	50128.0
175.00	3858.0
176.00	49352.0
177.00	3330.0
207.10	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38