

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040921\
 Data File : VU043002.D
 Acq On : 09 Apr 2021 15:09
 Operator : SY/MD
 Sample : M1977-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GWBR1-175-200-040721

Quant Time: Apr 09 16:25:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U040921W.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 09 09:26:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.382	168	123502	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.256	114	201371	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.423	117	196085	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.819	152	97089	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.710	65	102110	50.58	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.16%	
35) Dibromofluoromethane	5.298	113	71954	48.93	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.86%	
50) Toluene-d8	7.906	98	257715	48.65	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.30%	
62) 4-Bromofluorobenzene	10.639	95	94783	43.80	ug/l	0.00
Spiked Amount 50.000			Recovery	=	87.60%	
Target Compounds					Qvalue	
3) Chloromethane	1.527	50	632	Below Cal	#	43
4) Vinyl Chloride	1.607	62	298	0.23	ug/l #	1
6) Chloroethane	1.932	64	446	0.46	ug/l #	85
11) Tert butyl alcohol	3.186	59	946	1.72	ug/l #	71
12) 1,1-Dichloroethene	2.588	96	49410	43.43	ug/l	93
16) Acetone	2.629	43	3337	2.95	ug/l	96
20) Methylene Chloride	3.044	84	615	0.42	ug/l #	90
21) trans-1,2-Dichloroethene	3.363	96	851	0.66	ug/l	96
24) 1,1-Dichloroethane	3.880	63	7214	2.83	ug/l	100
25) 2-Butanone	4.713	43	1050	0.58	ug/l #	67
27) cis-1,2-Dichloroethene	4.674	96	20372	14.10	ug/l	89
29) Tetrahydrofuran	5.057	42	1478	1.28	ug/l #	80
30) Chloroform	5.099	83	2072	0.75	ug/l	95
31) Cyclohexane	5.385	56	3157	1.30	ug/l #	16
36) 1,1-Dichloropropene	5.382	75	10431	5.27	ug/l #	51
37) Ethyl Acetate	4.713	43	1050	0.31	ug/l #	72
38) Carbon Tetrachloride	5.385	117	12660	5.81	ug/l #	15
39) Methylcyclohexane	6.546	83	552	0.25	ug/l #	1
40) Benzene	5.784	78	1374	0.24	ug/l	93
41) Methacrylonitrile	5.060	41	929	0.51	ug/l #	51
42) 1,2-Dichloroethane	5.803	62	3007	1.17	ug/l	84
44) Trichloroethene	6.549	130	50469	33.79	ug/l	95
49) 1,4-Dioxane	6.970	88	681	32.58	ug/l #	83
51) 4-Methyl-2-Pentanone	7.800	43	982	9.82	ug/l #	88
52) Toluene	7.977	92	126215	34.76	ug/l	99
53) t-1,3-Dichloropropene	7.973	75	1596	2.82	ug/l #	1
59) 2-Hexanone	8.700	43	750	8.18	ug/l	65
76) 1,2,3-Trichloropropane	10.639	75	53700	19.39	ug/l #	40
81) trans-1,4-Dichloro-2-b...	10.639	75	53700	54.02	ug/l #	5
89) n-Butylbenzene	12.218	91	194	1.73	ug/l #	65
95) Naphthalene	14.095	128	1517	3.41	ug/l #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040921\
Data File : VU043002.D
Acq On : 09 Apr 2021 15:09
Operator : SY/MD
Sample : M1977-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721

Quant Time: Apr 09 16:25:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U040921W.M
Quant Title : SW846 8260
QLast Update : Fri Apr 09 09:26:47 2021
Response via : Initial Calibration




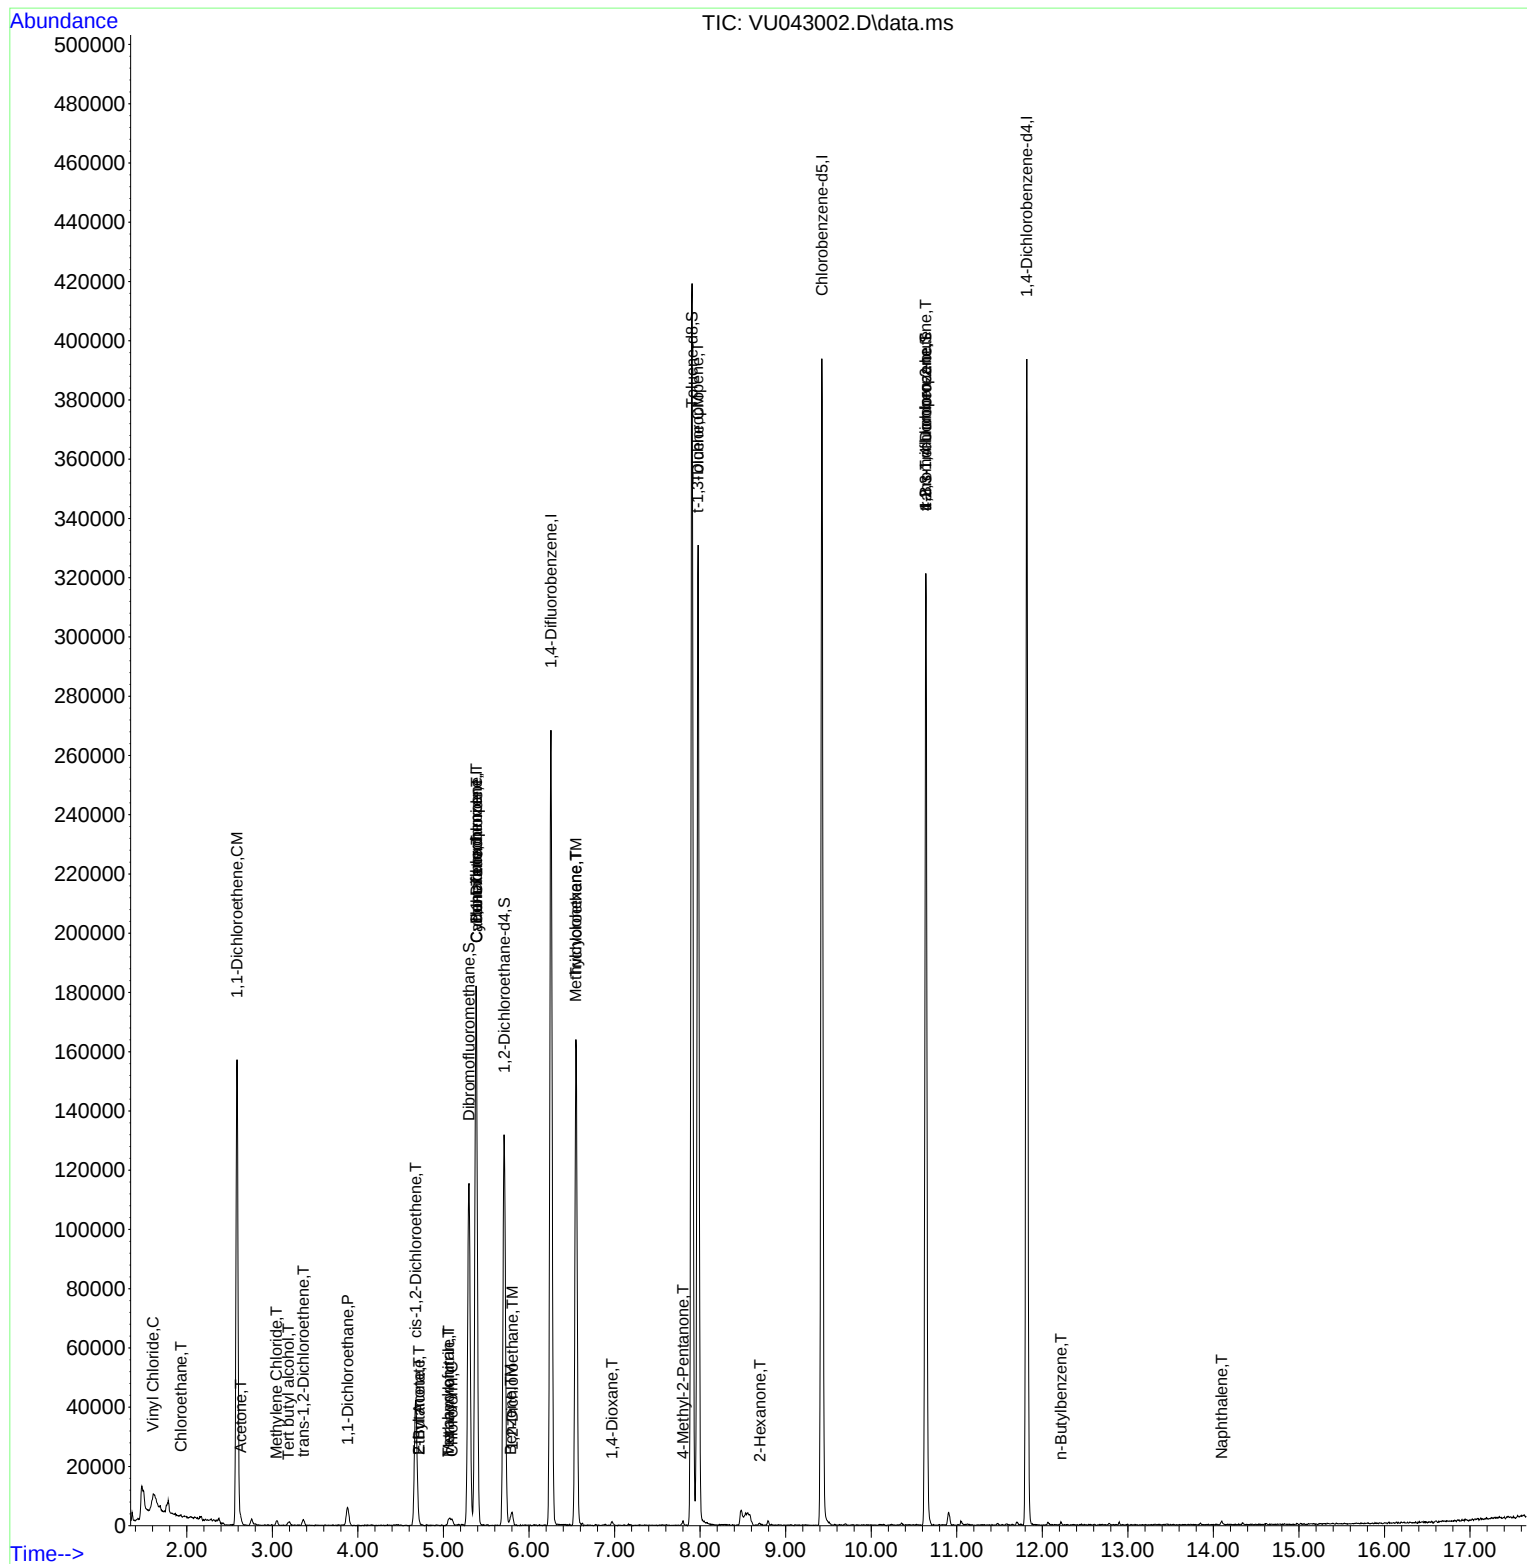


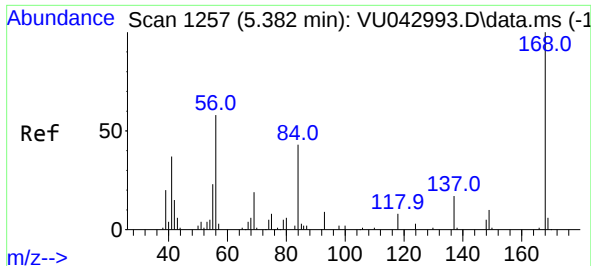

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09




Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721


Tgt Ion:168 Resp: 123502
Ion Ratio Lower Upper
168 100
99 57.5 47.5 71.3

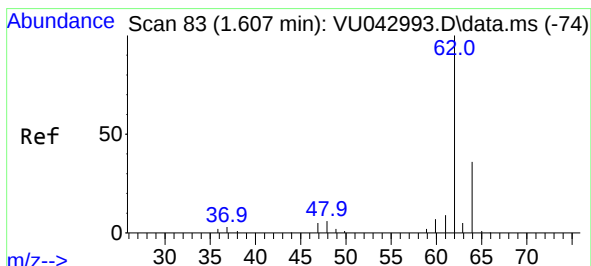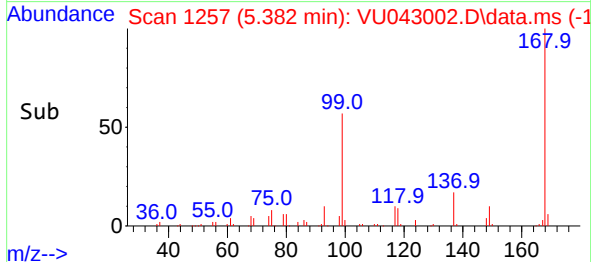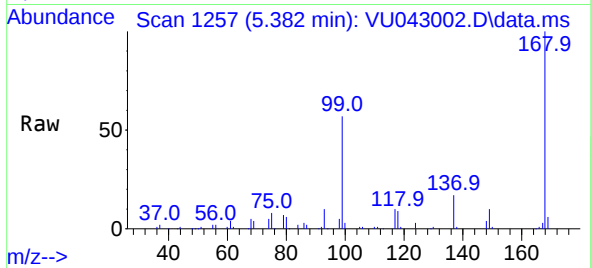

#4
Vinyl Chloride
Concen: 0.23 ug/l
RT: 1.607 min Scan# 83
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 62 Resp: 298
Ion Ratio Lower Upper
62 100
64 417.6 28.9 43.3#


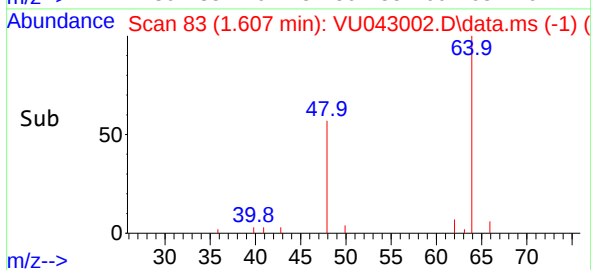

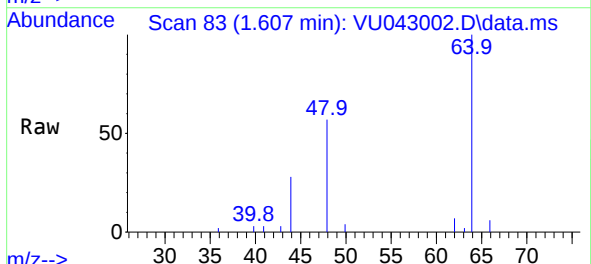




#6
Chloroethane
Concen: 0.46 ug/l
RT: 1.932 min Scan# 184
Delta R.T. 0.007 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09




Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721


Tgt Ion: 64 Resp: 446
Ion Ratio Lower Upper
64 100
66 24.8 26.9 40.3#



#11
Tert butyl alcohol
Concen: 1.72 ug/l
RT: 3.186 min Scan# 574
Delta R.T. -0.019 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 59 Resp: 946
Ion Ratio Lower Upper
59 100
57 0.0 8.6 13.0#



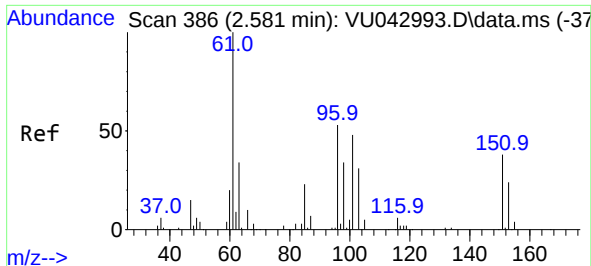

#12

1,1-Dichloroethene

Concen: 43.43 ug/l

RT: 2.588 min Scan# 388

Delta R.T. 0.007 min

Lab File: VU043002.D

Acq: 09 Apr 2021 15:09


Tgt Ion: 96 Resp: 49410

Ion Ratio Lower Upper




96 100

61 176.0 150.2 225.2

98 61.2 51.6 77.4

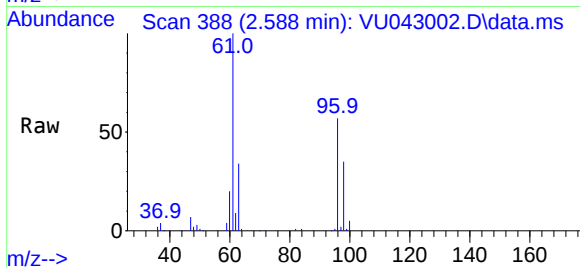

Abundance

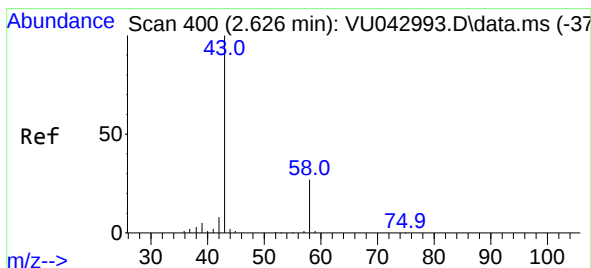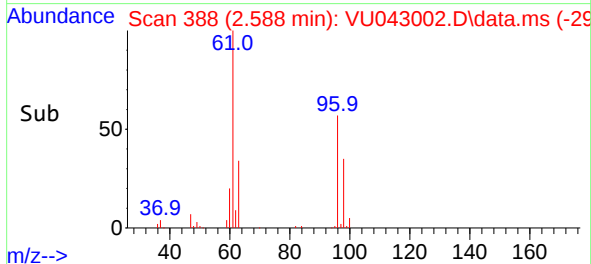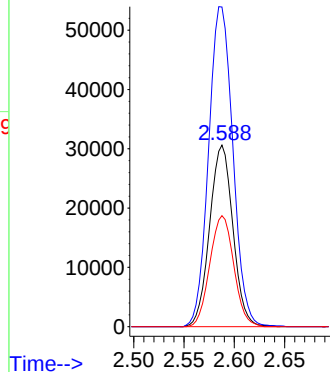

#16

Acetone

Concen: 2.95 ug/l

RT: 2.629 min Scan# 401

Delta R.T. 0.003 min

Lab File: VU043002.D


Acq: 09 Apr 2021 15:09

Tgt Ion: 43 Resp: 3337



Ion Ratio Lower Upper


43 100

58 24.5 21.4 32.0

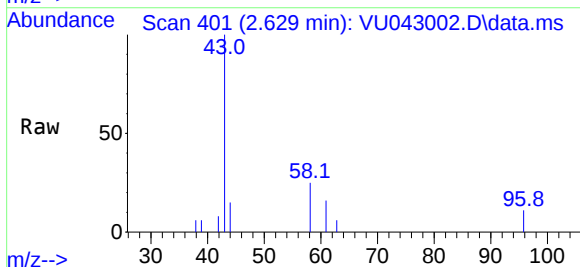


Abundance

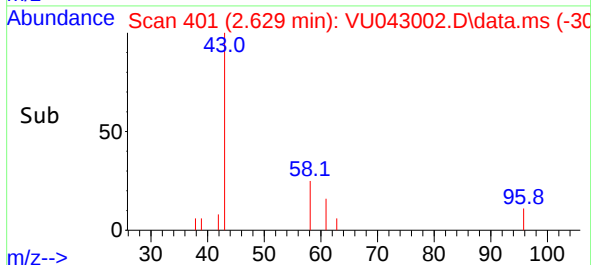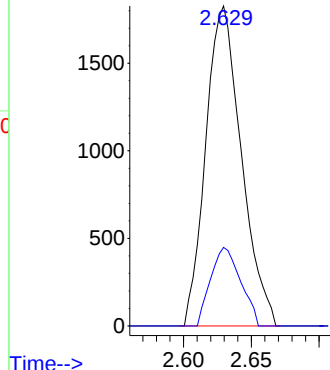






#20
Methylene Chloride
Concen: 0.42 ug/l
RT: 3.044 min Scan# 530
Delta R.T. -0.006 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721




Tgt Ion: 84 Resp: 615

Ion	Ratio	Lower	Upper
84	100		
49	128.5	116.1	174.1
51	34.4	35.1	52.7#
86	65.9	52.3	78.5






#21
trans-1,2-Dichloroethene
Concen: 0.66 ug/l
RT: 3.363 min Scan# 629
Delta R.T. 0.007 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09



Tgt Ion: 96 Resp: 851


Ion	Ratio	Lower	Upper
96	100		
61	148.0	119.1	178.7
98	53.0	48.8	73.2

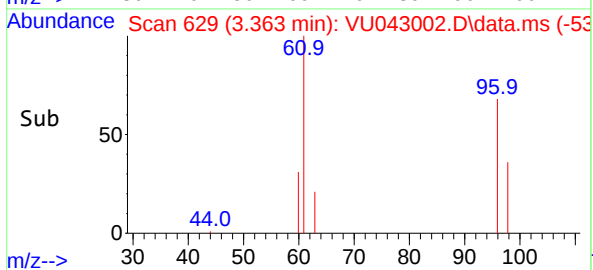






#24
1,1-Dichloroethane
Concen: 2.83 ug/l
RT: 3.880 min Scan# 790
Delta R.T. 0.003 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721







Tgt Ion: 63 Resp: 7214
Ion Ratio Lower Upper
63 100
98 6.2 3.1 9.3
100 3.8 1.8 5.4

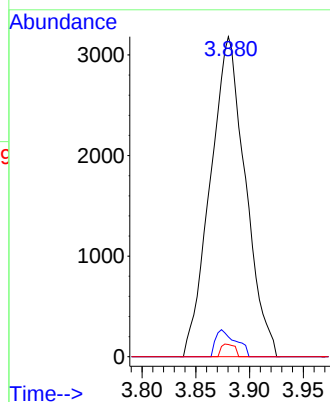

#25
2-Butanone
Concen: 0.58 ug/l
RT: 4.713 min Scan# 1049
Delta R.T. 0.007 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 43 Resp: 1050
Ion Ratio Lower Upper
43 100
72 37.7 17.4 26.2#

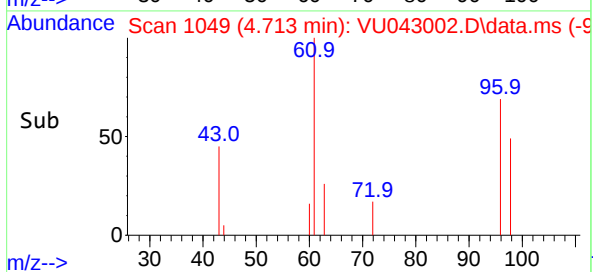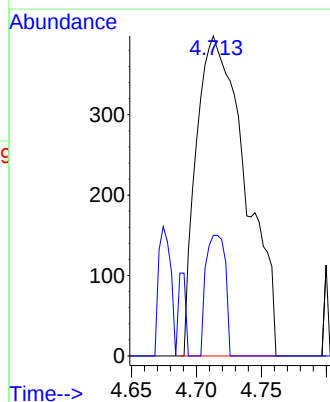







#27
cis-1,2-Dichloroethene
Concen: 14.10 ug/l
RT: 4.674 min Scan# 1037
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721

Tgt Ion: 96 Resp: 20372




Ion	Ratio	Lower	Upper
96	100		
61	144.4	0.0	327.0
98	64.5	0.0	127.4

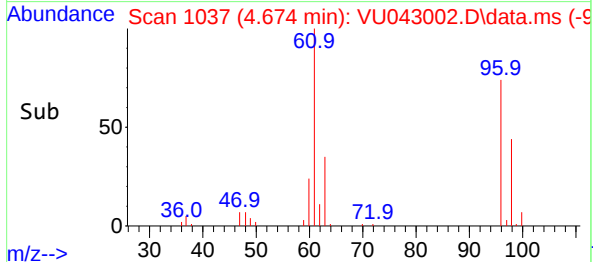


#29
Tetrahydrofuran
Concen: 1.28 ug/l
RT: 5.057 min Scan# 1156
Delta R.T. 0.003 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 42 Resp: 1478

Ion	Ratio	Lower	Upper
42	100		
72	21.5	30.1	45.1#
71	27.9	28.1	42.1#

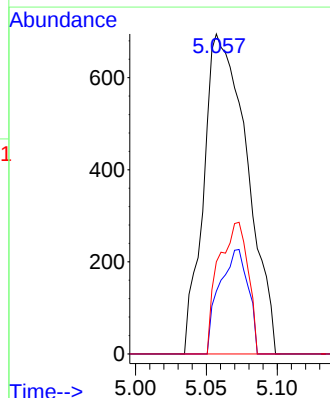







#30

Chloroform
Concen: 0.75 ug/l
RT: 5.099 min Scan# 1169
Delta R.T. 0.003 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721




Tgt Ion: 83 Resp: 2072
Ion Ratio Lower Upper
83 100
85 67.2 50.8 76.2




#31

Cyclohexane
Concen: 1.30 ug/l
RT: 5.385 min Scan# 1258
Delta R.T. -0.009 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 56 Resp: 3157
Ion Ratio Lower Upper
56 100
69 161.0 23.9 35.9#
84 92.5 59.8 89.6#

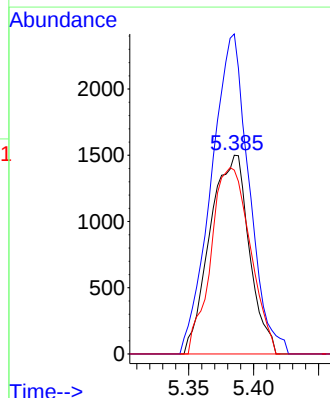







#33

1,2-Dichloroethane-d4
Concen: 50.58 ug/l
RT: 5.710 min Scan# 1359
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721




Tgt Ion: 65 Resp: 102110
Ion Ratio Lower Upper
65 100
67 50.1 0.0 98.6




#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.256 min Scan# 1529
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 114 Resp: 201371
Ion Ratio Lower Upper
114 100
63 23.4 0.0 48.0
88 16.6 0.0 32.6


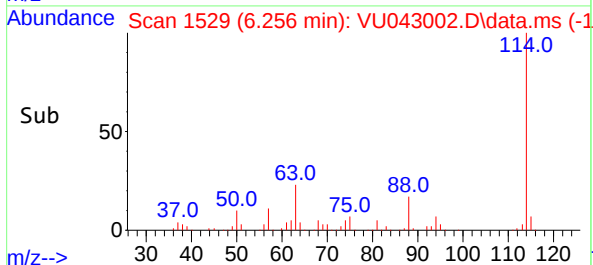
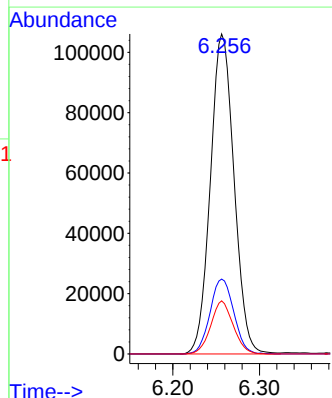
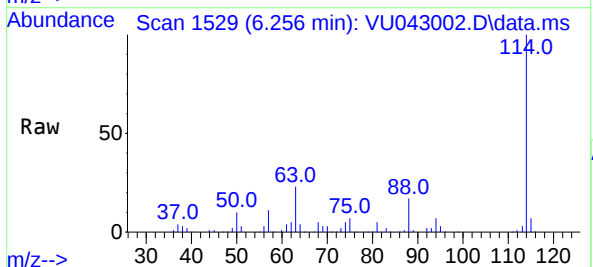




#35
Dibromofluoromethane
Concen: 48.93 ug/l
RT: 5.298 min Scan# 1231
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09




Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721


Tgt Ion:	113	Resp:	71954
Ion	Ratio	Lower	Upper
113	100		
111	101.1	81.7	122.5
192	20.8	17.1	25.7



#36
1,1-Dichloropropene
Concen: 5.27 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.151 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion:	75	Resp:	10431
Ion	Ratio	Lower	Upper
75	100		
110	8.5	16.3	48.8#
77	0.0	23.8	35.6#

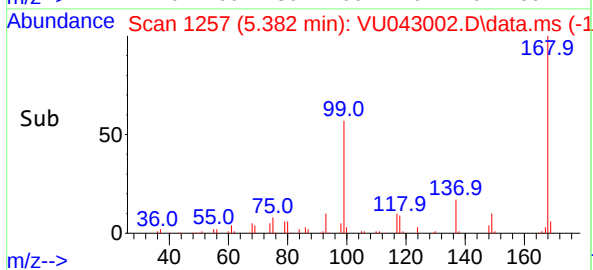



#37

Ethyl Acetate

Concen: 0.31 ug/l

RT: 4.713 min Scan# 1049





Delta R.T. -0.093 min

Lab File: VU043002.D

Acq: 09 Apr 2021 15:09

Tgt Ion: 43	Resp: 1050
Ion Ratio	Lower Upper
43 100	
61 0.0	9.6 14.4#
70 0.0	6.6 9.8#

Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721



#38

Carbon Tetrachloride

Concen: 5.81 ug/l




RT: 5.385 min Scan# 1258


Delta R.T. -0.148 min

Lab File: VU043002.D

Acq: 09 Apr 2021 15:09

Tgt Ion: 117	Resp: 12660
Ion Ratio	Lower Upper
117 100	
119 6.1	79.6 119.4#
121 0.0	24.1 36.1#


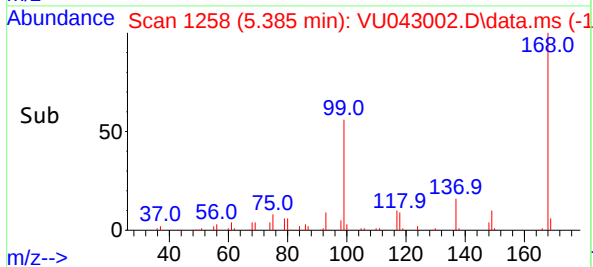

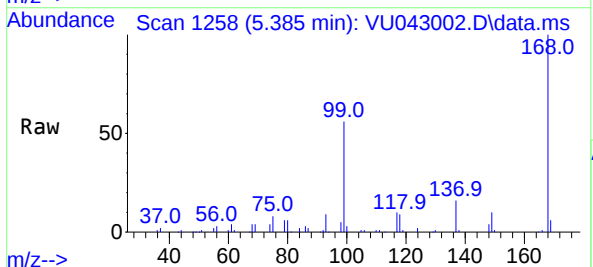




#39
Methylcyclohexane
Concen: 0.25 ug/l
RT: 6.546 min Scan# 1619
Delta R.T. -0.225 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09




Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721


Tgt Ion: 83 Resp: 552
Ion Ratio Lower Upper
83 100
55 0.0 68.6 103.0#
98 193.7 36.0 54.0#

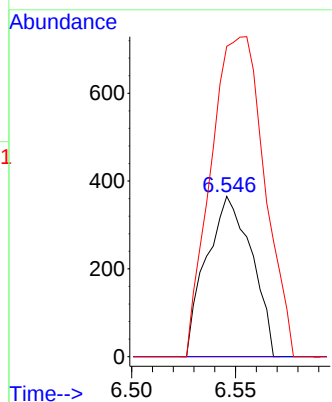

#40
Benzene
Concen: 0.24 ug/l
RT: 5.784 min Scan# 1382
Delta R.T. 0.003 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 78 Resp: 1374
Ion Ratio Lower Upper
78 100
77 21.1 19.8 29.6









#41
Methacrylonitrile
Concen: 0.51 ug/l
RT: 5.060 min Scan# 1157
Delta R.T. 0.081 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09




Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721


Tgt Ion:	41	Resp:	929
Ion	Ratio	Lower	Upper
41	100		
39	45.2	45.7	68.5#
67	0.0	48.0	72.0#
52	0.0	22.4	33.6#



#42
1,2-Dichloroethane
Concen: 1.17 ug/l
RT: 5.803 min Scan# 1388
Delta R.T. 0.003 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion:	62	Resp:	3007
Ion	Ratio	Lower	Upper
62	100		
98	1.6	0.0	14.4


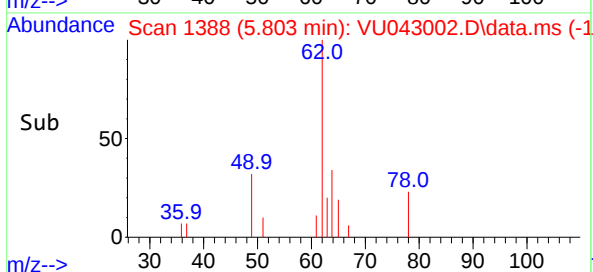






#44
Trichloroethene
Concen: 33.79 ug/l
RT: 6.549 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09




Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721


Tgt Ion:130 Resp: 50469
Ion Ratio Lower Upper
130 100
95 102.9 0.0 215.4



#49
1,4-Dioxane
Concen: 32.58 ug/l
RT: 6.970 min Scan# 1751
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 88 Resp: 681
Ion Ratio Lower Upper
88 100
43 31.3 30.8 46.2
58 88.3 57.8 86.6#


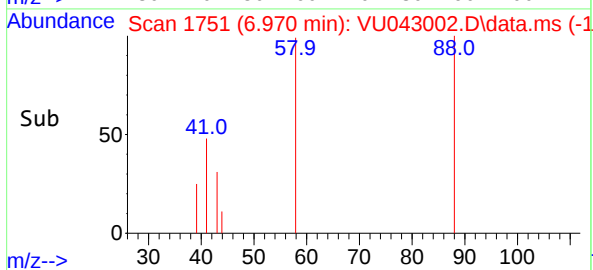






#50
Toluene-d8
Concen: 48.65 ug/l
RT: 7.906 min Scan# 2042
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09




Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721


Tgt Ion: 98 Resp: 257715
Ion Ratio Lower Upper
98 100
100 61.9 49.9 74.9

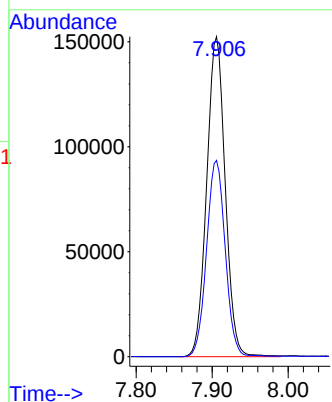

#51
4-Methyl-2-Pentanone
Concen: 9.82 ug/l
RT: 7.800 min Scan# 2009
Delta R.T. -0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 43 Resp: 982
Ion Ratio Lower Upper
43 100
58 27.4 27.7 41.5#


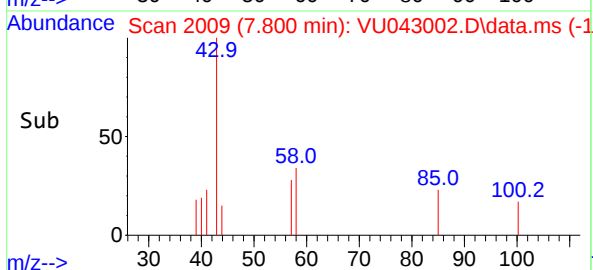






#52
Toluene
Concen: 34.76 ug/l
RT: 7.977 min Scan# 2064
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09




Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721


Tgt Ion: 92 Resp: 126215
Ion Ratio Lower Upper
92 100
91 175.7 141.1 211.7



#53
t-1,3-Dichloropropene
Concen: 2.82 ug/l
RT: 7.973 min Scan# 2063
Delta R.T. -0.244 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 75 Resp: 1596
Ion Ratio Lower Upper
75 100
77 177.7 26.5 39.7#


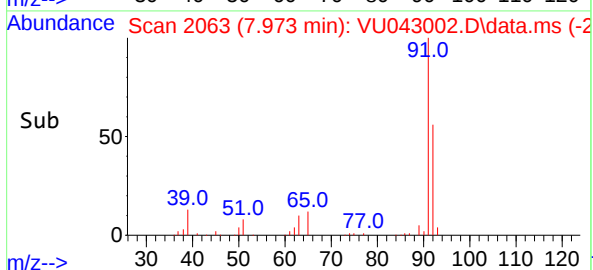






#59
2-Hexanone
Concen: 8.18 ug/l
RT: 8.700 min Scan# 2289
Delta R.T. 0.007 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09




Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721


Tgt Ion: 43 Resp: 750
Ion Ratio Lower Upper
43 100
58 24.1 23.7 71.1

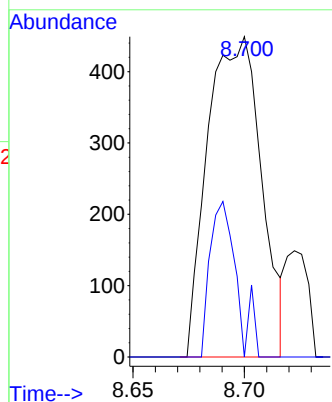

#62
4-Bromofluorobenzene
Concen: 43.80 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 95 Resp: 94783
Ion Ratio Lower Upper
95 100
174 88.3 0.0 168.8
176 85.1 0.0 164.6

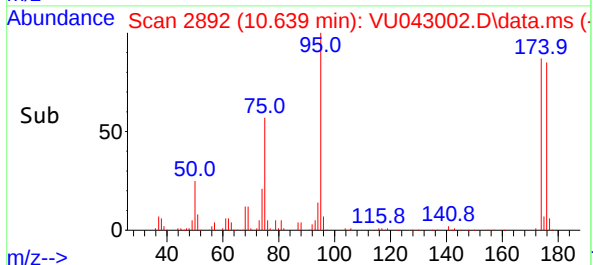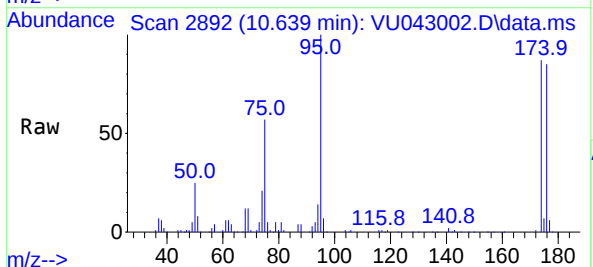







#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 9.423 min Scan# 2514
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721

Tgt Ion:117 Resp: 196085




Ion	Ratio	Lower	Upper
117	100		
82	57.1	46.5	69.7
119	33.4	25.7	38.5

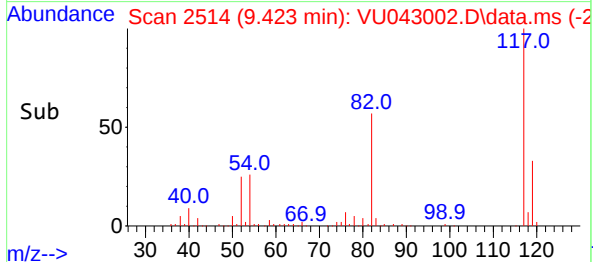


#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 11.819 min Scan# 3259
Delta R.T. -0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion:152 Resp: 97089

Ion	Ratio	Lower	Upper
152	100		
115	57.7	42.8	128.3
150	157.7	0.0	347.6



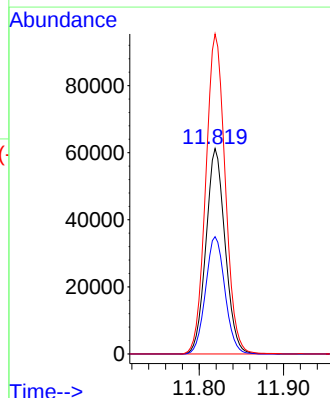



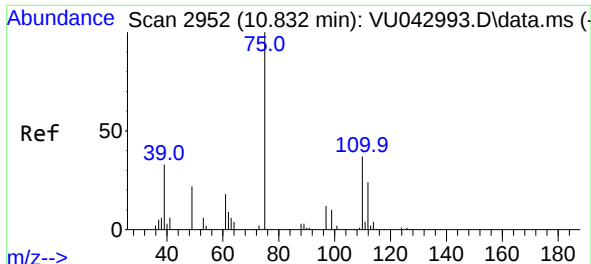

#76
1,2,3-Trichloropropane
Concen: 19.39 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.193 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09




Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721


Tgt Ion: 75 Resp: 53700
Ion Ratio Lower Upper
75 100
77 1.1 18.2 54.6#

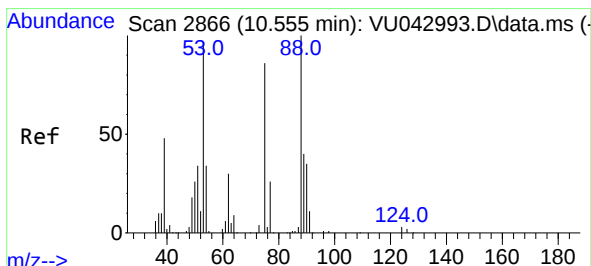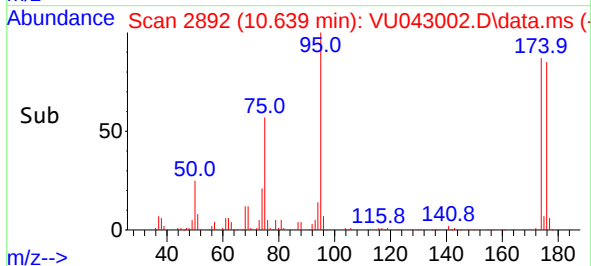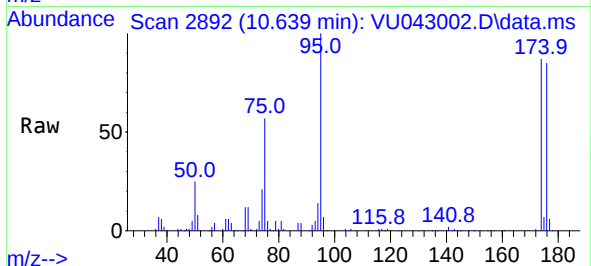

#81
trans-1,4-Dichloro-2-butene
Concen: 54.02 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.084 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 75 Resp: 53700
Ion Ratio Lower Upper
75 100
53 0.0 91.1 136.7#
89 0.0 37.1 55.7#

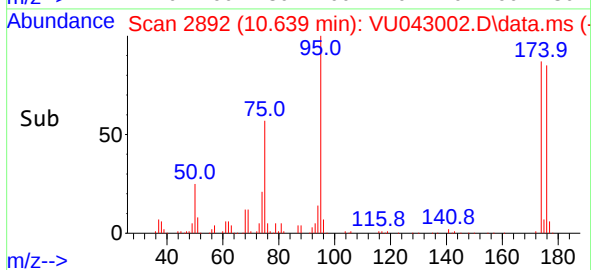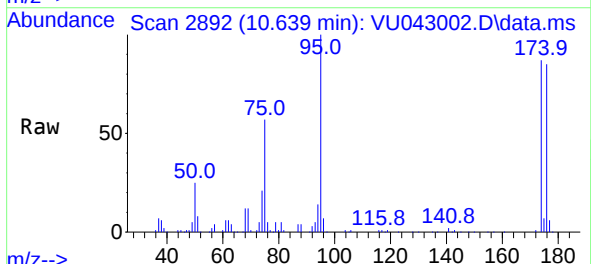




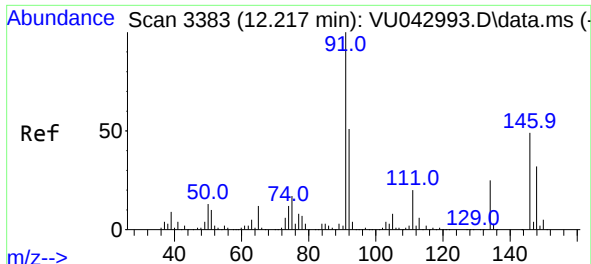


#89
n-Butylbenzene
Concen: 1.73 ug/l
RT: 12.218 min Scan# 3383
Delta R.T. 0.001 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Instrument :
MSVOA_U
ClientSampleId :
GWBR1-175-200-040721

Tgt Ion: 91 Resp: 194

Ion	Ratio	Lower	Upper
91	100		
92	32.0	25.7	77.1
134	0.0	12.2	36.4#

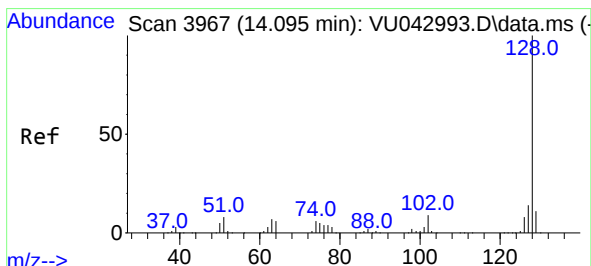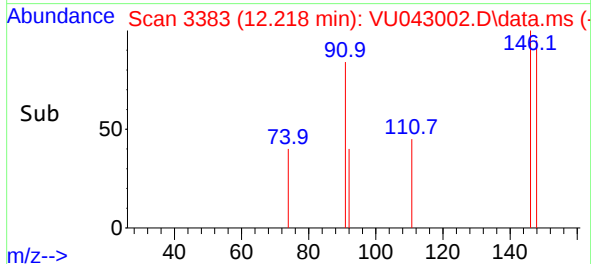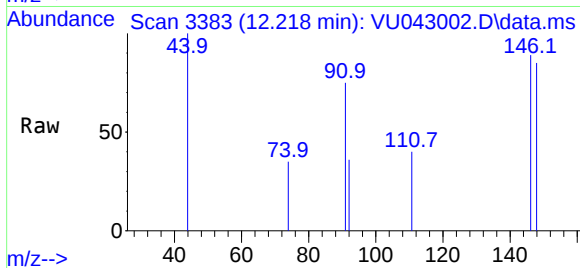

#95
Naphthalene
Concen: 3.41 ug/l
RT: 14.095 min Scan# 3967
Delta R.T. 0.000 min
Lab File: VU043002.D
Acq: 09 Apr 2021 15:09

Tgt Ion: 128 Resp: 1517

Ion	Ratio	Lower	Upper
128	100		
127	4.5	11.0	16.4#
129	3.0	8.7	13.1#

