
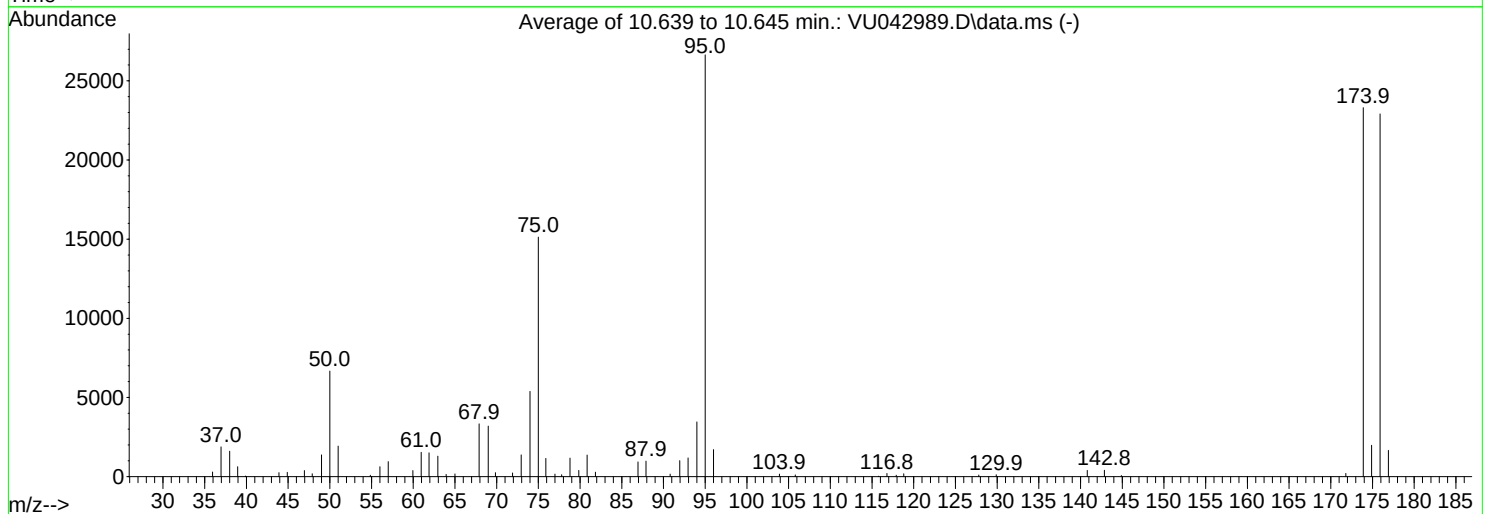


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040921\
Data File : VU042989.D
Acq On : 08 Apr 2021 16:22
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U040921W.M
Title : SW846 8260
Last Update : Fri Apr 09 09:26:47 2021

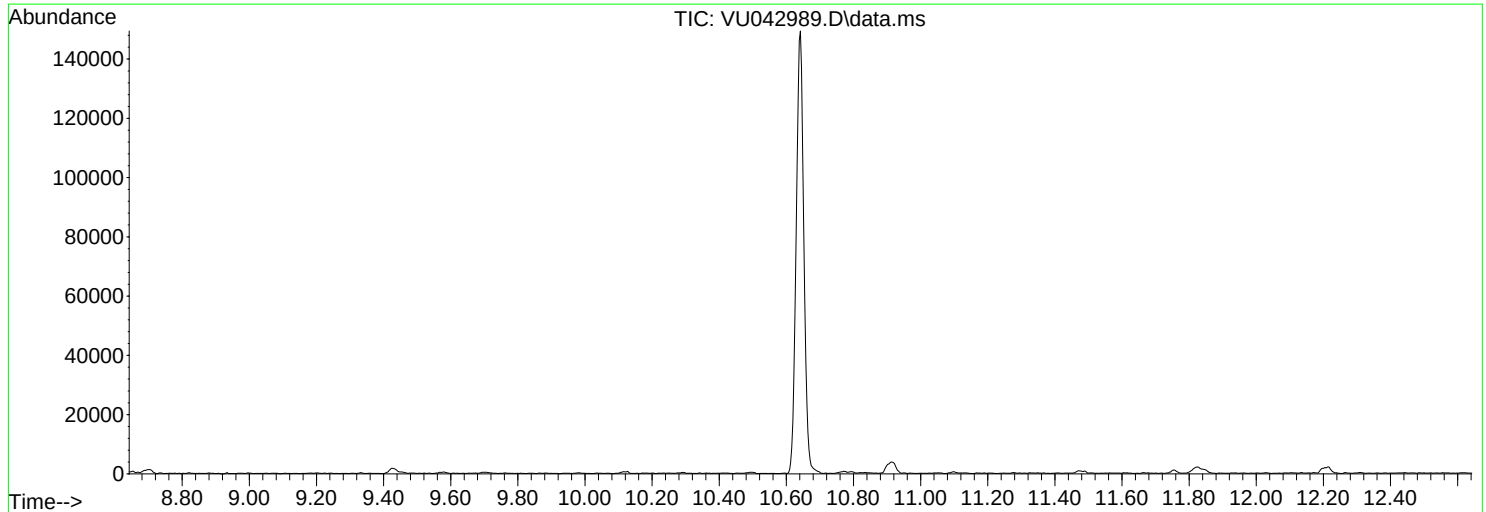

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.1	6675	PASS
75	95	30	60	56.8	15132	PASS
95	95	100	100	100.0	26643	PASS
96	95	5	9	6.4	1704	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.5	23304	PASS
175	174	5	9	8.5	1979	PASS
176	174	95	101	98.3	22912	PASS
177	176	5	9	7.2	1659	PASS