

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047874.D
 Acq On : 08 Apr 2022 18:10
 Operator : SY/MD
 Sample : N2343-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY1

Quant Time: Apr 09 02:05:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 09 01:58:44 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	255069	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	271225	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	140370	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	109876	59.403	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	118.800%	
7) Chloroethane-d5	1.916	69	94591	64.856	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	129.720%	
11) 1,1-Dichloroethene-d2	2.572	63	141834	41.912	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	83.820%	
21) 2-Butanone-d5	4.620	46	167234	105.337	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	105.340%	
24) Chloroform-d	5.067	84	197898	58.473	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	116.940%	
26) 1,2-Dichloroethane-d4	5.703	65	127517	61.433	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	122.860%	
32) Benzene-d6	5.729	84	397535	58.249	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	116.500%	
36) 1,2-Dichloropropane-d6	6.694	67	126704	60.452	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	120.900%#	
41) Toluene-d8	7.899	98	350874	52.768	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	105.540%	
43) trans-1,3-Dichloroprop...	8.179	79	53037	49.948	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	99.900%	
47) 2-Hexanone-d5	8.632	63	115085	93.796	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	93.800%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	190211	52.880	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	105.760%	
66) 1,2-Dichlorobenzene-d4	12.195	152	146595	58.701	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	117.400%	
Target Compounds						
13) Acetone	2.626	43	5655	3.828	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047874.D
Acq On : 08 Apr 2022 18:10
Operator : SY/MD
Sample : N2343-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY1

Quant Time: Apr 09 02:05:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 09 01:58:44 2022
Response via : Initial Calibration

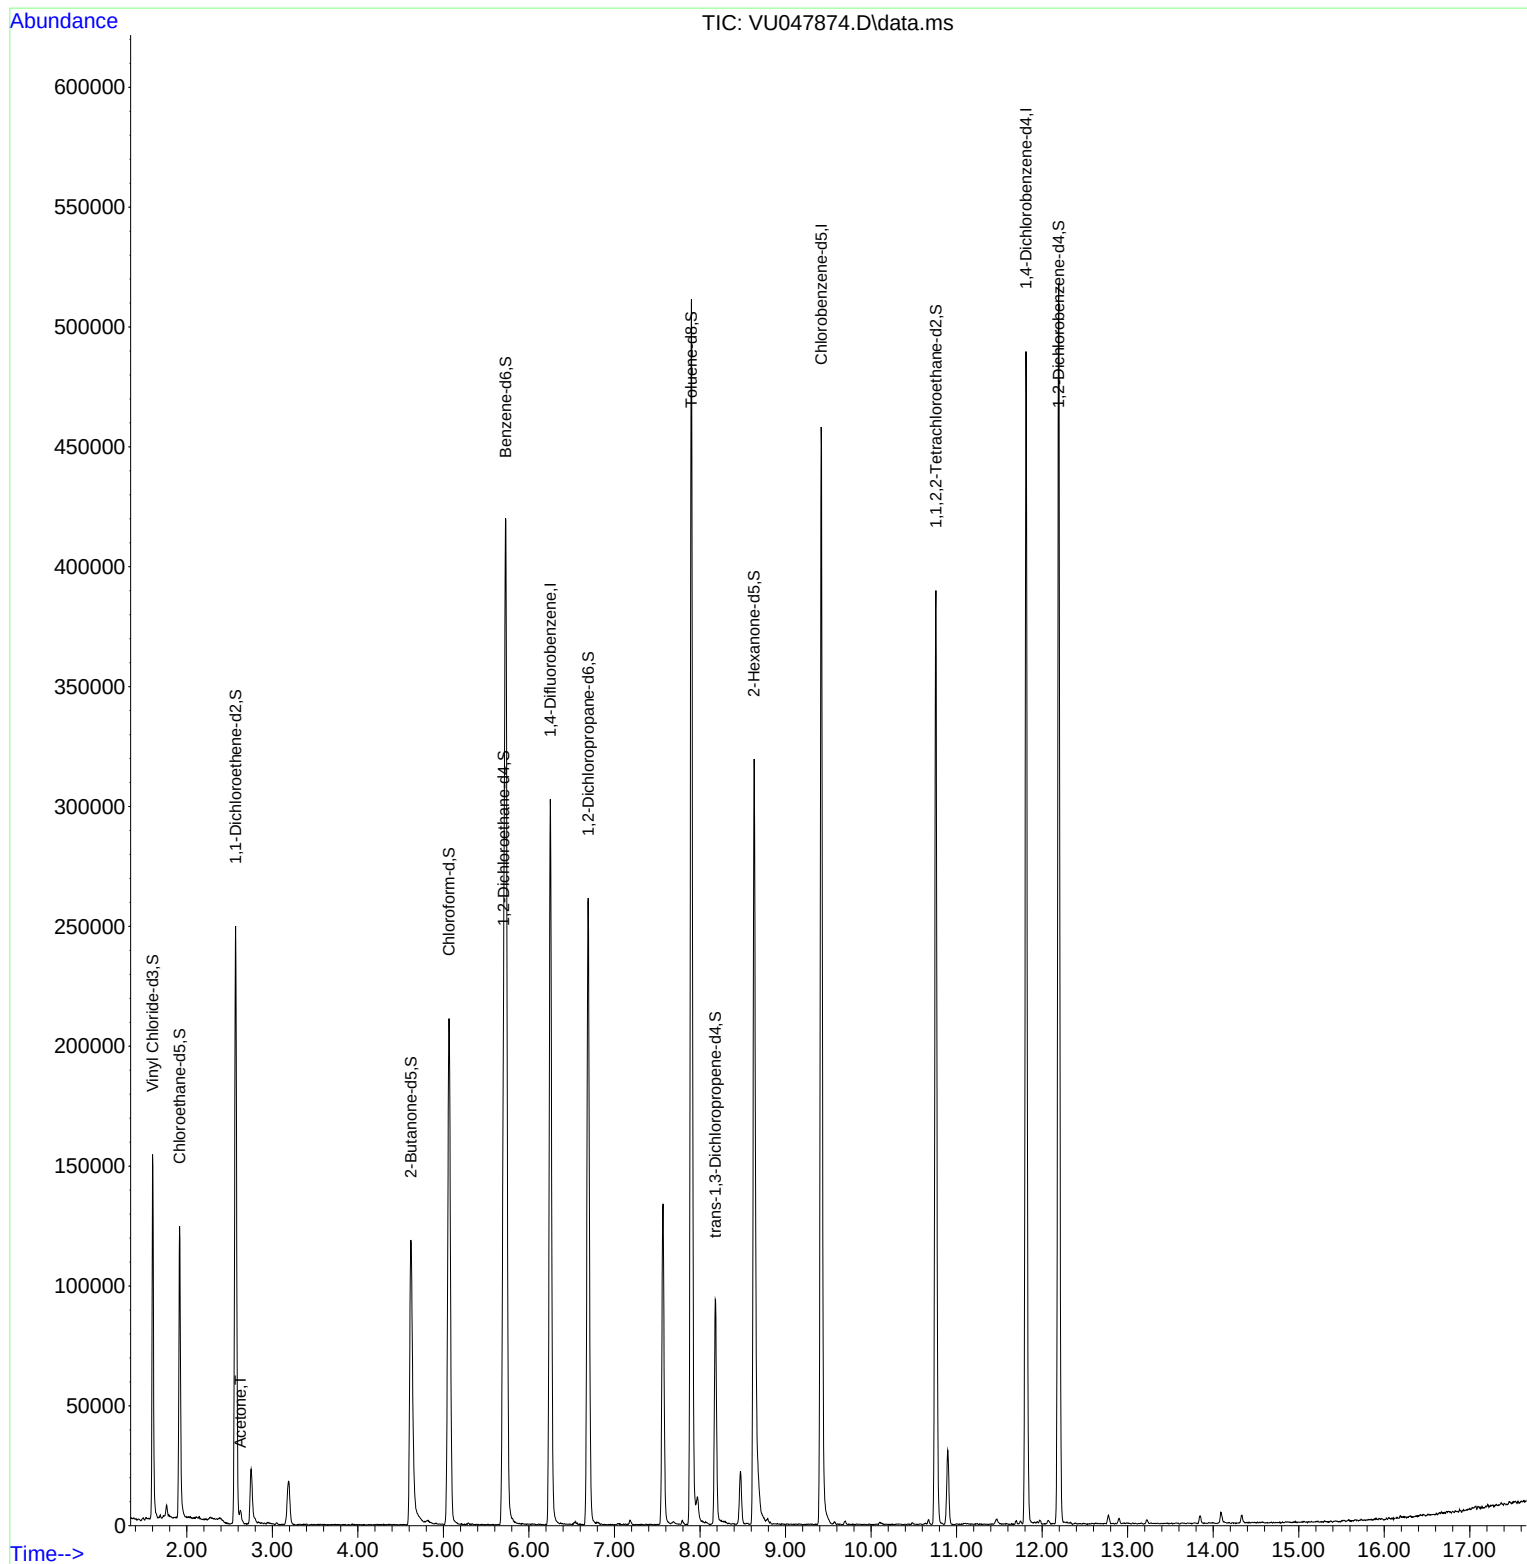

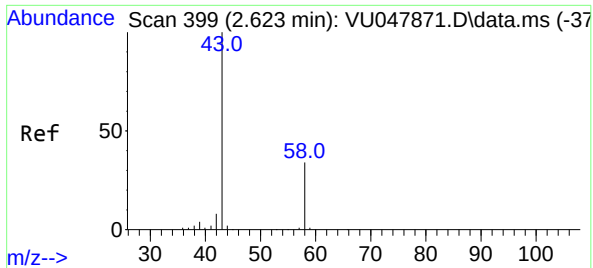

#13

Acetone

Concen: 3.828 ug/L

RT: 2.626 min Scan# 40

Delta R.T. 0.003 min

Lab File: VU047874.D

Acq: 08 Apr 2022 18:10

Instrument :
MSVOA_U
ClientSampleId :
C0HY1

Tgt Ion: 43 Resp: 5655

Ion	Ratio	Lower	Upper
43	100		
58	30.6	0.0	70.0

