

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047872.D
 Acq On : 08 Apr 2022 17:24
 Operator : SY/MD
 Sample : VU0409WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK080

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047872.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	98	rVB	158467	181810	15.03%	1.888%
2	1.916	170	179	200	rBV	125053	177476	14.67%	1.843%
3	2.571	371	383	397	rBV	262719	432900	35.78%	4.495%
4	2.800	445	454	463	rBV3	1225	2005	0.17%	0.021%
5	2.880	475	479	484	rBV2	309	357	0.03%	0.004%
6	2.948	495	500	504	rBV3	451	430	0.04%	0.004%
7	3.022	518	523	525	rBV2	396	375	0.03%	0.004%
8	3.051	525	532	543	rVB5	2212	3964	0.33%	0.041%
9	3.179	565	572	573	rBV3	988	932	0.08%	0.010%
10	3.324	611	617	619	rBV2	333	307	0.03%	0.003%
11	3.359	622	628	633	rVB4	979	1076	0.09%	0.011%
12	3.571	689	694	696	rBV	374	267	0.02%	0.003%
13	3.668	720	724	727	rVB2	333	227	0.02%	0.002%
14	3.732	739	744	746	rBV2	322	279	0.02%	0.003%
15	3.867	780	786	789	rBV3	498	493	0.04%	0.005%
16	3.915	795	801	803	rVB2	220	232	0.02%	0.002%
17	3.948	805	811	815	rBV2	414	406	0.03%	0.004%
18	4.118	860	864	869	rVB2	381	274	0.02%	0.003%
19	4.157	869	876	877	rBV	259	274	0.02%	0.003%
20	4.272	910	912	916	rVB3	378	261	0.02%	0.003%
21	4.443	960	965	967	rBV2	318	265	0.02%	0.003%
22	4.620	1005	1020	1063	rBV	124412	306346	25.32%	3.181%
23	5.067	1140	1159	1187	rBV	224538	490257	40.52%	5.091%
24	5.288	1224	1228	1231	rBV3	576	595	0.05%	0.006%
25	5.378	1253	1256	1257	rVV2	422	284	0.02%	0.003%
26	5.398	1260	1262	1265	rVV	419	254	0.02%	0.003%
27	5.533	1301	1304	1309	rVV2	455	328	0.03%	0.003%
28	5.729	1342	1365	1393	rBV2	445223	1209876	100.00%	12.564%
29	6.115	1480	1485	1488	rBV3	493	486	0.04%	0.005%
30	6.250	1510	1527	1552	rBV	358650	682427	56.40%	7.087%
31	6.539	1608	1617	1625	rVV6	1611	3165	0.26%	0.033%
32	6.578	1625	1629	1632	rVB3	466	351	0.03%	0.004%
33	6.597	1632	1635	1639	rBV2	352	263	0.02%	0.003%
34	6.693	1650	1665	1686	rBV	278258	541433	44.75%	5.623%
35	6.809	1698	1701	1706	rVB5	1151	978	0.08%	0.010%
36	7.047	1767	1775	1778	rBV3	410	600	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047872.D
 Acq On : 08 Apr 2022 17:24
 Operator : SY/MD
 Sample : VU0409WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK080

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.185	1811	1818	1828	rVB3	1917	3050	0.25%	0.032%
38	7.282	1844	1848	1850	rBV	436	332	0.03%	0.003%
39	7.349	1864	1869	1873	rVV2	345	331	0.03%	0.003%
40	7.568	1924	1937	1956	rBV	144991	256349	21.19%	2.662%
41	7.690	1967	1975	1983	rVB4	1198	1722	0.14%	0.018%
42	7.793	1999	2007	2016	rBV5	2942	4816	0.40%	0.050%
43	7.899	2026	2040	2056	rBV	544356	948856	78.43%	9.853%
44	8.179	2115	2127	2147	rBV	100718	175745	14.53%	1.825%
45	8.398	2193	2195	2199	rVB3	416	284	0.02%	0.003%
46	8.449	2206	2211	2215	rBV4	415	312	0.03%	0.003%
47	8.472	2215	2218	2223	rBV2	336	300	0.02%	0.003%
48	8.555	2241	2244	2249	rBV3	821	694	0.06%	0.007%
49	8.632	2256	2268	2317	rVV	357810	685150	56.63%	7.115%
50	8.947	2361	2366	2369	rBV2	357	380	0.03%	0.004%
51	8.986	2373	2378	2381	rBV3	302	325	0.03%	0.003%
52	9.079	2403	2407	2411	rBV2	295	290	0.02%	0.003%
53	9.417	2495	2512	2547	rBV	537272	917392	75.83%	9.527%
54	9.697	2592	2599	2611	rBV3	1953	2847	0.24%	0.030%
55	9.873	2648	2654	2658	rVV2	344	315	0.03%	0.003%
56	9.896	2658	2661	2666	rVB2	245	234	0.02%	0.002%
57	9.931	2669	2672	2676	rBV	358	257	0.02%	0.003%
58	9.999	2690	2693	2697	rBV3	313	274	0.02%	0.003%
59	10.111	2720	2728	2738	rVV7	1836	3490	0.29%	0.036%
60	10.166	2742	2745	2748	rVV2	326	274	0.02%	0.003%
61	10.397	2814	2817	2822	rVB2	273	236	0.02%	0.002%
62	10.491	2837	2846	2852	rBV4	1449	2141	0.18%	0.022%
63	10.600	2874	2880	2881	rBV	332	276	0.02%	0.003%
64	10.639	2885	2892	2897	rBV4	1720	2731	0.23%	0.028%
65	10.758	2916	2929	2946	rVV	413749	670885	55.45%	6.967%
66	10.828	2947	2951	2958	rVB4	1520	1746	0.14%	0.018%
67	11.021	3007	3011	3017	rVB3	312	310	0.03%	0.003%
68	11.089	3028	3032	3039	rVV2	1374	1472	0.12%	0.015%
69	11.243	3078	3080	3088	rVB	469	468	0.04%	0.005%
70	11.291	3088	3095	3096	rBV2	520	600	0.05%	0.006%
71	11.340	3103	3110	3116	rBV3	354	475	0.04%	0.005%
72	11.465	3141	3149	3164	rVB7	3527	6862	0.57%	0.071%
73	11.526	3164	3168	3172	rBV2	374	285	0.02%	0.003%
74	11.574	3180	3183	3188	rBV2	340	332	0.03%	0.003%
75	11.648	3204	3206	3212	rVB2	339	291	0.02%	0.003%
76	11.687	3215	3218	3219	rBV	414	241	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047872.D
 Acq On : 08 Apr 2022 17:24
 Operator : SY/MD
 Sample : VU0409WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK080

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.748	3229	3237	3245	rBV2	3498	4650	0.38%	0.048%
78	11.812	3245	3257	3282	rVV	566624	918747	75.94%	9.541%
79	11.976	3305	3308	3315	rVB6	1913	1627	0.13%	0.017%
80	12.034	3321	3326	3330	rBV2	519	497	0.04%	0.005%
81	12.121	3346	3353	3356	rBV3	421	596	0.05%	0.006%
82	12.195	3360	3376	3397	rBV	548029	899356	74.33%	9.339%
83	12.307	3408	3411	3415	rBV2	572	382	0.03%	0.004%
84	12.336	3415	3420	3423	rBV3	458	483	0.04%	0.005%
85	12.568	3486	3492	3494	rBV4	407	426	0.04%	0.004%
86	12.629	3509	3511	3518	rVB3	560	605	0.05%	0.006%
87	12.671	3518	3524	3526	rBV2	406	484	0.04%	0.005%
88	12.848	3576	3579	3582	rBV	388	290	0.02%	0.003%
89	13.005	3624	3628	3633	rVB3	1177	1161	0.10%	0.012%
90	13.156	3671	3675	3679	rBV3	419	425	0.04%	0.004%
91	13.224	3690	3696	3707	rVB4	4302	6816	0.56%	0.071%
92	13.278	3707	3713	3716	rBV2	367	450	0.04%	0.005%
93	13.394	3747	3749	3755	rBV2	337	284	0.02%	0.003%
94	13.503	3780	3783	3787	rBV2	372	327	0.03%	0.003%
95	13.844	3880	3889	3901	rBV2	8887	13057	1.08%	0.136%
96	14.092	3957	3966	3982	rVB	16953	27867	2.30%	0.289%
97	14.333	4033	4041	4052	rVB2	9670	14255	1.18%	0.148%
98	14.442	4072	4075	4078	rBV2	523	407	0.03%	0.004%
99	14.973	4237	4240	4243	rBV3	603	426	0.04%	0.004%
100	15.066	4266	4269	4273	rBV3	430	471	0.04%	0.005%




Sum of corrected areas: 9629712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047872.D
Acq On : 08 Apr 2022 17:24
Operator : SY/MD
Sample : VU0409WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK080

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

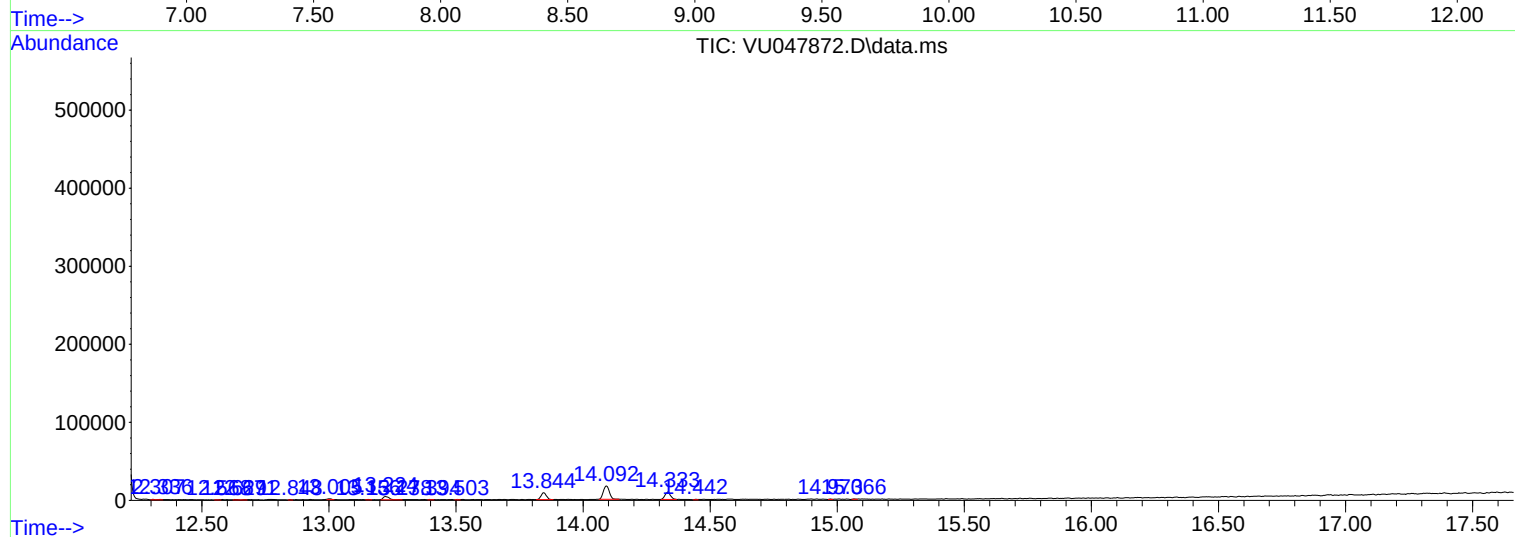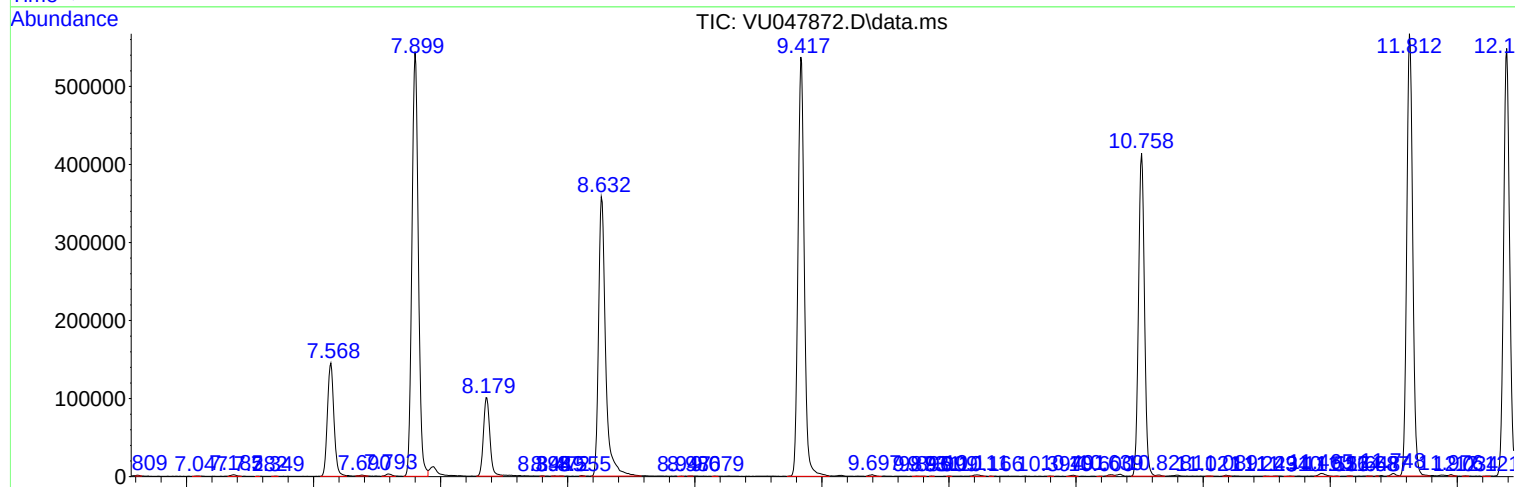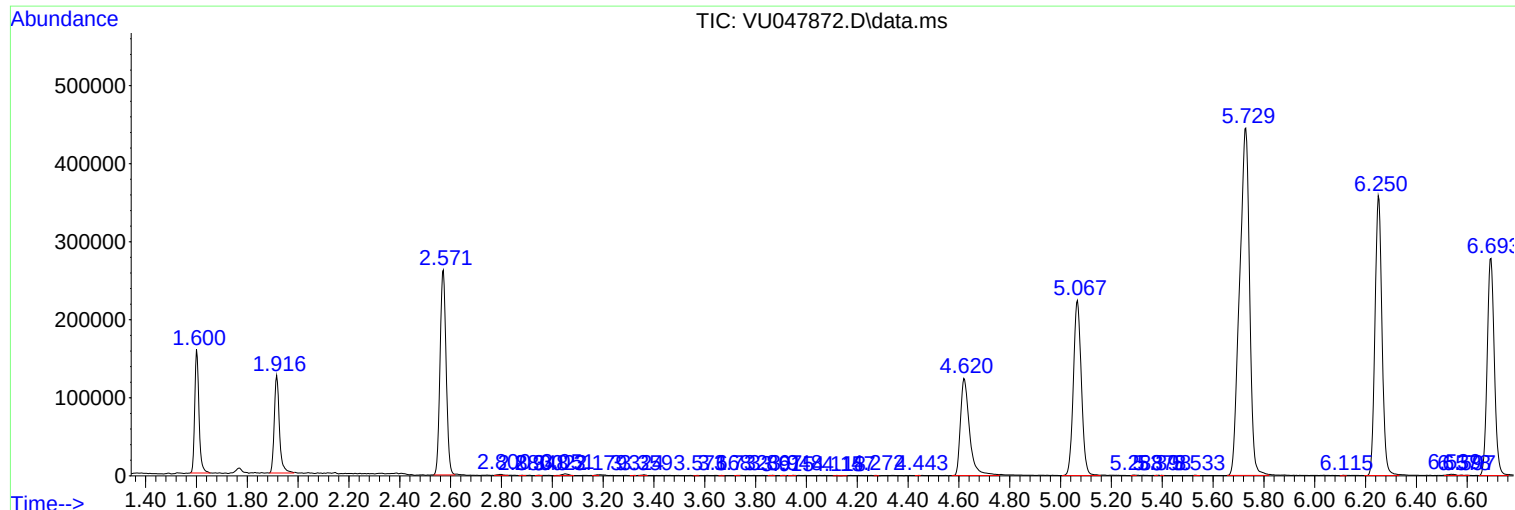

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047872.D
Acq On : 08 Apr 2022 17:24
Operator : SY/MD
Sample : VU0409WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK080

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047872.D
Acq On : 08 Apr 2022 17:24
Operator : SY/MD
Sample : VU0409WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK080

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------