

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047875.D
 Acq On : 08 Apr 2022 18:33
 Operator : SY/MD
 Sample : N2343-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rBV	148556	174120	2.38%	1.003%
2	1.916	170	179	200	rVB	123126	168343	2.30%	0.970%
3	2.572	369	383	399	rBV	248806	410778	5.61%	2.367%
4	2.713	424	427	434	rVB3	326	376	0.01%	0.002%
5	2.765	437	443	444	rBV3	861	765	0.01%	0.004%
6	2.781	446	448	455	rVB4	955	912	0.01%	0.005%
7	2.871	472	476	480	rBV2	466	448	0.01%	0.003%
8	3.044	527	530	535	rBV2	699	721	0.01%	0.004%
9	3.099	544	547	548	rBV	368	223	0.00%	0.001%
10	3.125	552	555	559	rVV3	309	231	0.00%	0.001%
11	3.192	560	576	593	rVV	16640	39156	0.53%	0.226%
12	3.356	623	627	628	rBV	522	332	0.00%	0.002%
13	3.408	641	643	650	rVB2	350	341	0.00%	0.002%
14	3.649	715	718	726	rBV2	254	265	0.00%	0.002%
15	3.835	772	776	780	rBV	313	214	0.00%	0.001%
16	3.945	806	810	812	rBV	276	265	0.00%	0.002%
17	4.305	919	922	928	rVB2	215	198	0.00%	0.001%
18	4.359	935	939	943	rBV3	268	225	0.00%	0.001%
19	4.398	947	951	954	rBV3	281	218	0.00%	0.001%
20	4.626	1006	1022	1067	rBV2	143905	384666	5.26%	2.217%
21	4.883	1100	1102	1111	rVB4	615	609	0.01%	0.004%
22	5.067	1142	1159	1179	rBV	211580	459966	6.28%	2.651%
23	5.237	1210	1212	1216	rVB2	508	334	0.00%	0.002%
24	5.279	1220	1225	1226	rBV3	329	262	0.00%	0.002%
25	5.366	1249	1252	1255	rBV2	253	198	0.00%	0.001%
26	5.388	1255	1259	1263	rBV2	435	446	0.01%	0.003%
27	5.472	1281	1285	1288	rVB	221	195	0.00%	0.001%
28	5.588	1316	1321	1324	rBV2	283	215	0.00%	0.001%
29	5.726	1343	1364	1396	rBV2	427182	1165535	15.92%	6.716%
30	5.899	1414	1418	1421	rBV3	315	257	0.00%	0.001%
31	6.041	1457	1462	1463	rBV	280	231	0.00%	0.001%
32	6.115	1483	1485	1489	rVB3	359	276	0.00%	0.002%
33	6.250	1510	1527	1547	rBV	346292	651577	8.90%	3.755%
34	6.401	1571	1574	1577	rBV	390	248	0.00%	0.001%
35	6.446	1584	1588	1591	rBV2	226	208	0.00%	0.001%
36	6.536	1608	1616	1623	rBV6	1302	2036	0.03%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047875.D
 Acq On : 08 Apr 2022 18:33
 Operator : SY/MD
 Sample : N2343-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.571	1625	1627	1633	rVB4	615	367	0.01%	0.002%
38	6.620	1637	1642	1646	rVB3	398	428	0.01%	0.002%
39	6.694	1650	1665	1688	rBV	264403	513328	7.01%	2.958%
40	6.980	1750	1754	1758	rVB4	588	582	0.01%	0.003%
41	7.041	1768	1773	1776	rBV3	431	425	0.01%	0.002%
42	7.189	1805	1819	1826	rBV4	1729	3044	0.04%	0.018%
43	7.272	1841	1845	1846	rBV	272	198	0.00%	0.001%
44	7.330	1860	1863	1866	rBV	304	230	0.00%	0.001%
45	7.436	1894	1896	1899	rVB2	340	193	0.00%	0.001%
46	7.568	1921	1937	1959	rBV	135730	241907	3.30%	1.394%
47	7.687	1968	1974	1982	rBV5	1133	1770	0.02%	0.010%
48	7.732	1985	1988	1989	rBV2	312	205	0.00%	0.001%
49	7.793	2002	2007	2016	rBV3	1548	2245	0.03%	0.013%
50	7.899	2026	2040	2055	rBV	522911	896795	12.25%	5.168%
51	8.179	2116	2127	2145	rBV	95528	164171	2.24%	0.946%
52	8.475	2208	2219	2231	rVB2	15637	27034	0.37%	0.156%
53	8.552	2240	2243	2244	rBV3	908	600	0.01%	0.003%
54	8.581	2248	2252	2254	rBV	277	191	0.00%	0.001%
55	8.636	2254	2269	2306	rBV	357310	668449	9.13%	3.852%
56	8.922	2351	2358	2359	rBV3	323	333	0.00%	0.002%
57	9.009	2381	2385	2389	rVB3	317	277	0.00%	0.002%
58	9.054	2394	2399	2401	rVB2	413	289	0.00%	0.002%
59	9.073	2401	2405	2409	rBV3	428	379	0.01%	0.002%
60	9.131	2420	2423	2426	rBV3	348	337	0.00%	0.002%
61	9.295	2471	2474	2479	rBV3	343	341	0.00%	0.002%
62	9.446	2499	2521	2558	rBV2	3904171	7319829	100.00%	42.180%
63	9.693	2589	2598	2608	rVB4	3537	5558	0.08%	0.032%
64	9.739	2608	2612	2614	rBV3	334	193	0.00%	0.001%
65	9.758	2615	2618	2622	rVV2	494	328	0.00%	0.002%
66	9.796	2622	2630	2636	rVV3	504	676	0.01%	0.004%
67	9.832	2636	2641	2644	rVB4	397	387	0.01%	0.002%
68	9.890	2655	2659	2663	rVB3	415	347	0.00%	0.002%
69	10.031	2698	2703	2706	rBV2	326	354	0.00%	0.002%
70	10.102	2718	2725	2731	rBV6	1525	2067	0.03%	0.012%
71	10.218	2756	2761	2762	rBV2	359	295	0.00%	0.002%
72	10.365	2805	2807	2812	rVB	293	196	0.00%	0.001%
73	10.488	2839	2845	2852	rVB	819	1028	0.01%	0.006%
74	10.674	2896	2903	2913	rVB5	2242	3312	0.05%	0.019%
75	10.758	2915	2929	2945	rBV	401329	641335	8.76%	3.696%
76	10.893	2958	2971	2986	rBV	24550	42345	0.58%	0.244%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047875.D
 Acq On : 08 Apr 2022 18:33
 Operator : SY/MD
 Sample : N2343-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.989	2996	3001	3004	rBV3	748	733	0.01%	0.004%
78	11.092	3027	3033	3041	rBV4	1169	1651	0.02%	0.010%
79	11.147	3046	3050	3053	rBV	258	220	0.00%	0.001%
80	11.295	3092	3096	3101	rVB3	319	265	0.00%	0.002%
81	11.343	3107	3111	3114	rBV3	366	273	0.00%	0.002%
82	11.468	3141	3150	3157	rVV8	2327	4531	0.06%	0.026%
83	11.581	3180	3185	3190	rVB4	436	495	0.01%	0.003%
84	11.697	3215	3221	3226	rBV3	1310	1458	0.02%	0.008%
85	11.745	3226	3236	3246	rBV	67998	108982	1.49%	0.628%
86	11.816	3246	3258	3260	rBV	638799	883154	12.07%	5.089%
87	11.941	3293	3297	3298	rBV2	724	477	0.01%	0.003%
88	12.070	3327	3337	3345	rBV7	2906	5452	0.07%	0.031%
89	12.208	3360	3380	3408	rBV2	966871	2224313	30.39%	12.817%
90	12.365	3426	3429	3433	rBV4	317	278	0.00%	0.002%
91	12.404	3437	3441	3442	rBV3	336	233	0.00%	0.001%
92	12.774	3547	3556	3565	rBV4	4904	7877	0.11%	0.045%
93	12.896	3589	3594	3598	rVB5	1167	1212	0.02%	0.007%
94	13.224	3690	3696	3700	rBV3	1359	1602	0.02%	0.009%
95	13.841	3878	3888	3900	rBV	52500	80049	1.09%	0.461%
96	14.092	3959	3966	3980	rVB2	5207	7599	0.10%	0.044%
97	14.192	3994	3997	4001	rBV	428	330	0.00%	0.002%
98	14.330	4032	4040	4053	rBV2	9668	13840	0.19%	0.080%
99	14.565	4109	4113	4114	rBV	561	364	0.00%	0.002%
100	15.198	4307	4310	4314	rBV4	752	632	0.01%	0.004%




Sum of corrected areas: 17353778

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047875.D
Acq On : 08 Apr 2022 18:33
Operator : SY/MD
Sample : N2343-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

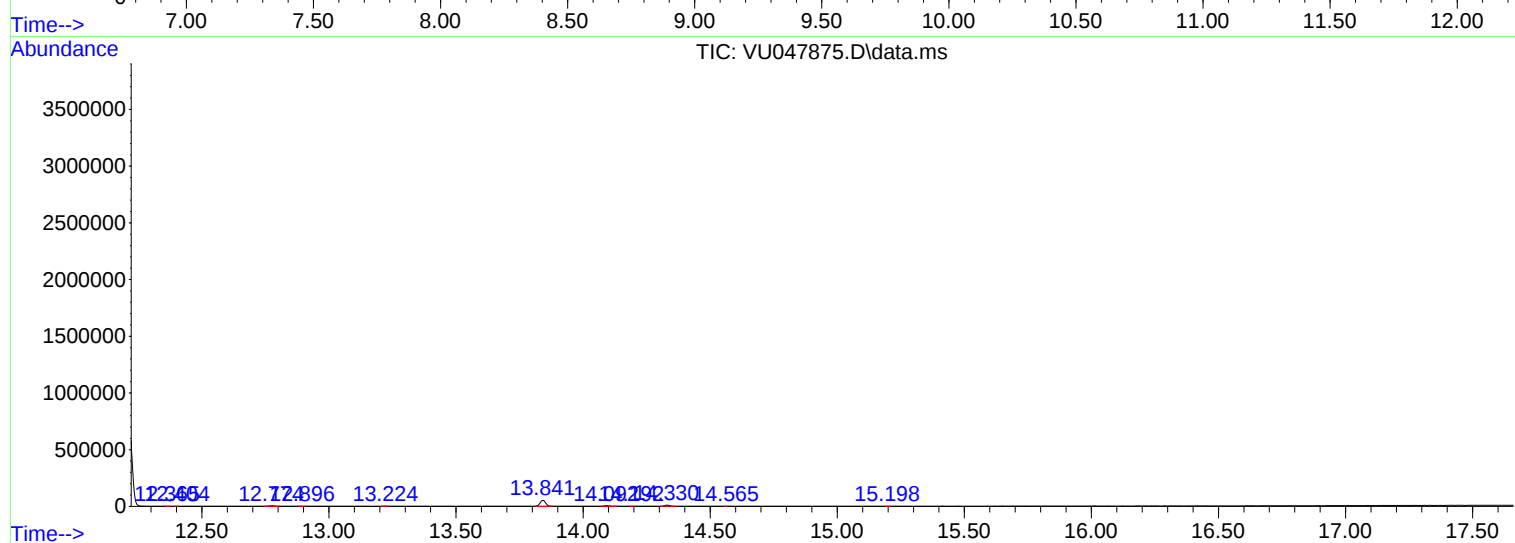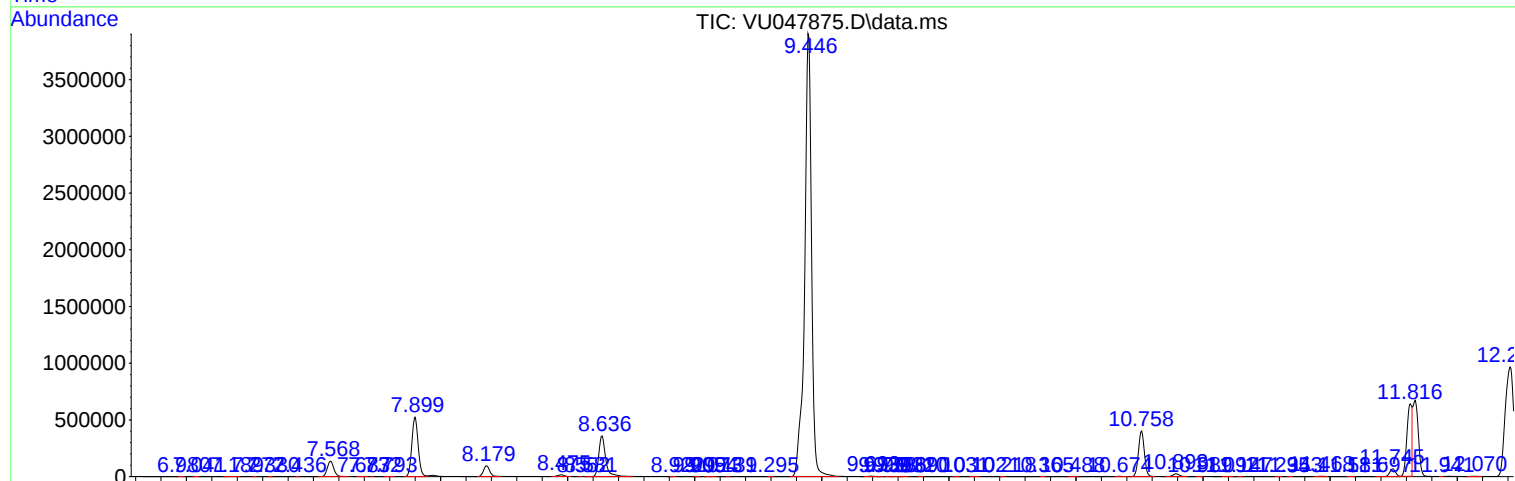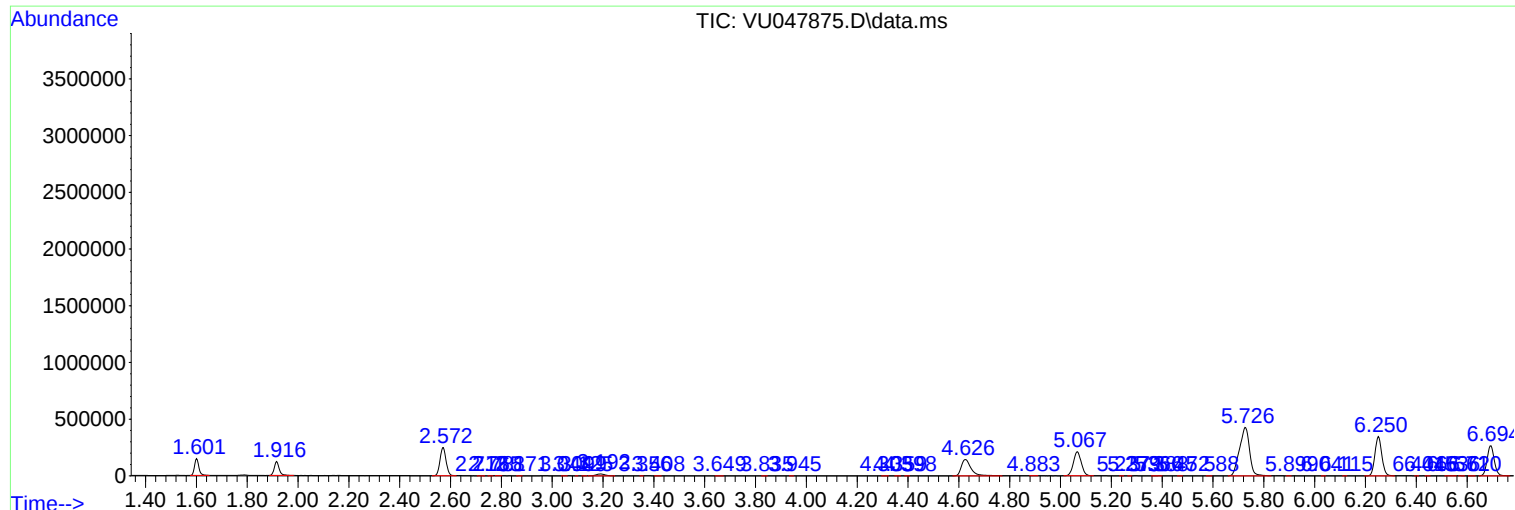

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047875.D
Acq On : 08 Apr 2022 18:33
Operator : SY/MD
Sample : N2343-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047875.D
Acq On : 08 Apr 2022 18:33
Operator : SY/MD
Sample : N2343-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc