

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047876.D
 Acq On : 08 Apr 2022 18:56
 Operator : SY/MD
 Sample : N2343-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	103	rVB	150214	174703	3.62%	1.311%
2	1.916	171	179	196	rVB	123760	164722	3.41%	1.236%
3	2.572	370	383	401	rBV	241727	404038	8.37%	3.032%
4	3.125	550	555	556	rBV2	192	126	0.00%	0.001%
5	3.131	556	557	559	rBV2	228	92	0.00%	0.001%
6	3.189	564	575	588	rVB	14654	31660	0.66%	0.238%
7	3.321	613	616	619	rBV2	235	119	0.00%	0.001%
8	3.363	623	629	633	rBV4	437	463	0.01%	0.003%
9	3.520	670	678	682	rBV2	268	376	0.01%	0.003%
10	3.636	710	714	719	rBV2	299	328	0.01%	0.002%
11	3.781	755	759	763	rBV3	266	317	0.01%	0.002%
12	3.838	775	777	778	rBV	258	112	0.00%	0.001%
13	3.890	790	793	796	rBV2	215	166	0.00%	0.001%
14	3.909	796	799	800	rBV	171	99	0.00%	0.001%
15	3.996	821	826	829	rBV2	290	260	0.01%	0.002%
16	4.018	829	833	835	rBV3	280	193	0.00%	0.001%
17	4.044	839	841	843	rBV2	147	93	0.00%	0.001%
18	4.099	856	858	860	rBV	145	93	0.00%	0.001%
19	4.247	901	904	906	rBV	301	202	0.00%	0.002%
20	4.295	915	919	922	rBV2	226	167	0.00%	0.001%
21	4.369	939	942	945	rVB2	303	183	0.00%	0.001%
22	4.420	955	958	959	rBV	253	127	0.00%	0.001%
23	4.633	1009	1024	1058	rBV2	146929	411374	8.52%	3.087%
24	5.067	1143	1159	1184	rBV	208015	457118	9.47%	3.431%
25	5.215	1203	1205	1210	rBV3	296	216	0.00%	0.002%
26	5.260	1215	1219	1220	rBV	226	104	0.00%	0.001%
27	5.295	1225	1230	1238	rVB3	631	860	0.02%	0.006%
28	5.330	1239	1241	1244	rBV2	233	104	0.00%	0.001%
29	5.379	1253	1256	1260	rBV2	349	290	0.01%	0.002%
30	5.417	1266	1268	1270	rVB	284	90	0.00%	0.001%
31	5.433	1270	1273	1277	rBV2	307	233	0.00%	0.002%
32	5.636	1334	1336	1338	rVB	289	98	0.00%	0.001%
33	5.726	1338	1364	1394	rBV2	421687	1145411	23.73%	8.597%
34	6.028	1455	1458	1460	rBV2	214	149	0.00%	0.001%
35	6.096	1476	1479	1481	rBV	174	102	0.00%	0.001%
36	6.115	1482	1485	1488	rVB	216	110	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047876.D
 Acq On : 08 Apr 2022 18:56
 Operator : SY/MD
 Sample : N2343-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.131	1488	1490	1493	rVB	229	107	0.00%	0.001%
38	6.182	1504	1506	1509	rBV	199	92	0.00%	0.001%
39	6.250	1512	1527	1555	rBV	340960	642247	13.31%	4.820%
40	6.488	1599	1601	1606	rVB2	344	237	0.00%	0.002%
41	6.526	1609	1613	1615	rBV2	830	716	0.01%	0.005%
42	6.581	1627	1630	1631	rBV2	564	349	0.01%	0.003%
43	6.623	1640	1643	1645	rBV	411	231	0.00%	0.002%
44	6.636	1645	1647	1649	rBV	289	162	0.00%	0.001%
45	6.694	1650	1665	1688	rBV	260500	510268	10.57%	3.830%
46	6.854	1712	1715	1717	rBV2	419	210	0.00%	0.002%
47	7.025	1765	1768	1771	rBV2	169	123	0.00%	0.001%
48	7.044	1771	1774	1776	rBV	346	235	0.00%	0.002%
49	7.182	1810	1817	1819	rBV3	1678	1808	0.04%	0.014%
50	7.234	1831	1833	1836	rBV	238	136	0.00%	0.001%
51	7.272	1840	1845	1849	rVB3	322	328	0.01%	0.002%
52	7.333	1861	1864	1867	rBV2	310	211	0.00%	0.002%
53	7.391	1877	1882	1883	rBV2	241	174	0.00%	0.001%
54	7.427	1891	1893	1895	rBV2	210	113	0.00%	0.001%
55	7.478	1907	1909	1912	rVB2	270	135	0.00%	0.001%
56	7.568	1919	1937	1956	rBV	134016	241057	4.99%	1.809%
57	7.899	2025	2040	2055	rBV	510838	887789	18.39%	6.663%
58	8.131	2108	2112	2114	rBV3	348	286	0.01%	0.002%
59	8.179	2116	2127	2148	rVV	94323	165388	3.43%	1.241%
60	8.436	2204	2207	2209	rBV2	307	218	0.00%	0.002%
61	8.475	2209	2219	2234	rVV3	7344	13403	0.28%	0.101%
62	8.552	2239	2243	2244	rBV2	489	345	0.01%	0.003%
63	8.636	2257	2269	2307	rBV	361114	685229	14.20%	5.143%
64	8.944	2358	2365	2369	rBV3	276	438	0.01%	0.003%
65	9.009	2383	2385	2389	rBV3	307	167	0.00%	0.001%
66	9.121	2417	2420	2422	rBV	303	181	0.00%	0.001%
67	9.157	2426	2431	2436	rBV2	251	346	0.01%	0.003%
68	9.230	2451	2454	2455	rBV	246	128	0.00%	0.001%
69	9.330	2479	2485	2489	rBV3	333	378	0.01%	0.003%
70	9.353	2489	2492	2497	rBV3	271	162	0.00%	0.001%
71	9.446	2499	2521	2558	rBV2	2370462	4826358	100.00%	36.223%
72	9.693	2590	2598	2610	rBV3	3471	5557	0.12%	0.042%
73	9.771	2620	2622	2625	rBV2	378	241	0.00%	0.002%
74	9.790	2626	2628	2632	rVV	366	233	0.00%	0.002%
75	9.829	2637	2640	2643	rVB2	342	235	0.00%	0.002%
76	9.983	2686	2688	2690	rBV	328	198	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047876.D
 Acq On : 08 Apr 2022 18:56
 Operator : SY/MD
 Sample : N2343-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.018	2698	2699	2705	rVB3	333	264	0.01%	0.002%
78	10.047	2705	2708	2713	rBV2	364	398	0.01%	0.003%
79	10.105	2719	2726	2736	rVB6	1920	3287	0.07%	0.025%
80	10.221	2758	2762	2767	rVB2	376	301	0.01%	0.002%
81	10.308	2785	2789	2793	rBV	277	298	0.01%	0.002%
82	10.417	2820	2823	2829	rBV	235	329	0.01%	0.002%
83	10.459	2834	2836	2839	rBV2	426	251	0.01%	0.002%
84	10.481	2839	2843	2844	rBV	510	369	0.01%	0.003%
85	10.536	2855	2860	2864	rBV2	294	313	0.01%	0.002%
86	10.626	2887	2888	2892	rVB	232	104	0.00%	0.001%
87	10.674	2897	2903	2910	rVB3	2416	3172	0.07%	0.024%
88	10.758	2916	2929	2948	rBV	394824	638144	13.22%	4.789%
89	10.845	2954	2956	2960	rBV3	351	277	0.01%	0.002%
90	10.893	2963	2971	2983	rVB3	11849	20518	0.43%	0.154%
91	10.964	2990	2993	2995	rBV2	314	207	0.00%	0.002%
92	11.465	3141	3149	3162	rVB6	2692	5090	0.11%	0.038%
93	11.693	3214	3220	3227	rVB7	1435	1945	0.04%	0.015%
94	11.751	3230	3238	3244	rBV5	3930	5517	0.11%	0.041%
95	11.812	3244	3257	3280	rBV	557924	926867	19.20%	6.956%
96	11.973	3303	3307	3314	rVB4	1767	2127	0.04%	0.016%
97	12.002	3314	3316	3320	rBV2	424	243	0.01%	0.002%
98	12.195	3363	3376	3395	rBV	530257	913142	18.92%	6.853%
99	12.777	3548	3557	3569	rVB4	2182	3771	0.08%	0.028%
100	13.844	3881	3889	3901	rVB3	10434	15922	0.33%	0.119%




Sum of corrected areas: 13323973

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047876.D
Acq On : 08 Apr 2022 18:56
Operator : SY/MD
Sample : N2343-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

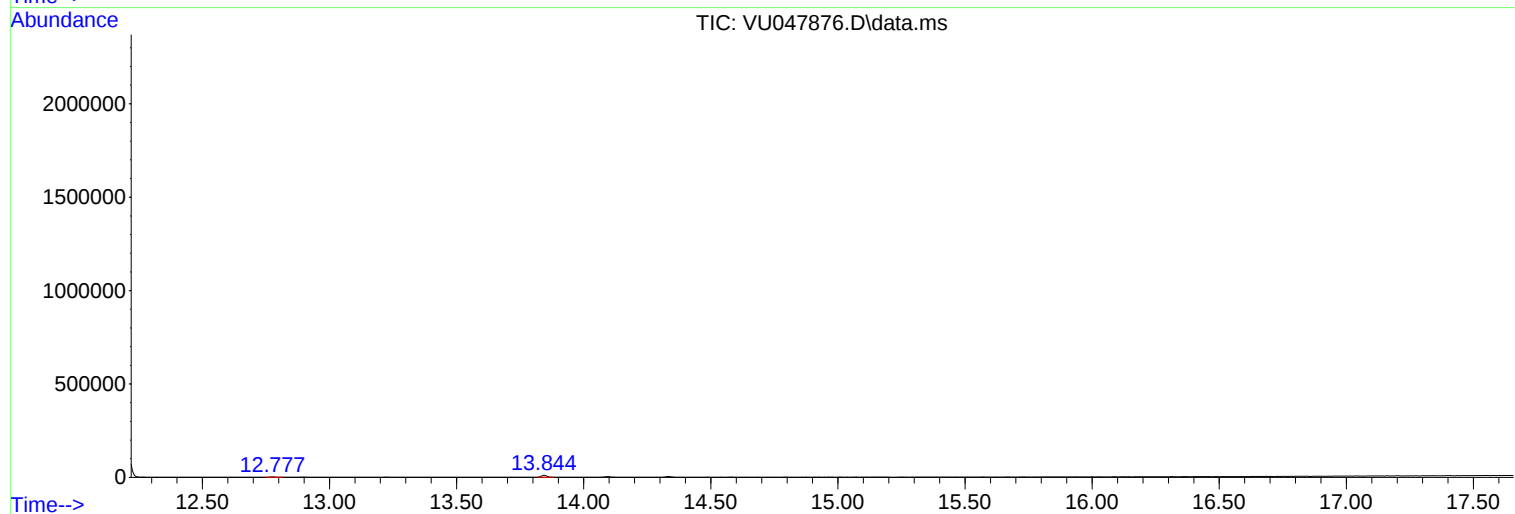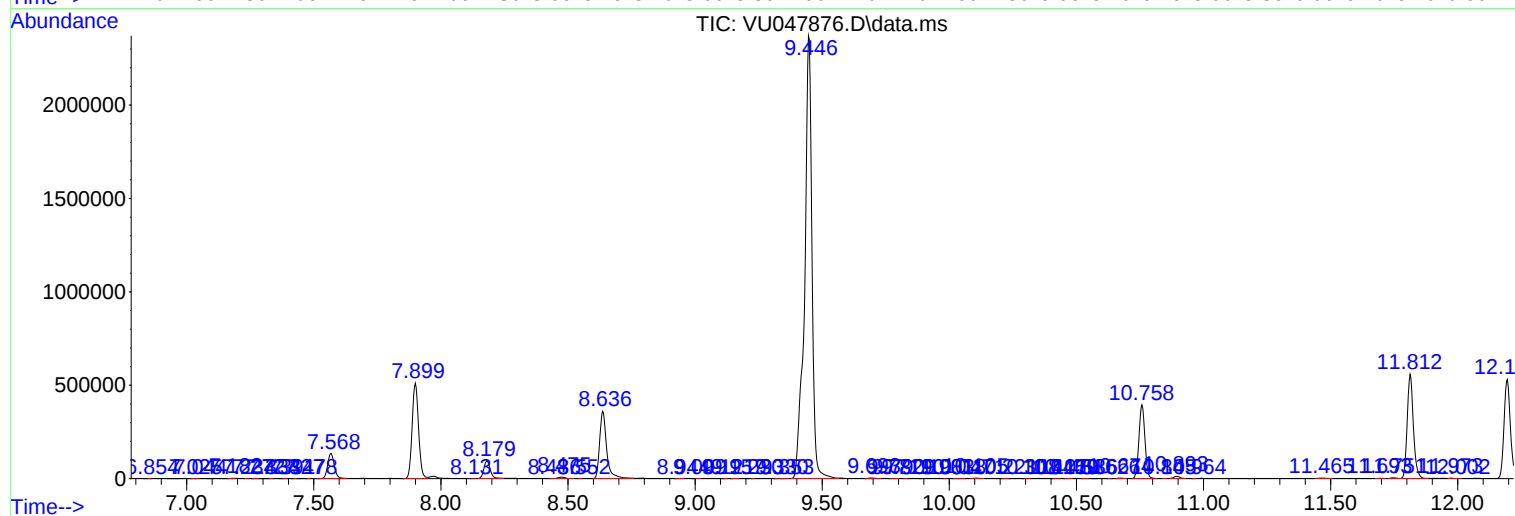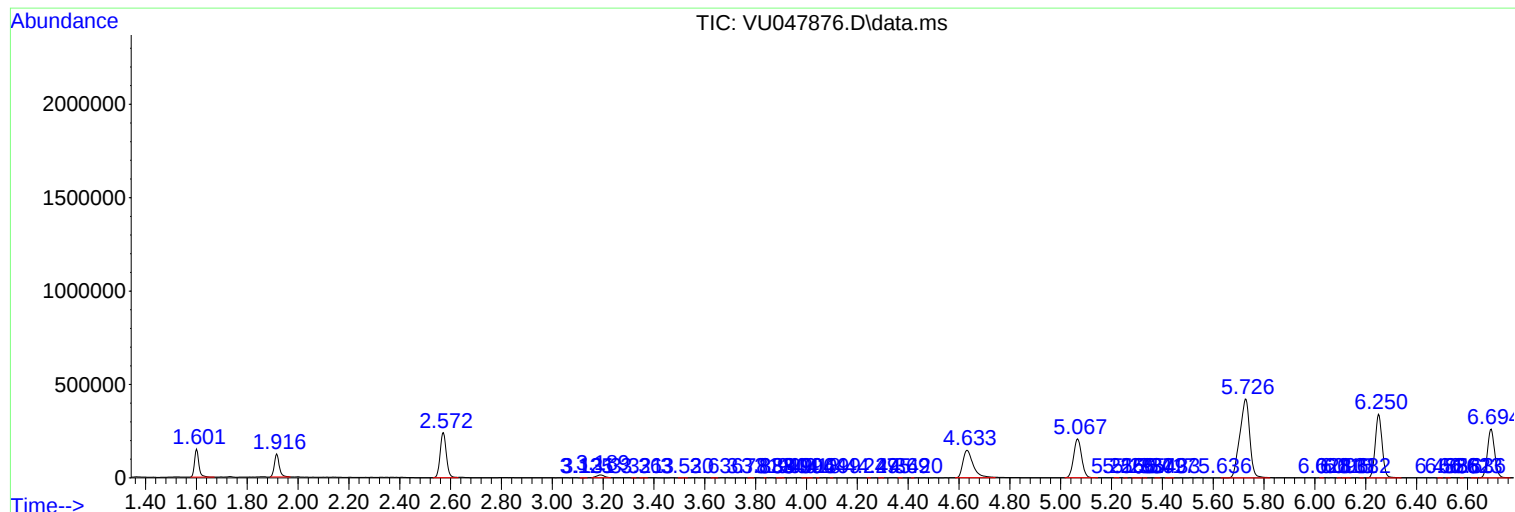

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047876.D
Acq On : 08 Apr 2022 18:56
Operator : SY/MD
Sample : N2343-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047876.D
Acq On : 08 Apr 2022 18:56
Operator : SY/MD
Sample : N2343-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc