

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047877.D
 Acq On : 08 Apr 2022 19:19
 Operator : SY/MD
 Sample : N2343-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	51	rBV	4153	4727	0.09%	0.024%
2	1.601	74	81	101	rVB	140208	163023	3.13%	0.833%
3	1.916	170	179	193	rBV	116210	156439	3.01%	0.799%
4	2.572	370	383	400	rBV	231132	383145	7.36%	1.958%
5	2.752	435	439	441	rBV2	400	353	0.01%	0.002%
6	2.781	444	448	451	rVV4	697	742	0.01%	0.004%
7	2.800	452	454	462	rVB4	748	751	0.01%	0.004%
8	2.890	479	482	485	rBV3	347	338	0.01%	0.002%
9	2.948	495	500	501	rBV2	446	293	0.01%	0.001%
10	3.047	526	531	532	rBV2	533	299	0.01%	0.002%
11	3.189	564	575	593	rVB3	3157	7212	0.14%	0.037%
12	3.356	623	627	628	rBV	662	351	0.01%	0.002%
13	3.372	630	632	635	rVB3	854	471	0.01%	0.002%
14	3.436	650	652	658	rVB3	396	412	0.01%	0.002%
15	3.572	692	694	700	rVV2	380	322	0.01%	0.002%
16	3.700	729	734	737	rBV	358	326	0.01%	0.002%
17	4.002	822	828	835	rBV2	291	476	0.01%	0.002%
18	4.289	914	917	924	rVB3	335	335	0.01%	0.002%
19	4.324	924	928	934	rBV2	250	360	0.01%	0.002%
20	4.388	943	948	950	rBV	283	271	0.01%	0.001%
21	4.498	979	982	986	rVB2	286	258	0.00%	0.001%
22	4.526	986	991	994	rBV3	448	412	0.01%	0.002%
23	4.626	1008	1022	1057	rBV	111638	284584	5.47%	1.454%
24	4.858	1089	1094	1097	rBV3	413	332	0.01%	0.002%
25	5.067	1142	1159	1182	rBV	198706	433603	8.33%	2.216%
26	5.295	1222	1230	1236	rBV3	654	1000	0.02%	0.005%
27	5.427	1268	1271	1277	rVB2	206	255	0.00%	0.001%
28	5.472	1277	1285	1291	rBV2	293	528	0.01%	0.003%
29	5.523	1291	1301	1305	rBV3	1055	1646	0.03%	0.008%
30	5.620	1326	1331	1336	rVB2	310	285	0.01%	0.001%
31	5.729	1343	1365	1370	rBV2	399550	1022126	19.64%	5.223%
32	5.777	1371	1380	1413	rVB	1718233	3435822	66.02%	17.555%
33	6.121	1484	1487	1490	rVB4	489	303	0.01%	0.002%
34	6.250	1514	1527	1550	rBV	356670	669002	12.86%	3.418%
35	6.414	1573	1578	1581	rBV2	275	325	0.01%	0.002%
36	6.536	1608	1616	1623	rBV4	1715	2903	0.06%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047877.D
 Acq On : 08 Apr 2022 19:19
 Operator : SY/MD
 Sample : N2343-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.597	1631	1635	1641	rVB3	729	659	0.01%	0.003%
38	6.694	1650	1665	1685	rBV	248223	483111	9.28%	2.468%
39	6.796	1693	1697	1707	rVB6	902	1370	0.03%	0.007%
40	6.861	1715	1717	1722	rVB3	362	260	0.00%	0.001%
41	6.896	1722	1728	1733	rVB3	347	465	0.01%	0.002%
42	7.050	1769	1776	1778	rBV2	534	682	0.01%	0.003%
43	7.092	1784	1789	1796	rBV2	383	465	0.01%	0.002%
44	7.186	1807	1818	1825	rBV5	1931	3020	0.06%	0.015%
45	7.279	1844	1847	1851	rVV3	342	293	0.01%	0.001%
46	7.485	1904	1911	1915	rBV2	296	410	0.01%	0.002%
47	7.520	1917	1922	1924	rBV2	311	293	0.01%	0.001%
48	7.568	1924	1937	1956	rBV	125969	224477	4.31%	1.147%
49	7.684	1968	1973	1974	rBV3	904	647	0.01%	0.003%
50	7.796	1998	2008	2014	rBV4	807	1367	0.03%	0.007%
51	7.899	2025	2040	2056	rBV	487838	842278	16.19%	4.304%
52	8.105	2099	2104	2106	rBV2	478	318	0.01%	0.002%
53	8.182	2115	2128	2143	rBV	88843	152361	2.93%	0.778%
54	8.475	2205	2219	2230	rBV2	12381	22931	0.44%	0.117%
55	8.555	2239	2244	2251	rVB6	1520	1737	0.03%	0.009%
56	8.636	2256	2269	2309	rBV	333535	626206	12.03%	3.200%
57	8.935	2358	2362	2364	rBV2	363	257	0.00%	0.001%
58	9.266	2456	2465	2468	rBV3	226	336	0.01%	0.002%
59	9.446	2499	2521	2558	rBV2	2611764	5203937	100.00%	26.590%
60	9.616	2572	2574	2578	rVB2	412	258	0.00%	0.001%
61	9.693	2589	2598	2607	rVB5	1724	3016	0.06%	0.015%
62	9.732	2607	2610	2613	rBV	523	285	0.01%	0.001%
63	9.803	2626	2632	2635	rBV2	338	344	0.01%	0.002%
64	10.034	2697	2704	2705	rBV2	425	385	0.01%	0.002%
65	10.102	2716	2725	2732	rBV4	865	1453	0.03%	0.007%
66	10.301	2784	2787	2794	rVB3	372	399	0.01%	0.002%
67	10.346	2794	2801	2803	rBV3	496	494	0.01%	0.003%
68	10.394	2812	2816	2823	rVB2	360	329	0.01%	0.002%
69	10.484	2841	2844	2850	rVB3	563	582	0.01%	0.003%
70	10.517	2850	2854	2858	rBV2	338	388	0.01%	0.002%
71	10.555	2862	2866	2868	rBV2	321	258	0.00%	0.001%
72	10.607	2877	2882	2885	rBV3	347	329	0.01%	0.002%
73	10.671	2895	2902	2910	rBV4	2016	2827	0.05%	0.014%
74	10.758	2915	2929	2946	rBV	367501	596917	11.47%	3.050%
75	10.893	2959	2971	2983	rBV	20618	34762	0.67%	0.178%
76	11.092	3028	3033	3038	rBV3	883	927	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047877.D
 Acq On : 08 Apr 2022 19:19
 Operator : SY/MD
 Sample : N2343-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.124	3040	3043	3048	rVV4	329	318	0.01%	0.002%
78	11.179	3055	3060	3063	rVB2	294	275	0.01%	0.001%
79	11.433	3135	3139	3140	rBV	351	258	0.00%	0.001%
80	11.465	3140	3149	3162	rVB7	2480	5341	0.10%	0.027%
81	11.523	3163	3167	3169	rBV2	340	255	0.00%	0.001%
82	11.578	3181	3184	3189	rBV3	695	683	0.01%	0.003%
83	11.693	3216	3220	3221	rBV2	728	509	0.01%	0.003%
84	11.745	3226	3236	3246	rBV	64425	102922	1.98%	0.526%
85	11.835	3246	3264	3291	rVB2	1028403	2452989	47.14%	12.534%
86	11.935	3293	3295	3299	rBV3	801	506	0.01%	0.003%
87	12.066	3328	3336	3352	rVB3	6043	10499	0.20%	0.054%
88	12.208	3362	3380	3399	rBV2	897261	2055500	39.50%	10.503%
89	12.404	3439	3441	3445	rVB3	499	329	0.01%	0.002%
90	12.481	3463	3465	3470	rBV2	309	323	0.01%	0.002%
91	12.590	3492	3499	3504	rBV4	486	774	0.01%	0.004%
92	12.770	3547	3555	3566	rVB3	4230	7055	0.14%	0.036%
93	12.896	3589	3594	3598	rBV3	1021	1046	0.02%	0.005%
94	13.082	3647	3652	3654	rBV3	323	305	0.01%	0.002%
95	13.224	3689	3696	3702	rVB4	1954	2531	0.05%	0.013%
96	13.658	3828	3831	3835	rBV	381	333	0.01%	0.002%
97	13.841	3877	3888	3904	rBV2	79537	125539	2.41%	0.641%
98	14.092	3959	3966	3976	rVB2	2623	3740	0.07%	0.019%
99	14.333	4032	4041	4054	rVB3	7931	13020	0.25%	0.067%
100	14.931	4224	4227	4229	rVB	708	344	0.01%	0.002%




Sum of corrected areas: 19571257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047877.D
Acq On : 08 Apr 2022 19:19
Operator : SY/MD
Sample : N2343-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

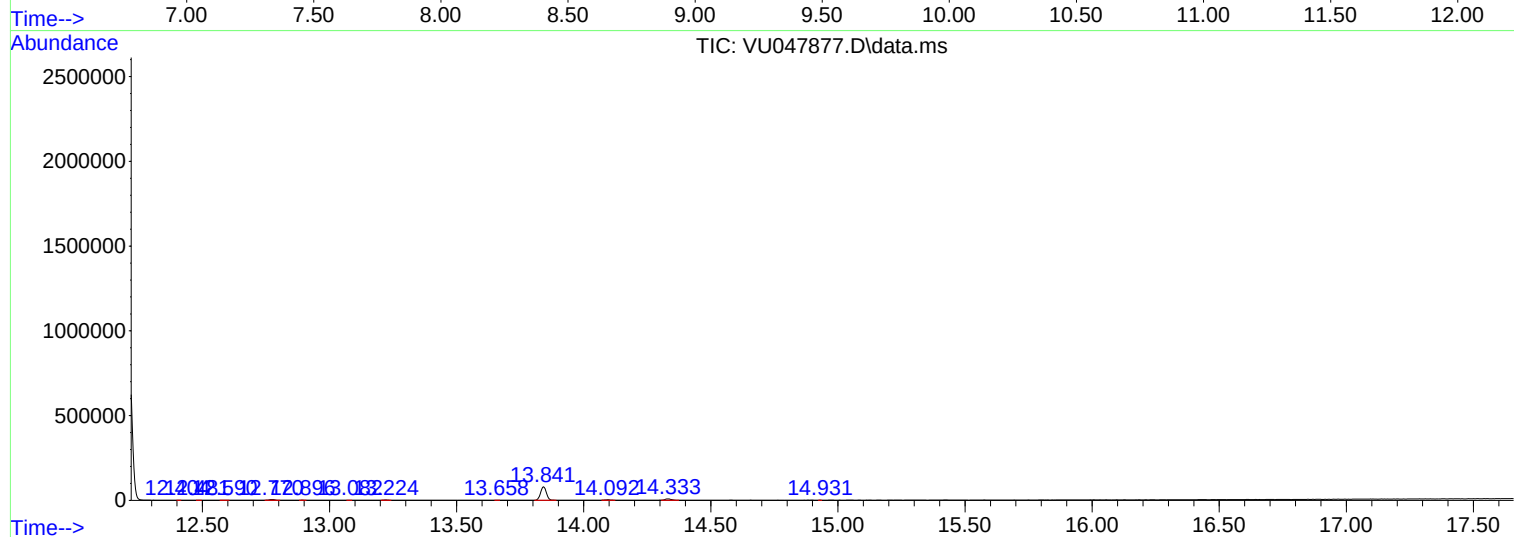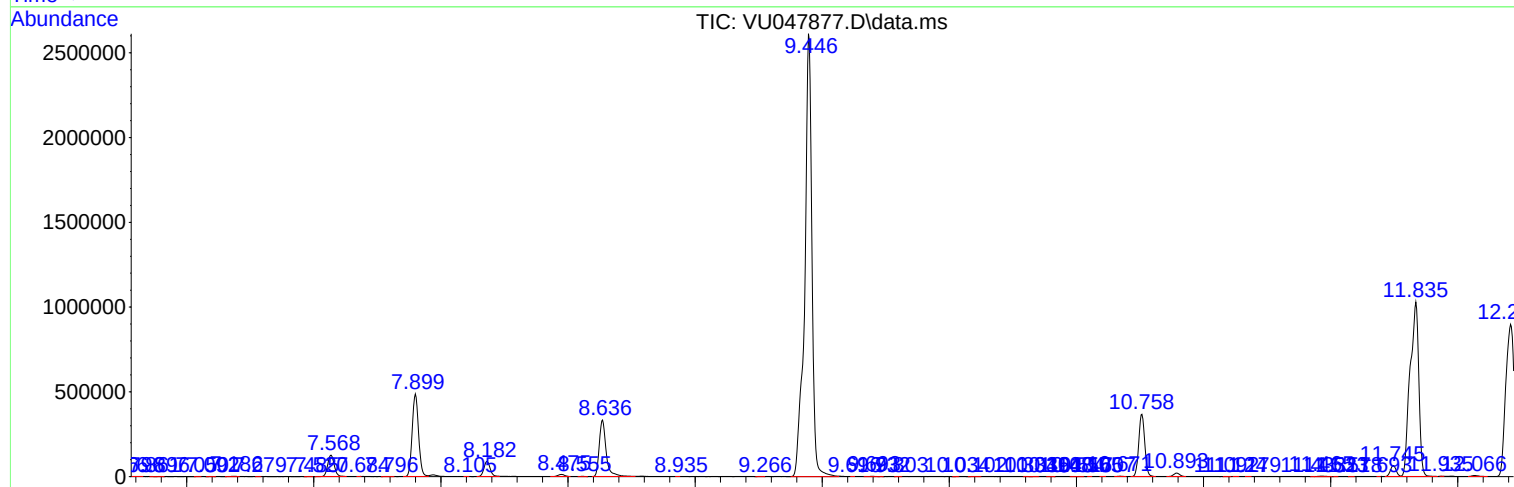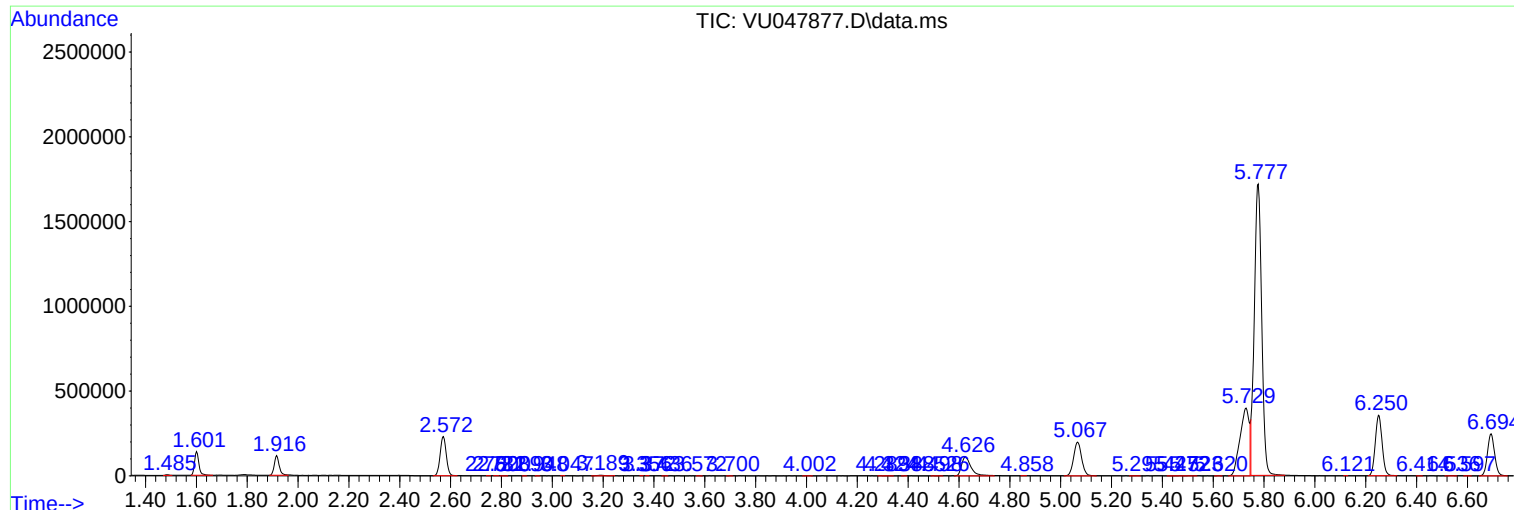

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047877.D
Acq On : 08 Apr 2022 19:19
Operator : SY/MD
Sample : N2343-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047877.D
Acq On : 08 Apr 2022 19:19
Operator : SY/MD
Sample : N2343-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------