

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047878.D
 Acq On : 08 Apr 2022 19:42
 Operator : SY/MD
 Sample : N2343-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	102	rVB	146352	170834	5.74%	1.416%
2	1.915	171	179	202	rVB	116245	162735	5.47%	1.348%
3	2.571	370	383	398	rBV	242638	399273	13.42%	3.308%
4	2.697	420	422	426	rVB3	295	202	0.01%	0.002%
5	2.758	433	441	447	rBV5	1740	3086	0.10%	0.026%
6	2.922	490	492	495	rBV2	332	226	0.01%	0.002%
7	2.983	508	511	518	rVB3	539	571	0.02%	0.005%
8	3.044	526	530	532	rBV2	635	551	0.02%	0.005%
9	3.105	546	549	552	rBV2	263	207	0.01%	0.002%
10	3.134	553	558	560	rVV3	342	340	0.01%	0.003%
11	3.189	561	575	591	rVV	13225	29678	1.00%	0.246%
12	3.366	622	630	636	rBV3	757	1214	0.04%	0.010%
13	3.440	647	653	656	rBV2	243	258	0.01%	0.002%
14	3.542	682	685	688	rVB2	312	212	0.01%	0.002%
15	3.841	776	778	783	rVB2	289	237	0.01%	0.002%
16	4.025	832	835	838	rBV	295	269	0.01%	0.002%
17	4.102	855	859	865	rVB2	205	218	0.01%	0.002%
18	4.317	921	926	928	rBV2	316	222	0.01%	0.002%
19	4.478	973	976	983	rVB2	391	423	0.01%	0.004%
20	4.520	983	989	990	rBV	276	251	0.01%	0.002%
21	4.620	1003	1020	1048	rBV	115767	289906	9.74%	2.402%
22	4.951	1120	1123	1127	rBV2	270	206	0.01%	0.002%
23	5.066	1142	1159	1184	rBV2	208518	453350	15.24%	3.756%
24	5.282	1223	1226	1227	rBV2	337	223	0.01%	0.002%
25	5.378	1253	1256	1263	rVB2	501	423	0.01%	0.004%
26	5.433	1270	1273	1277	rBV2	268	283	0.01%	0.002%
27	5.520	1297	1300	1303	rVV2	235	217	0.01%	0.002%
28	5.729	1342	1365	1373	rBV2	415369	1126328	37.86%	9.333%
29	6.021	1451	1456	1461	rVV3	411	459	0.02%	0.004%
30	6.050	1461	1465	1470	rVB3	364	335	0.01%	0.003%
31	6.105	1479	1482	1484	rBV	367	235	0.01%	0.002%
32	6.163	1498	1500	1504	rVB2	421	213	0.01%	0.002%
33	6.250	1513	1527	1551	rBV	348064	659965	22.18%	5.468%
34	6.504	1602	1606	1608	rBV2	409	330	0.01%	0.003%
35	6.536	1609	1616	1619	rBV4	1319	1600	0.05%	0.013%
36	6.693	1650	1665	1685	rBV	257400	504940	16.97%	4.184%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047878.D
 Acq On : 08 Apr 2022 19:42
 Operator : SY/MD
 Sample : N2343-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.806	1695	1700	1704	rBV4	746	751	0.03%	0.006%
38	6.857	1712	1716	1718	rBV	246	204	0.01%	0.002%
39	6.980	1751	1754	1757	rBV2	206	203	0.01%	0.002%
40	7.041	1770	1773	1777	rBV	304	267	0.01%	0.002%
41	7.105	1789	1793	1797	rBV2	270	306	0.01%	0.003%
42	7.185	1809	1818	1827	rVV2	1849	3080	0.10%	0.026%
43	7.465	1903	1905	1909	rVB2	319	213	0.01%	0.002%
44	7.568	1924	1937	1957	rBV	131714	233661	7.85%	1.936%
45	7.681	1968	1972	1973	rBV4	954	621	0.02%	0.005%
46	7.899	2026	2040	2056	rBV	506245	881153	29.62%	7.301%
47	8.179	2115	2127	2149	rBV	94428	163142	5.48%	1.352%
48	8.475	2207	2219	2229	rVV	9839	16917	0.57%	0.140%
49	8.555	2241	2244	2251	rBV5	651	584	0.02%	0.005%
50	8.635	2255	2269	2300	rBV	320233	631460	21.22%	5.232%
51	8.835	2327	2331	2335	rVB5	410	345	0.01%	0.003%
52	9.169	2431	2435	2438	rBV2	355	254	0.01%	0.002%
53	9.314	2475	2480	2483	rBV3	341	321	0.01%	0.003%
54	9.446	2499	2521	2556	rBV2	1254718	2975318	100.00%	24.653%
55	9.616	2572	2574	2577	rVB	417	226	0.01%	0.002%
56	9.693	2588	2598	2607	rVB2	3822	5712	0.19%	0.047%
57	9.735	2607	2611	2612	rBV	335	241	0.01%	0.002%
58	10.102	2718	2725	2733	rBV2	1708	2405	0.08%	0.020%
59	10.195	2750	2754	2757	rBV2	299	218	0.01%	0.002%
60	10.227	2762	2764	2766	rVB	491	223	0.01%	0.002%
61	10.256	2766	2773	2775	rBV2	437	407	0.01%	0.003%
62	10.291	2781	2784	2788	rVB2	393	239	0.01%	0.002%
63	10.487	2841	2845	2853	rVB3	544	690	0.02%	0.006%
64	10.635	2886	2891	2895	rBV2	260	260	0.01%	0.002%
65	10.671	2895	2902	2909	rVV5	1874	2719	0.09%	0.023%
66	10.758	2916	2929	2949	rVV	388293	630590	21.19%	5.225%
67	10.832	2949	2952	2957	rVV3	391	385	0.01%	0.003%
68	10.896	2959	2972	2986	rVB	15996	29686	1.00%	0.246%
69	10.999	3001	3004	3011	rVB3	492	540	0.02%	0.004%
70	11.031	3011	3014	3017	rBV3	287	280	0.01%	0.002%
71	11.095	3030	3034	3037	rBV2	518	378	0.01%	0.003%
72	11.124	3041	3043	3048	rVB3	560	393	0.01%	0.003%
73	11.262	3082	3086	3088	rBV2	240	213	0.01%	0.002%
74	11.468	3140	3150	3161	rBV9	3006	5851	0.20%	0.048%
75	11.597	3187	3190	3193	rVB2	397	288	0.01%	0.002%
76	11.619	3195	3197	3205	rBV2	384	383	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047878.D
 Acq On : 08 Apr 2022 19:42
 Operator : SY/MD
 Sample : N2343-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.661	3205	3210	3214	rBV2	284	345	0.01%	0.003%
78	11.696	3214	3221	3227	rBV6	875	1040	0.03%	0.009%
79	11.748	3227	3237	3245	rBV2	18600	28609	0.96%	0.237%
80	11.812	3245	3257	3283	rVV2	578369	1292431	43.44%	10.709%
81	11.970	3302	3306	3307	rBV4	839	598	0.02%	0.005%
82	12.073	3331	3338	3343	rBV6	1053	1429	0.05%	0.012%
83	12.143	3357	3360	3362	rBV3	504	326	0.01%	0.003%
84	12.195	3363	3376	3398	rVV2	584338	1290219	43.36%	10.691%
85	12.327	3415	3417	3420	rBV2	381	283	0.01%	0.002%
86	12.397	3436	3439	3440	rBV	527	314	0.01%	0.003%
87	12.433	3448	3450	3454	rVB4	412	261	0.01%	0.002%
88	12.478	3462	3464	3468	rVB	472	257	0.01%	0.002%
89	12.587	3493	3498	3505	rBV2	386	588	0.02%	0.005%
90	12.677	3522	3526	3528	rBV2	344	242	0.01%	0.002%
91	12.780	3551	3558	3565	rVB3	1727	2443	0.08%	0.020%
92	12.851	3575	3580	3581	rBV2	492	354	0.01%	0.003%
93	13.114	3659	3662	3667	rBV2	344	285	0.01%	0.002%
94	13.336	3727	3731	3733	rBV2	255	221	0.01%	0.002%
95	13.365	3736	3740	3748	rVB2	538	547	0.02%	0.005%
96	13.844	3878	3889	3903	rBV	23789	35384	1.19%	0.293%
97	14.098	3959	3968	3975	rBV2	2430	3741	0.13%	0.031%
98	14.333	4034	4041	4055	rVB4	4352	6467	0.22%	0.054%
99	15.214	4312	4315	4318	rBV3	503	401	0.01%	0.003%
100	15.272	4327	4333	4337	rBV5	622	816	0.03%	0.007%




Sum of corrected areas: 12068748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047878.D
Acq On : 08 Apr 2022 19:42
Operator : SY/MD
Sample : N2343-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

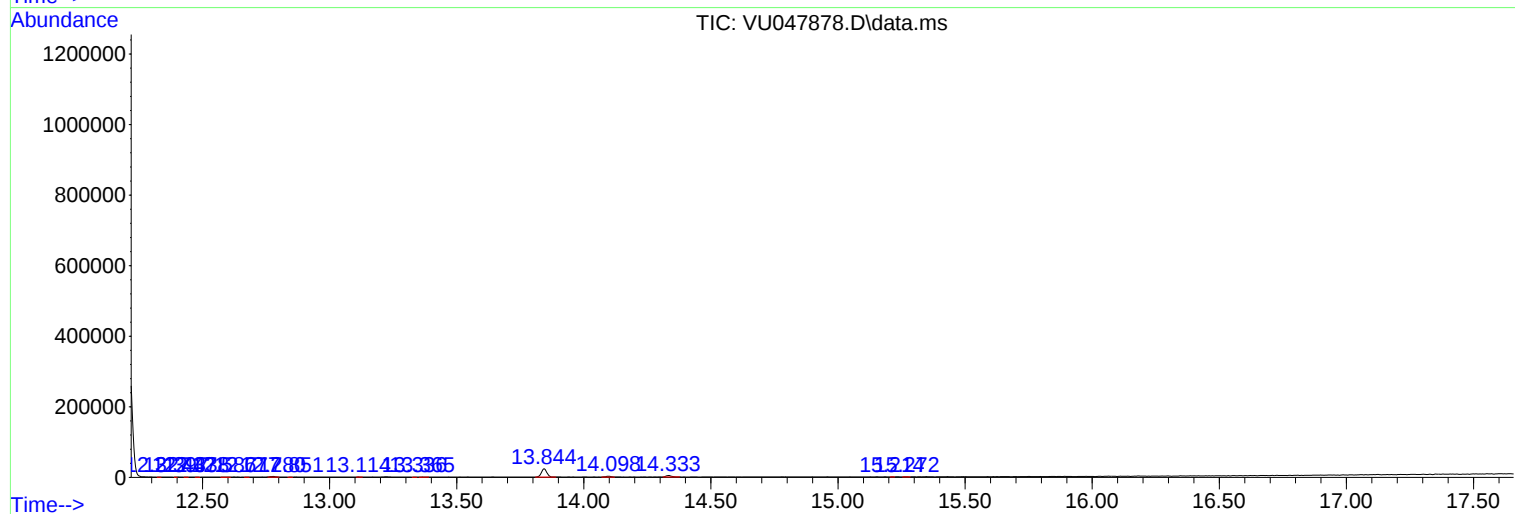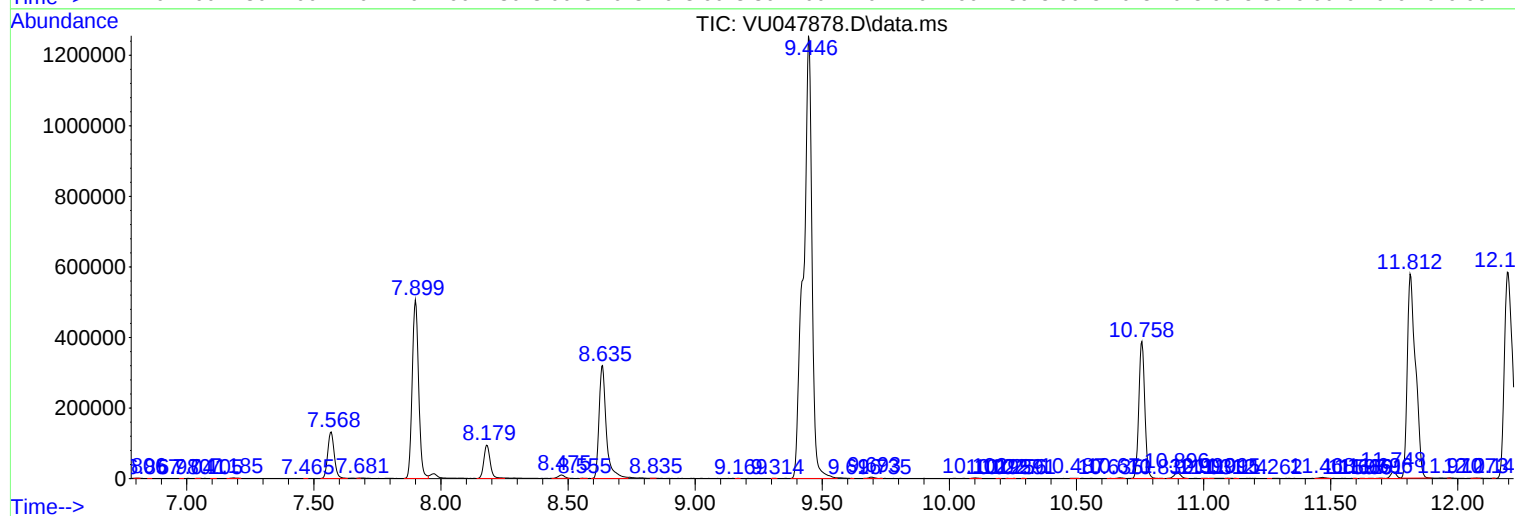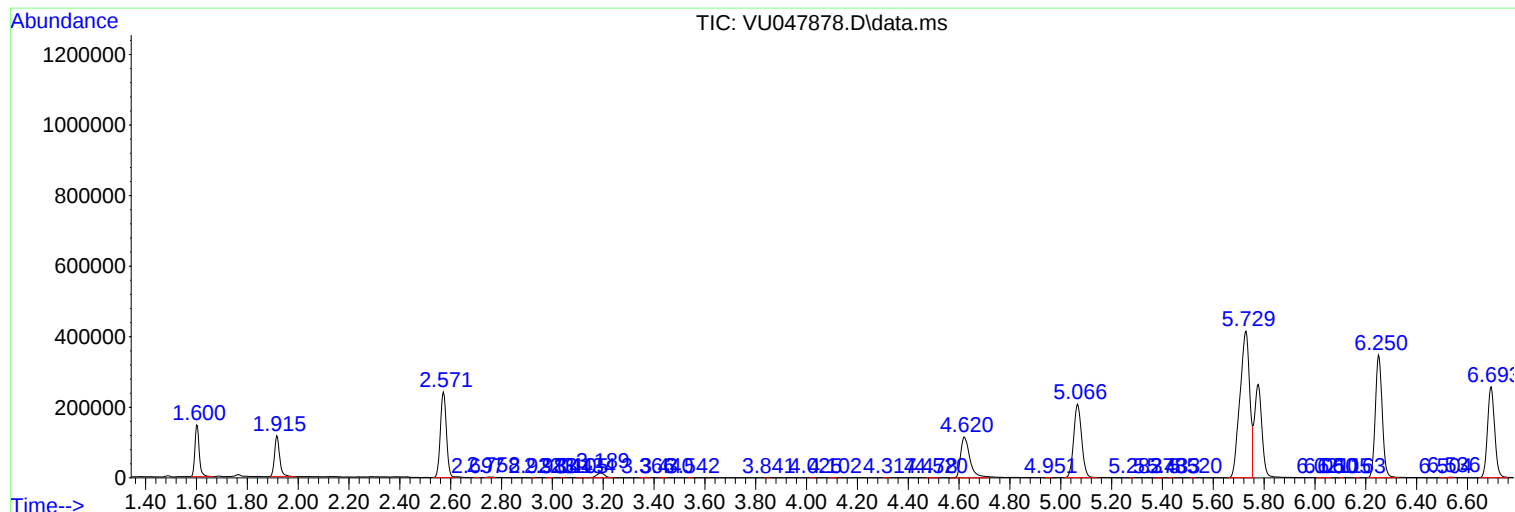

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047878.D
Acq On : 08 Apr 2022 19:42
Operator : SY/MD
Sample : N2343-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047878.D
Acq On : 08 Apr 2022 19:42
Operator : SY/MD
Sample : N2343-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc