

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047879.D
 Acq On : 08 Apr 2022 20:05
 Operator : SY/MD
 Sample : N2343-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047879.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	103	rVB	148904	175388	15.49%	1.922%
2	1.916	170	179	196	rBV	119942	164066	14.49%	1.798%
3	2.571	369	383	396	rBV	244916	402421	35.54%	4.411%
4	2.797	447	453	458	rBV3	802	866	0.08%	0.009%
5	2.954	499	502	507	rBV4	520	469	0.04%	0.005%
6	3.015	518	521	523	rBV2	335	294	0.03%	0.003%
7	3.057	526	534	536	rVV3	494	601	0.05%	0.007%
8	3.147	559	562	564	rVV2	358	258	0.02%	0.003%
9	3.189	564	575	591	rVB2	3025	7734	0.68%	0.085%
10	3.276	597	602	605	rBV3	232	252	0.02%	0.003%
11	3.366	628	630	635	rBV3	529	411	0.04%	0.005%
12	3.430	644	650	652	rBV2	353	285	0.03%	0.003%
13	3.520	672	678	680	rBV2	239	270	0.02%	0.003%
14	3.536	681	683	687	rVB	382	234	0.02%	0.003%
15	3.565	687	692	698	rBV2	265	292	0.03%	0.003%
16	3.597	698	702	705	rBV2	273	259	0.02%	0.003%
17	3.803	759	766	767	rBV	360	299	0.03%	0.003%
18	4.005	824	829	839	rVB2	249	383	0.03%	0.004%
19	4.227	895	898	903	rVB	308	224	0.02%	0.002%
20	4.263	903	909	912	rVB	317	330	0.03%	0.004%
21	4.282	912	915	918	rBV2	276	242	0.02%	0.003%
22	4.356	933	938	942	rVB2	304	350	0.03%	0.004%
23	4.623	1008	1021	1062	rBV2	116667	293489	25.92%	3.217%
24	5.067	1143	1159	1181	rBV	206079	451288	39.85%	4.946%
25	5.192	1196	1198	1203	rVB2	279	219	0.02%	0.002%
26	5.298	1223	1231	1235	rVB4	683	975	0.09%	0.011%
27	5.327	1235	1240	1246	rBV3	464	726	0.06%	0.008%
28	5.539	1302	1306	1314	rVB	349	418	0.04%	0.005%
29	5.578	1314	1318	1320	rBV	301	257	0.02%	0.003%
30	5.729	1342	1365	1398	rBV2	412512	1132365	100.00%	12.411%
31	6.070	1468	1471	1476	rVB3	263	273	0.02%	0.003%
32	6.095	1476	1479	1482	rBV2	307	211	0.02%	0.002%
33	6.118	1482	1486	1490	rBV2	473	419	0.04%	0.005%
34	6.185	1503	1507	1513	rBV3	449	537	0.05%	0.006%
35	6.250	1513	1527	1550	rBV	340691	650225	57.42%	7.127%
36	6.533	1609	1615	1618	rBV6	820	950	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047879.D
 Acq On : 08 Apr 2022 20:05
 Operator : SY/MD
 Sample : N2343-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.581	1623	1630	1631	rBV2	336	373	0.03%	0.004%
38	6.693	1651	1665	1689	rBV	263212	508025	44.86%	5.568%
39	6.960	1743	1748	1752	rBV2	388	359	0.03%	0.004%
40	7.047	1772	1775	1778	rBV2	442	316	0.03%	0.003%
41	7.185	1811	1818	1830	rVB3	1568	2839	0.25%	0.031%
42	7.272	1838	1845	1849	rBV2	250	380	0.03%	0.004%
43	7.472	1904	1907	1911	rBV2	289	258	0.02%	0.003%
44	7.568	1924	1937	1955	rBV	131518	233741	20.64%	2.562%
45	7.684	1967	1973	1974	rBV2	866	775	0.07%	0.008%
46	7.803	2007	2010	2014	rVB2	432	328	0.03%	0.004%
47	7.899	2026	2040	2056	rBV	504695	878493	77.58%	9.629%
48	8.063	2088	2091	2093	rBV2	477	256	0.02%	0.003%
49	8.179	2111	2127	2143	rBV	92929	160910	14.21%	1.764%
50	8.404	2192	2197	2203	rBV3	423	608	0.05%	0.007%
51	8.475	2209	2219	2231	rVB2	9476	15785	1.39%	0.173%
52	8.552	2241	2243	2248	rVB3	471	405	0.04%	0.004%
53	8.632	2256	2268	2296	rBV	341092	639525	56.48%	7.009%
54	8.861	2332	2339	2341	rBV3	410	537	0.05%	0.006%
55	8.944	2362	2365	2369	rBV2	267	252	0.02%	0.003%
56	9.118	2416	2419	2424	rVB3	386	383	0.03%	0.004%
57	9.311	2474	2479	2481	rBV	405	352	0.03%	0.004%
58	9.417	2499	2512	2546	rBV	515855	906368	80.04%	9.934%
59	9.578	2552	2562	2565	rBV3	769	1145	0.10%	0.013%
60	9.619	2571	2575	2576	rBV	335	247	0.02%	0.003%
61	9.697	2590	2599	2606	rBV4	1416	2142	0.19%	0.023%
62	9.774	2620	2623	2628	rVB3	498	515	0.05%	0.006%
63	9.938	2665	2674	2676	rBV3	456	544	0.05%	0.006%
64	10.108	2720	2727	2729	rBV4	794	815	0.07%	0.009%
65	10.195	2751	2754	2763	rVB3	281	432	0.04%	0.005%
66	10.240	2763	2768	2771	rBV	245	246	0.02%	0.003%
67	10.288	2781	2783	2791	rVB3	321	335	0.03%	0.004%
68	10.343	2796	2800	2805	rBV2	205	249	0.02%	0.003%
69	10.484	2839	2844	2847	rBV3	382	424	0.04%	0.005%
70	10.552	2863	2865	2868	rVB	372	217	0.02%	0.002%
71	10.574	2868	2872	2874	rBV	307	273	0.02%	0.003%
72	10.671	2893	2902	2915	rBV4	1763	2806	0.25%	0.031%
73	10.758	2915	2929	2946	rBV	388498	629056	55.55%	6.895%
74	10.893	2961	2971	2984	rVB	15966	26871	2.37%	0.295%
75	11.053	3018	3021	3023	rBV	316	249	0.02%	0.003%
76	11.092	3028	3033	3038	rBV2	726	787	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047879.D
 Acq On : 08 Apr 2022 20:05
 Operator : SY/MD
 Sample : N2343-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.301	3095	3098	3103	rVB2	259	208	0.02%	0.002%
78	11.381	3120	3123	3127	rVB3	360	271	0.02%	0.003%
79	11.404	3127	3130	3135	rBV2	281	215	0.02%	0.002%
80	11.462	3136	3148	3157	rBV7	1621	3293	0.29%	0.036%
81	11.578	3180	3184	3188	rBV2	298	226	0.02%	0.002%
82	11.700	3216	3222	3227	rBV5	850	904	0.08%	0.010%
83	11.748	3231	3237	3245	rVB5	1483	2042	0.18%	0.022%
84	11.812	3245	3257	3282	rBV	553133	905734	79.99%	9.927%
85	11.931	3290	3294	3296	rBV4	601	523	0.05%	0.006%
86	12.066	3327	3336	3347	rBV4	7460	13276	1.17%	0.146%
87	12.195	3361	3376	3395	rBV	529587	872156	77.02%	9.559%
88	12.330	3415	3418	3423	rBV4	624	617	0.05%	0.007%
89	12.391	3436	3437	3440	rBV	428	230	0.02%	0.003%
90	12.520	3474	3477	3481	rVB3	507	326	0.03%	0.004%
91	12.693	3528	3531	3536	rBV3	292	289	0.03%	0.003%
92	12.774	3548	3556	3569	rVB3	3044	5492	0.49%	0.060%
93	12.825	3569	3572	3574	rBV2	358	288	0.03%	0.003%
94	13.082	3650	3652	3656	rBV2	333	240	0.02%	0.003%
95	13.227	3691	3697	3703	rVB4	796	1004	0.09%	0.011%
96	13.844	3882	3889	3901	rVB5	4065	6101	0.54%	0.067%
97	14.092	3960	3966	3976	rBV4	1350	2195	0.19%	0.024%
98	14.934	4224	4228	4231	rBV3	525	440	0.04%	0.005%
99	15.121	4279	4286	4287	rBV2	536	473	0.04%	0.005%
100	15.378	4364	4366	4368	rBV2	454	269	0.02%	0.003%




Sum of corrected areas: 9123713

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047879.D
Acq On : 08 Apr 2022 20:05
Operator : SY/MD
Sample : N2343-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

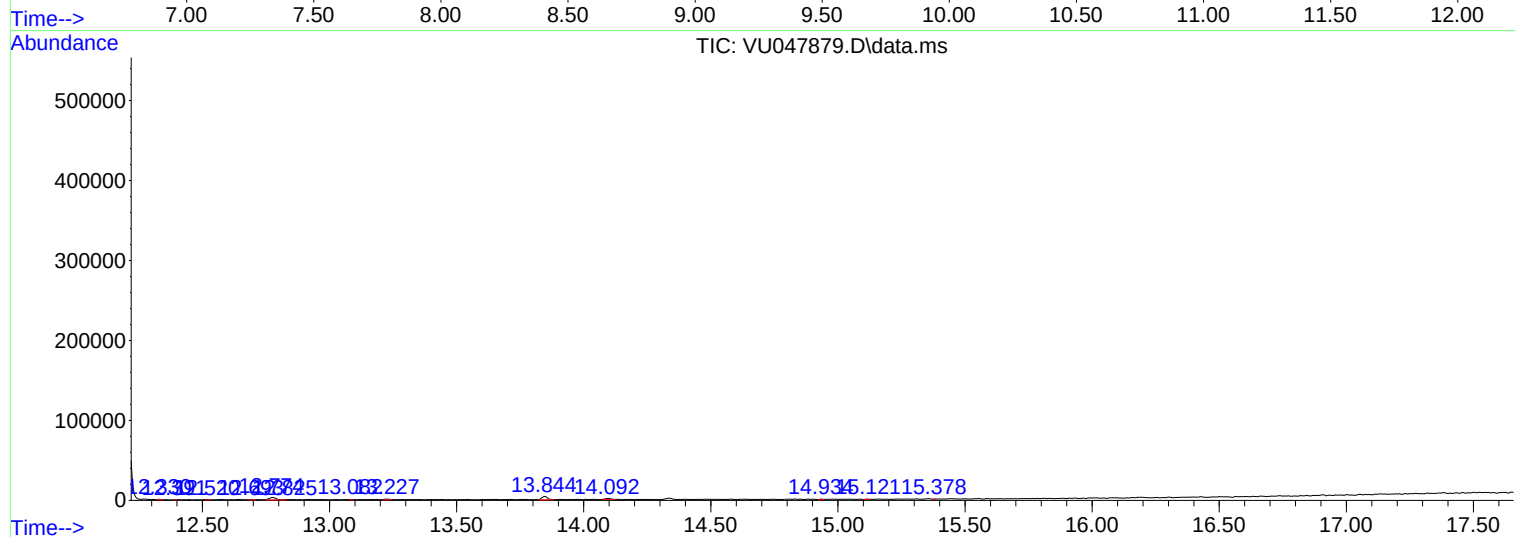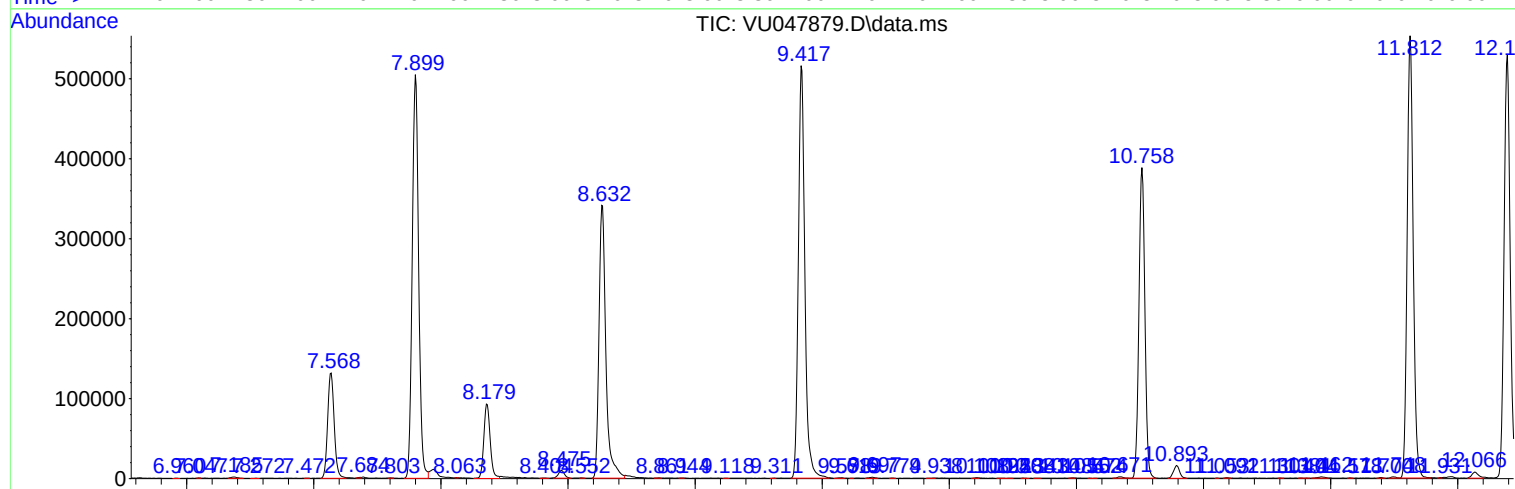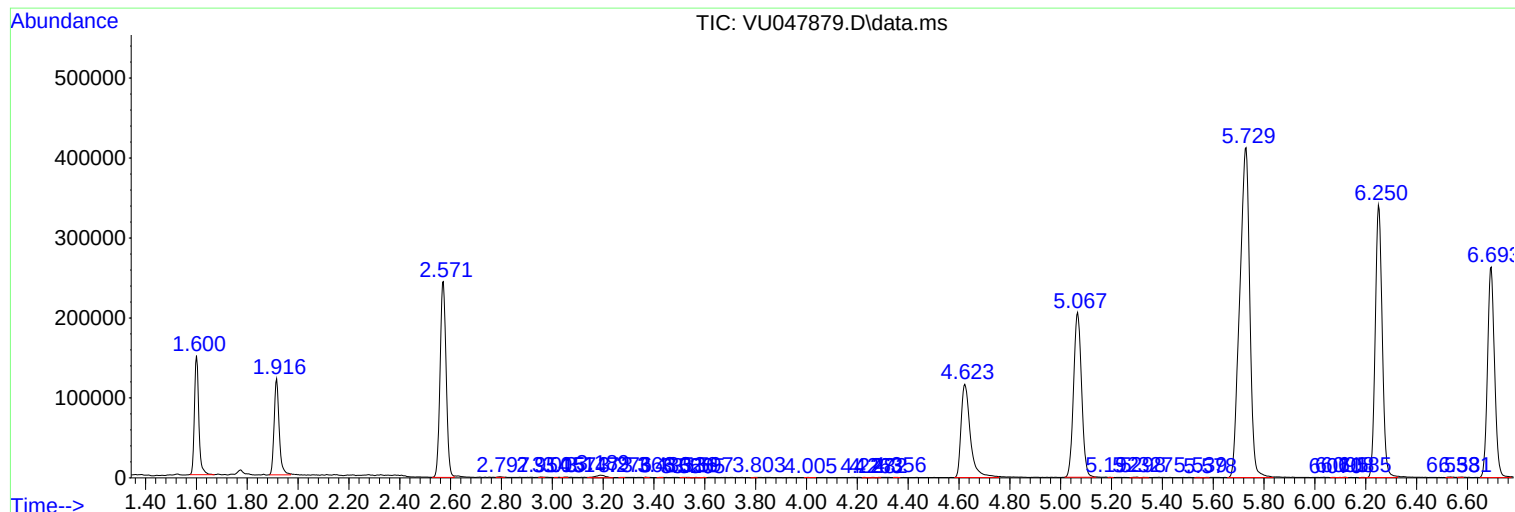

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047879.D
Acq On : 08 Apr 2022 20:05
Operator : SY/MD
Sample : N2343-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047879.D
Acq On : 08 Apr 2022 20:05
Operator : SY/MD
Sample : N2343-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc