

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047880.D
 Acq On : 08 Apr 2022 20:28
 Operator : SY/MD
 Sample : N2343-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	95	rBV	147827	173509	15.27%	1.908%
2	1.916	171	179	196	rBV	118875	161975	14.26%	1.781%
3	2.568	370	382	396	rBV	247750	404437	35.60%	4.448%
4	2.661	409	411	415	rVB2	467	249	0.02%	0.003%
5	2.793	448	452	454	rBV2	624	503	0.04%	0.006%
6	2.964	496	505	508	rBV3	327	479	0.04%	0.005%
7	2.980	508	510	514	rVB2	440	236	0.02%	0.003%
8	3.012	515	520	523	rBV2	232	252	0.02%	0.003%
9	3.105	544	549	552	rBV2	370	384	0.03%	0.004%
10	3.137	556	559	562	rVV2	327	306	0.03%	0.003%
11	3.189	562	575	590	rVV	5779	12943	1.14%	0.142%
12	3.256	593	596	599	rVB	289	212	0.02%	0.002%
13	3.279	599	603	608	rBV2	296	317	0.03%	0.003%
14	3.337	617	621	624	rVB	333	267	0.02%	0.003%
15	3.359	624	628	629	rBV2	435	281	0.02%	0.003%
16	3.456	655	658	662	rVB3	278	185	0.02%	0.002%
17	3.481	662	666	669	rVB2	300	223	0.02%	0.002%
18	3.633	709	713	716	rVV2	191	185	0.02%	0.002%
19	3.764	750	754	757	rBV3	225	202	0.02%	0.002%
20	3.932	802	806	811	rBV2	166	214	0.02%	0.002%
21	3.996	823	826	829	rVV2	281	239	0.02%	0.003%
22	4.105	858	860	864	rVB	295	201	0.02%	0.002%
23	4.173	877	881	885	rBV	226	198	0.02%	0.002%
24	4.353	934	937	940	rBV2	233	189	0.02%	0.002%
25	4.623	1007	1021	1053	rBV	117125	291894	25.70%	3.210%
26	4.861	1092	1095	1097	rBV2	317	199	0.02%	0.002%
27	5.067	1142	1159	1182	rVV	208105	453057	39.88%	4.982%
28	5.282	1222	1226	1228	rBV	571	465	0.04%	0.005%
29	5.549	1306	1309	1312	rVB2	258	190	0.02%	0.002%
30	5.594	1318	1323	1325	rBV2	201	198	0.02%	0.002%
31	5.726	1343	1364	1393	rBV2	415639	1135941	100.00%	12.492%
32	5.951	1431	1434	1436	rBV2	335	194	0.02%	0.002%
33	6.025	1453	1457	1461	rBV2	321	322	0.03%	0.004%
34	6.128	1483	1489	1492	rVB3	447	505	0.04%	0.006%
35	6.250	1508	1527	1547	rBV	335729	645318	56.81%	7.097%
36	6.494	1601	1603	1607	rVB	309	226	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047880.D
 Acq On : 08 Apr 2022 20:28
 Operator : SY/MD
 Sample : N2343-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.533	1610	1615	1616	rBV	814	646	0.06%	0.007%
38	6.587	1630	1632	1637	rVB3	318	186	0.02%	0.002%
39	6.693	1650	1665	1689	rBV	259987	511234	45.01%	5.622%
40	6.851	1709	1714	1716	rBV3	495	327	0.03%	0.004%
41	6.890	1719	1726	1728	rBV2	192	203	0.02%	0.002%
42	7.047	1769	1775	1776	rBV2	328	279	0.02%	0.003%
43	7.128	1797	1800	1804	rVB2	260	202	0.02%	0.002%
44	7.147	1804	1806	1810	rBV3	238	207	0.02%	0.002%
45	7.185	1810	1818	1829	rVV3	1601	2852	0.25%	0.031%
46	7.304	1851	1855	1857	rBV2	272	193	0.02%	0.002%
47	7.333	1862	1864	1868	rVB3	286	212	0.02%	0.002%
48	7.362	1868	1873	1876	rBV2	334	307	0.03%	0.003%
49	7.497	1911	1915	1919	rVB3	337	332	0.03%	0.004%
50	7.568	1919	1937	1961	rBV	130469	236593	20.83%	2.602%
51	7.687	1968	1974	1991	rVB7	1727	3540	0.31%	0.039%
52	7.787	2000	2005	2006	rBV2	622	425	0.04%	0.005%
53	7.899	2024	2040	2056	rBV	506327	884574	77.87%	9.728%
54	8.182	2114	2128	2144	rBV	91140	159240	14.02%	1.751%
55	8.346	2177	2179	2188	rVB	575	590	0.05%	0.006%
56	8.472	2207	2218	2229	rBV	8766	14969	1.32%	0.165%
57	8.552	2240	2243	2244	rBV	324	187	0.02%	0.002%
58	8.632	2256	2268	2303	rBV	340772	651096	57.32%	7.160%
59	8.922	2353	2358	2362	rBV3	494	509	0.04%	0.006%
60	9.127	2418	2422	2425	rVB2	380	254	0.02%	0.003%
61	9.253	2458	2461	2465	rVB2	374	282	0.02%	0.003%
62	9.420	2499	2513	2552	rVB	503857	884344	77.85%	9.725%
63	9.552	2552	2554	2557	rBV2	296	243	0.02%	0.003%
64	9.568	2557	2559	2562	rBV2	461	291	0.03%	0.003%
65	9.690	2592	2597	2600	rBV4	1031	1082	0.10%	0.012%
66	9.832	2638	2641	2644	rVB2	381	236	0.02%	0.003%
67	9.954	2676	2679	2683	rBV	344	276	0.02%	0.003%
68	9.989	2686	2690	2693	rBV	276	212	0.02%	0.002%
69	10.172	2742	2747	2748	rBV	251	194	0.02%	0.002%
70	10.398	2815	2817	2819	rBV	325	208	0.02%	0.002%
71	10.468	2835	2839	2840	rBV	272	189	0.02%	0.002%
72	10.481	2840	2843	2846	rVV2	302	237	0.02%	0.003%
73	10.561	2866	2868	2874	rVB2	418	329	0.03%	0.004%
74	10.600	2874	2880	2883	rBV2	308	307	0.03%	0.003%
75	10.623	2883	2887	2889	rBV2	247	208	0.02%	0.002%
76	10.671	2894	2902	2913	rVB4	1895	2798	0.25%	0.031%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047880.D
 Acq On : 08 Apr 2022 20:28
 Operator : SY/MD
 Sample : N2343-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.758	2917	2929	2950	rVB	393888	637883	56.15%	7.015%
78	10.896	2960	2972	2984	rBV2	13003	23304	2.05%	0.256%
79	11.089	3026	3032	3034	rBV3	438	436	0.04%	0.005%
80	11.198	3062	3066	3068	rBV	354	242	0.02%	0.003%
81	11.291	3091	3095	3098	rBV2	315	288	0.03%	0.003%
82	11.369	3114	3119	3122	rVB2	256	244	0.02%	0.003%
83	11.391	3122	3126	3128	rBV	346	246	0.02%	0.003%
84	11.462	3138	3148	3150	rBV4	1591	2027	0.18%	0.022%
85	11.700	3217	3222	3227	rVB5	703	806	0.07%	0.009%
86	11.745	3230	3236	3245	rVB5	1434	1934	0.17%	0.021%
87	11.812	3245	3257	3273	rBV	545710	882415	77.68%	9.704%
88	11.938	3293	3296	3298	rBV2	567	340	0.03%	0.004%
89	12.066	3326	3336	3345	rBV3	7919	13182	1.16%	0.145%
90	12.195	3359	3376	3398	rBV	525357	871106	76.69%	9.580%
91	12.272	3398	3400	3409	rVB6	834	834	0.07%	0.009%
92	12.471	3457	3462	3468	rBV3	368	596	0.05%	0.007%
93	12.780	3550	3558	3570	rVB5	1477	2291	0.20%	0.025%
94	12.960	3609	3614	3617	rBV	343	401	0.04%	0.004%
95	13.227	3691	3697	3705	rBV2	766	1003	0.09%	0.011%
96	13.529	3789	3791	3794	rBV2	288	188	0.02%	0.002%
97	13.851	3885	3891	3897	rVB4	2116	2821	0.25%	0.031%
98	14.098	3964	3968	3973	rVB2	1105	872	0.08%	0.010%
99	14.336	4036	4042	4052	rBV6	1593	2274	0.20%	0.025%
100	15.024	4254	4256	4260	rBV	463	352	0.03%	0.004%




Sum of corrected areas: 9093373

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047880.D
Acq On : 08 Apr 2022 20:28
Operator : SY/MD
Sample : N2343-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

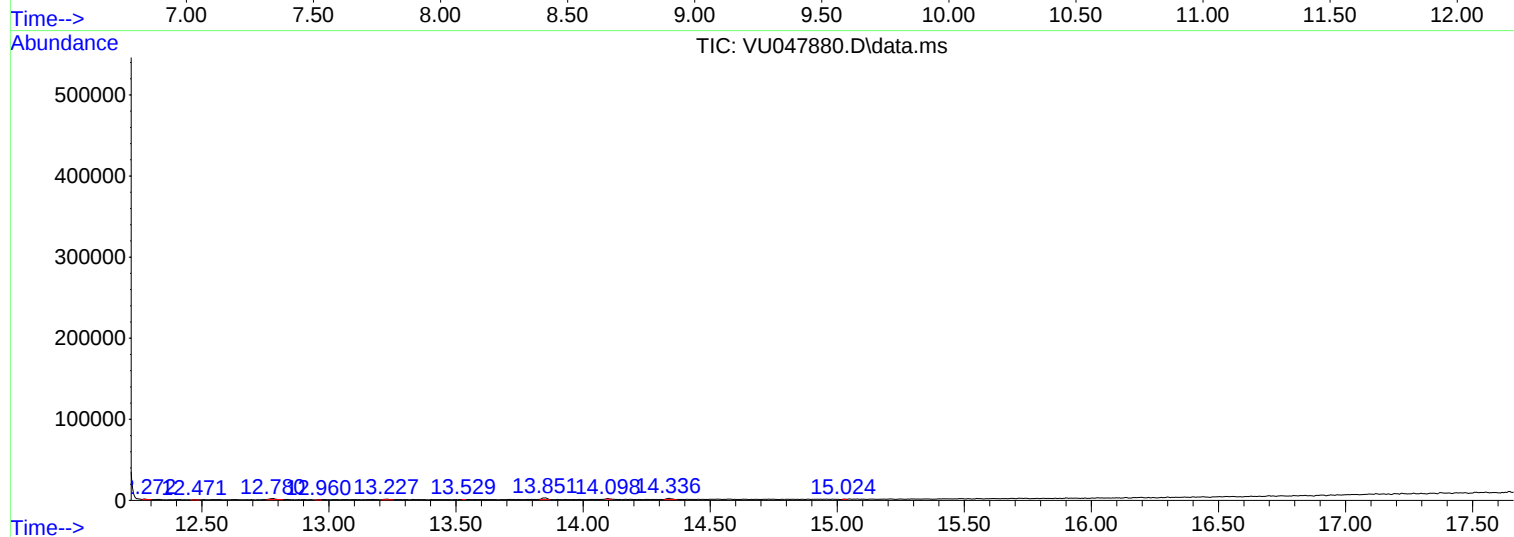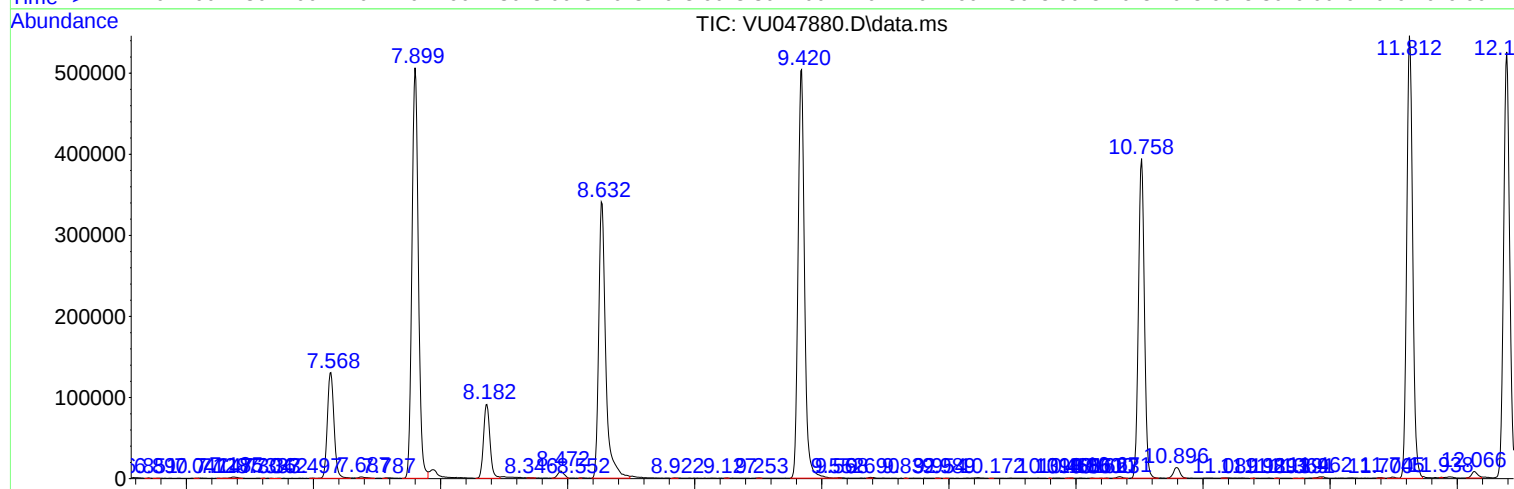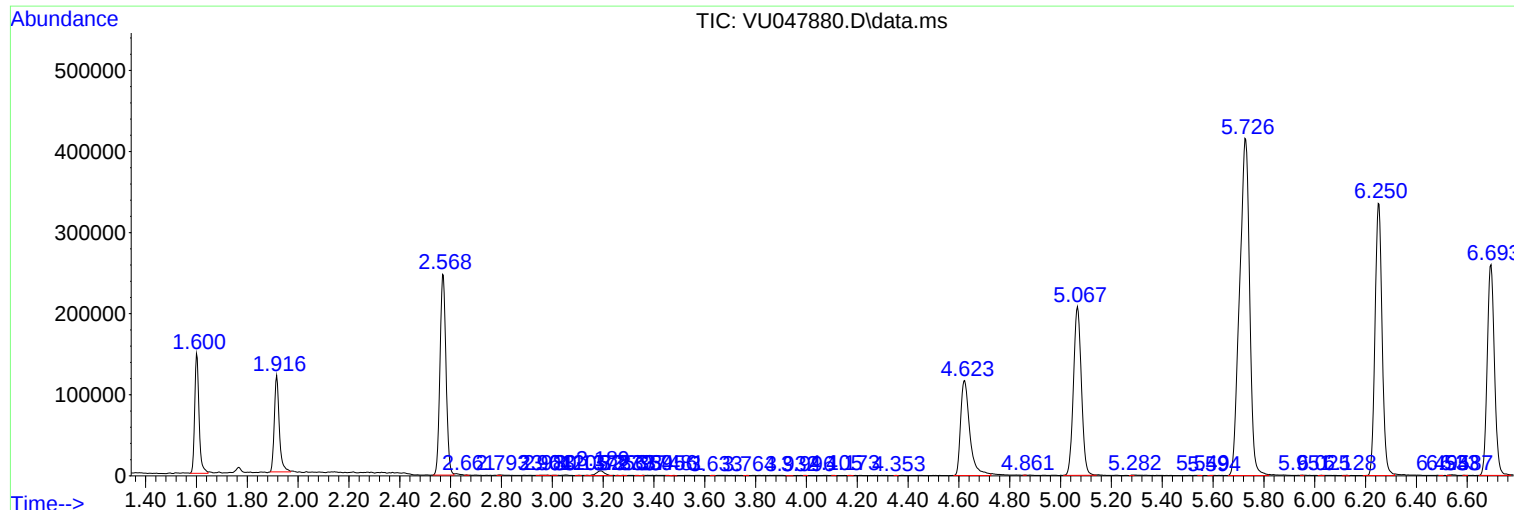

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047880.D
Acq On : 08 Apr 2022 20:28
Operator : SY/MD
Sample : N2343-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047880.D
Acq On : 08 Apr 2022 20:28
Operator : SY/MD
Sample : N2343-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------