

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047883.D
 Acq On : 08 Apr 2022 21:38
 Operator : SY/MD
 Sample : N2343-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047883.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rBV	149426	181802	15.88%	2.001%
2	1.916	171	179	197	rVB	117798	162235	14.17%	1.786%
3	2.569	367	382	399	rBV	248558	406621	35.51%	4.476%
4	2.681	414	417	419	rBV2	372	231	0.02%	0.003%
5	2.749	435	438	439	rBV2	535	296	0.03%	0.003%
6	2.829	460	463	467	rBV3	239	228	0.02%	0.003%
7	2.848	467	469	475	rVB2	282	192	0.02%	0.002%
8	2.909	485	488	492	rBV	624	635	0.06%	0.007%
9	3.012	516	520	525	rBV3	312	309	0.03%	0.003%
10	3.057	527	534	540	rVB4	725	963	0.08%	0.011%
11	3.189	562	575	587	rVB	5436	11008	0.96%	0.121%
12	3.392	635	638	640	rBV2	332	191	0.02%	0.002%
13	3.607	702	705	709	rVB	293	212	0.02%	0.002%
14	3.655	716	720	723	rVB2	328	276	0.02%	0.003%
15	3.758	748	752	755	rBV2	319	296	0.03%	0.003%
16	3.797	760	764	767	rVB2	288	236	0.02%	0.003%
17	3.819	767	771	776	rVB	336	320	0.03%	0.004%
18	3.858	776	783	787	rBV3	427	499	0.04%	0.005%
19	3.900	792	796	799	rBV2	325	297	0.03%	0.003%
20	3.916	799	801	806	rVB2	323	236	0.02%	0.003%
21	3.951	806	812	814	rBV2	223	203	0.02%	0.002%
22	4.031	835	837	840	rVB	328	183	0.02%	0.002%
23	4.144	868	872	875	rVB2	229	194	0.02%	0.002%
24	4.167	875	879	882	rVB2	328	254	0.02%	0.003%
25	4.189	882	886	892	rBV2	543	637	0.06%	0.007%
26	4.224	892	897	900	rBV2	309	261	0.02%	0.003%
27	4.276	909	913	916	rBV2	257	274	0.02%	0.003%
28	4.337	929	932	937	rVB2	231	217	0.02%	0.002%
29	4.392	947	949	953	rVV	285	207	0.02%	0.002%
30	4.482	972	977	980	rBV2	207	192	0.02%	0.002%
31	4.623	1007	1021	1058	rBV	120110	297255	25.96%	3.272%
32	5.067	1137	1159	1182	rBV	210033	461361	40.29%	5.078%
33	5.215	1202	1205	1211	rVB3	408	356	0.03%	0.004%
34	5.295	1223	1230	1236	rBV3	645	918	0.08%	0.010%
35	5.353	1246	1248	1253	rVB2	336	242	0.02%	0.003%
36	5.379	1253	1256	1258	rBV	303	185	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047883.D
 Acq On : 08 Apr 2022 21:38
 Operator : SY/MD
 Sample : N2343-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.469	1281	1284	1290	rBV2	232	273	0.02%	0.003%
38	5.565	1312	1314	1320	rVB2	305	265	0.02%	0.003%
39	5.636	1332	1336	1338	rBV2	184	190	0.02%	0.002%
40	5.726	1342	1364	1396	rBV2	422074	1145188	100.00%	12.605%
41	5.967	1436	1439	1441	rVB2	381	194	0.02%	0.002%
42	6.015	1451	1454	1458	rVB3	305	256	0.02%	0.003%
43	6.099	1474	1480	1481	rBV2	243	209	0.02%	0.002%
44	6.189	1504	1508	1511	rBV2	355	283	0.02%	0.003%
45	6.250	1513	1527	1545	rBV	339539	640299	55.91%	7.048%
46	6.430	1579	1583	1585	rBV3	431	289	0.03%	0.003%
47	6.523	1608	1612	1613	rBV2	622	416	0.04%	0.005%
48	6.533	1613	1615	1621	rVB4	783	792	0.07%	0.009%
49	6.584	1628	1631	1634	rVB2	321	229	0.02%	0.003%
50	6.694	1649	1665	1690	rVV	260607	515268	44.99%	5.672%
51	7.182	1810	1817	1826	rBV5	1506	2565	0.22%	0.028%
52	7.221	1826	1829	1835	rVB2	388	350	0.03%	0.004%
53	7.298	1849	1853	1856	rBV2	234	230	0.02%	0.003%
54	7.568	1924	1937	1954	rBV	132076	234089	20.44%	2.577%
55	7.745	1989	1992	1998	rBV3	295	317	0.03%	0.003%
56	7.790	2004	2006	2009	rVB3	443	199	0.02%	0.002%
57	7.899	2026	2040	2057	rBV	509226	890187	77.73%	9.798%
58	8.179	2115	2127	2147	rBV	90927	159678	13.94%	1.758%
59	8.475	2203	2219	2231	rBV3	5362	10461	0.91%	0.115%
60	8.552	2240	2243	2247	rVB2	949	512	0.04%	0.006%
61	8.633	2256	2268	2304	rBV	344248	664241	58.00%	7.311%
62	8.916	2354	2356	2361	rVB3	408	278	0.02%	0.003%
63	8.973	2369	2374	2376	rBV	223	216	0.02%	0.002%
64	9.015	2383	2387	2390	rBV3	228	231	0.02%	0.003%
65	9.311	2477	2479	2482	rVB2	309	178	0.02%	0.002%
66	9.337	2483	2487	2491	rBV3	278	275	0.02%	0.003%
67	9.417	2498	2512	2536	rBV	512897	877701	76.64%	9.661%
68	9.575	2558	2561	2566	rVB3	804	751	0.07%	0.008%
69	9.697	2591	2599	2605	rBV2	995	1530	0.13%	0.017%
70	9.970	2680	2684	2691	rBV3	219	299	0.03%	0.003%
71	10.067	2712	2714	2717	rVB2	365	196	0.02%	0.002%
72	10.096	2717	2723	2724	rBV	424	385	0.03%	0.004%
73	10.411	2817	2821	2825	rBV2	353	362	0.03%	0.004%
74	10.533	2856	2859	2862	rBV2	240	186	0.02%	0.002%
75	10.671	2894	2902	2911	rBV3	1714	2423	0.21%	0.027%
76	10.758	2916	2929	2953	rVB	394366	646778	56.48%	7.119%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047883.D
 Acq On : 08 Apr 2022 21:38
 Operator : SY/MD
 Sample : N2343-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.896	2958	2972	2983	rVB2	8831	15342	1.34%	0.169%
78	11.038	3012	3016	3021	rVB2	422	500	0.04%	0.006%
79	11.063	3021	3024	3028	rBV2	391	371	0.03%	0.004%
80	11.096	3030	3034	3040	rVV3	504	574	0.05%	0.006%
81	11.124	3041	3043	3047	rVB2	606	324	0.03%	0.004%
82	11.147	3047	3050	3053	rBV2	315	280	0.02%	0.003%
83	11.269	3085	3088	3090	rBV2	335	223	0.02%	0.002%
84	11.459	3140	3147	3152	rBV6	1516	2029	0.18%	0.022%
85	11.642	3201	3204	3208	rBV2	252	203	0.02%	0.002%
86	11.694	3217	3220	3221	rBV2	684	399	0.03%	0.004%
87	11.748	3233	3237	3239	rBV3	685	516	0.05%	0.006%
88	11.813	3244	3257	3277	rBV	528891	863816	75.43%	9.508%
89	12.070	3327	3337	3348	rBV6	4921	8999	0.79%	0.099%
90	12.195	3361	3376	3399	rBV	520616	856365	74.78%	9.426%
91	12.333	3416	3419	3422	rVB5	408	294	0.03%	0.003%
92	12.581	3492	3496	3500	rVB4	389	373	0.03%	0.004%
93	12.645	3512	3516	3518	rBV3	430	369	0.03%	0.004%
94	12.713	3533	3537	3539	rBV2	311	257	0.02%	0.003%
95	12.771	3549	3555	3565	rVB4	1091	1772	0.15%	0.020%
96	13.012	3628	3630	3633	rVB	408	205	0.02%	0.002%
97	13.369	3738	3741	3745	rBV3	383	260	0.02%	0.003%
98	13.848	3883	3890	3894	rBV5	1221	1704	0.15%	0.019%
99	14.063	3951	3957	3960	rBV2	510	654	0.06%	0.007%
100	14.902	4216	4218	4223	rBV2	456	332	0.03%	0.004%




Sum of corrected areas: 9084952

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047883.D
Acq On : 08 Apr 2022 21:38
Operator : SY/MD
Sample : N2343-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

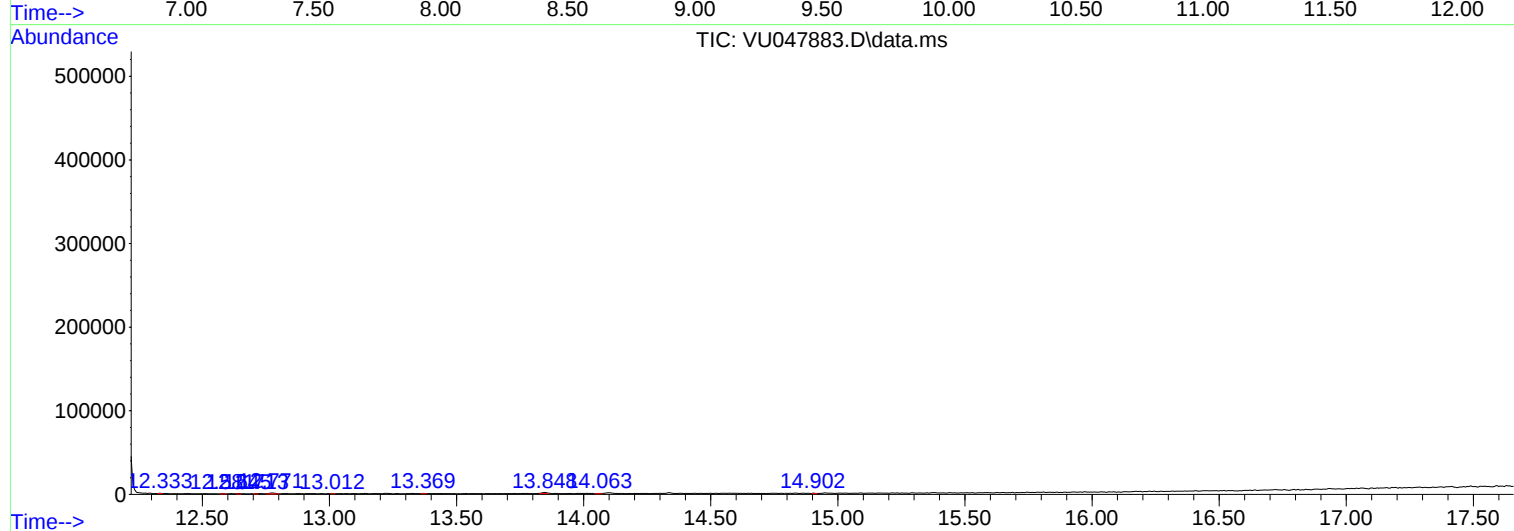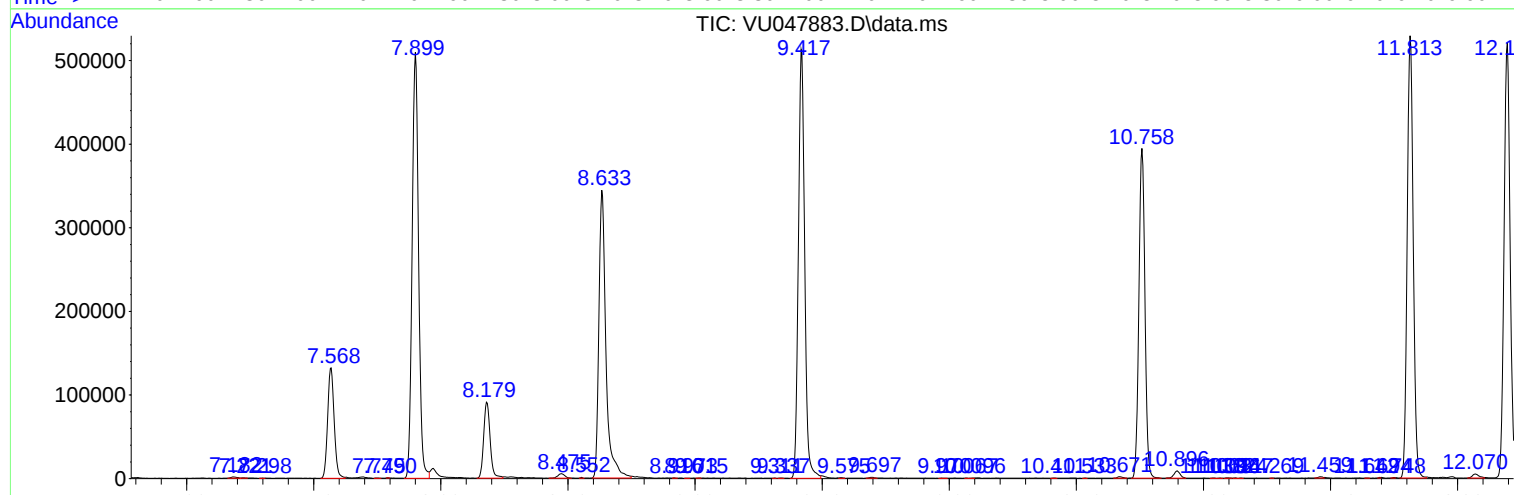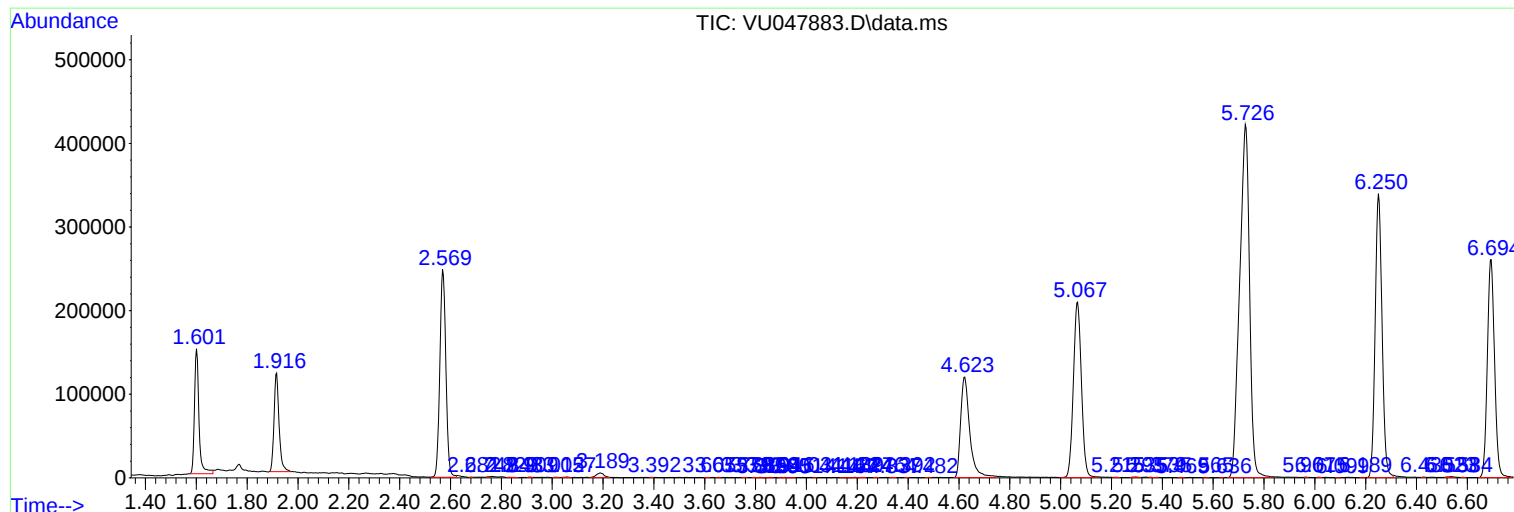

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047883.D
Acq On : 08 Apr 2022 21:38
Operator : SY/MD
Sample : N2343-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047883.D
Acq On : 08 Apr 2022 21:38
Operator : SY/MD
Sample : N2343-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc