

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047884.D
 Acq On : 08 Apr 2022 22:01
 Operator : SY/MD
 Sample : N2343-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	96	rBV	145233	167614	14.61%	1.841%
2	1.916	171	179	201	rVB	117102	163033	14.21%	1.790%
3	2.568	370	382	398	rBV	247191	404383	35.24%	4.441%
4	2.716	426	428	432	rVB3	441	333	0.03%	0.004%
5	2.755	432	440	448	rBV4	3304	5963	0.52%	0.065%
6	2.916	485	490	494	rBV2	434	368	0.03%	0.004%
7	2.957	499	503	505	rVV2	384	365	0.03%	0.004%
8	2.973	505	508	513	rVB3	480	409	0.04%	0.004%
9	3.034	523	527	528	rBV	384	208	0.02%	0.002%
10	3.047	528	531	533	rVV2	337	251	0.02%	0.003%
11	3.105	543	549	551	rBV2	342	370	0.03%	0.004%
12	3.192	561	576	590	rVB2	13177	28977	2.53%	0.318%
13	3.359	625	628	631	rBV3	274	214	0.02%	0.002%
14	3.491	666	669	674	rVB	315	229	0.02%	0.003%
15	3.613	705	707	711	rVB2	260	212	0.02%	0.002%
16	3.854	778	782	785	rBV	239	228	0.02%	0.003%
17	3.996	824	826	830	rVB2	402	270	0.02%	0.003%
18	4.057	843	845	853	rVB	413	364	0.03%	0.004%
19	4.321	924	927	936	rVB	286	419	0.04%	0.005%
20	4.452	965	968	971	rBV	217	210	0.02%	0.002%
21	4.623	1006	1021	1058	rBV	119836	300503	26.19%	3.300%
22	4.886	1100	1103	1107	rBV3	332	318	0.03%	0.003%
23	5.067	1142	1159	1182	rBV	210461	459754	40.06%	5.049%
24	5.227	1207	1209	1213	rVB2	544	346	0.03%	0.004%
25	5.253	1213	1217	1218	rBV	364	284	0.02%	0.003%
26	5.292	1223	1229	1236	rBV4	902	1268	0.11%	0.014%
27	5.729	1342	1365	1398	rVV2	419885	1147548	100.00%	12.602%
28	5.925	1423	1426	1432	rVB3	255	277	0.02%	0.003%
29	6.018	1450	1455	1457	rBV2	281	288	0.03%	0.003%
30	6.115	1482	1485	1492	rBV2	385	527	0.05%	0.006%
31	6.250	1513	1527	1554	rBV	345898	657672	57.31%	7.223%
32	6.394	1569	1572	1580	rVB4	389	443	0.04%	0.005%
33	6.427	1580	1582	1586	rVB3	464	321	0.03%	0.004%
34	6.533	1608	1615	1620	rBV4	1027	1360	0.12%	0.015%
35	6.626	1638	1644	1646	rBV2	432	359	0.03%	0.004%
36	6.693	1650	1665	1686	rBV	262330	512231	44.64%	5.625%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047884.D
 Acq On : 08 Apr 2022 22:01
 Operator : SY/MD
 Sample : N2343-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.044	1769	1774	1777	rBV2	394	484	0.04%	0.005%
38	7.153	1804	1808	1811	rBV	245	236	0.02%	0.003%
39	7.179	1811	1816	1817	rBV3	1358	1094	0.10%	0.012%
40	7.314	1852	1858	1860	rBV	253	223	0.02%	0.002%
41	7.362	1870	1873	1879	rVB2	249	283	0.02%	0.003%
42	7.491	1908	1913	1916	rBV2	316	241	0.02%	0.003%
43	7.568	1920	1937	1960	rVV2	130103	236077	20.57%	2.593%
44	7.681	1965	1972	1973	rBV2	1004	756	0.07%	0.008%
45	7.793	2005	2007	2011	rVV2	330	208	0.02%	0.002%
46	7.899	2026	2040	2056	rBV	503698	885885	77.20%	9.729%
47	8.179	2116	2127	2150	rVV	93302	161912	14.11%	1.778%
48	8.414	2197	2200	2203	rBV2	431	323	0.03%	0.004%
49	8.475	2208	2219	2234	rVV3	5219	9698	0.85%	0.107%
50	8.558	2240	2245	2249	rVB4	407	353	0.03%	0.004%
51	8.632	2256	2268	2306	rBV	332073	654710	57.05%	7.190%
52	8.880	2343	2345	2349	rVB	451	289	0.03%	0.003%
53	8.906	2349	2353	2356	rBV2	285	279	0.02%	0.003%
54	8.922	2356	2358	2363	rVB2	374	265	0.02%	0.003%
55	8.992	2376	2380	2384	rVB4	374	327	0.03%	0.004%
56	9.134	2420	2424	2429	rBV3	205	252	0.02%	0.003%
57	9.234	2451	2455	2458	rBV	376	281	0.02%	0.003%
58	9.266	2462	2465	2470	rVB	360	310	0.03%	0.003%
59	9.340	2483	2488	2491	rBV	277	257	0.02%	0.003%
60	9.417	2498	2512	2539	rBV	515187	889555	77.52%	9.769%
61	9.574	2556	2561	2569	rVB5	636	809	0.07%	0.009%
62	9.697	2592	2599	2609	rVB2	1099	1467	0.13%	0.016%
63	9.825	2636	2639	2642	rVB2	332	239	0.02%	0.003%
64	9.851	2642	2647	2653	rVB	312	400	0.03%	0.004%
65	9.883	2653	2657	2662	rBV2	411	427	0.04%	0.005%
66	10.057	2708	2711	2714	rBV2	296	210	0.02%	0.002%
67	10.089	2715	2721	2722	rBV	413	307	0.03%	0.003%
68	10.217	2756	2761	2767	rVB2	265	328	0.03%	0.004%
69	10.320	2790	2793	2799	rBV2	411	374	0.03%	0.004%
70	10.443	2827	2831	2836	rVB	350	253	0.02%	0.003%
71	10.471	2836	2840	2841	rBV	423	280	0.02%	0.003%
72	10.671	2895	2902	2910	rBV4	1555	2110	0.18%	0.023%
73	10.758	2916	2929	2949	rBV	397982	644840	56.19%	7.082%
74	10.896	2959	2972	2982	rBV2	6898	12705	1.11%	0.140%
75	11.089	3026	3032	3035	rBV4	520	545	0.05%	0.006%
76	11.417	3129	3134	3138	rVB	440	332	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047884.D
 Acq On : 08 Apr 2022 22:01
 Operator : SY/MD
 Sample : N2343-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.459	3138	3147	3161	rVB5	1649	3334	0.29%	0.037%
78	11.523	3161	3167	3170	rBV3	373	348	0.03%	0.004%
79	11.610	3191	3194	3200	rBV	242	264	0.02%	0.003%
80	11.651	3203	3207	3214	rVV2	344	479	0.04%	0.005%
81	11.703	3218	3223	3229	rVB5	815	831	0.07%	0.009%
82	11.751	3234	3238	3243	rBV3	609	711	0.06%	0.008%
83	11.812	3245	3257	3275	rBV	528019	872089	76.00%	9.577%
84	11.925	3290	3292	3295	rBV2	342	231	0.02%	0.003%
85	11.944	3295	3298	3302	rVV4	896	644	0.06%	0.007%
86	11.976	3302	3308	3314	rVB6	1235	1536	0.13%	0.017%
87	12.069	3329	3337	3346	rVV6	1652	3215	0.28%	0.035%
88	12.195	3361	3376	3394	rVV	523852	848567	73.95%	9.319%
89	12.397	3435	3439	3443	rBV3	499	452	0.04%	0.005%
90	12.459	3452	3458	3460	rBV2	305	353	0.03%	0.004%
91	12.645	3513	3516	3521	rVB2	414	330	0.03%	0.004%
92	12.693	3526	3531	3539	rBV2	405	513	0.04%	0.006%
93	12.774	3550	3556	3563	rBV3	758	929	0.08%	0.010%
94	12.905	3594	3597	3599	rBV2	311	213	0.02%	0.002%
95	12.947	3607	3610	3612	rBV2	338	210	0.02%	0.002%
96	13.147	3670	3672	3678	rBV4	402	283	0.02%	0.003%
97	13.854	3885	3892	3898	rVB5	1072	1437	0.13%	0.016%
98	14.687	4149	4151	4156	rBV3	359	381	0.03%	0.004%
99	14.909	4218	4220	4222	rBV	424	217	0.02%	0.002%
100	15.696	4463	4465	4468	rBV4	704	339	0.03%	0.004%




Sum of corrected areas: 9105749

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047884.D
Acq On : 08 Apr 2022 22:01
Operator : SY/MD
Sample : N2343-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

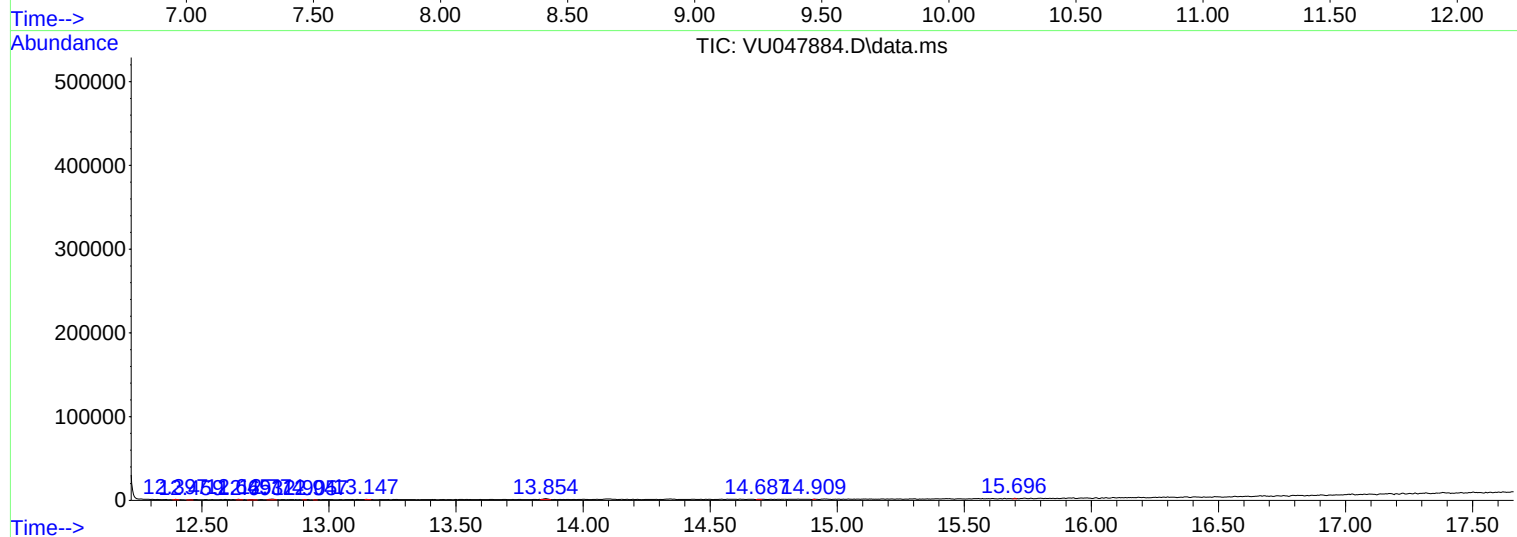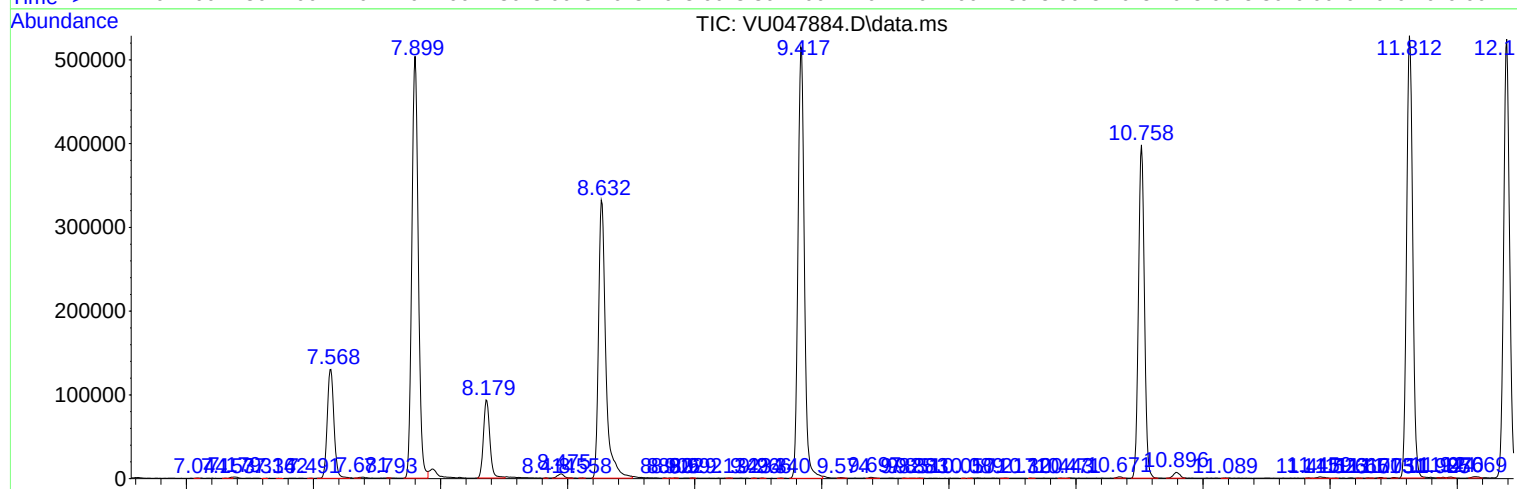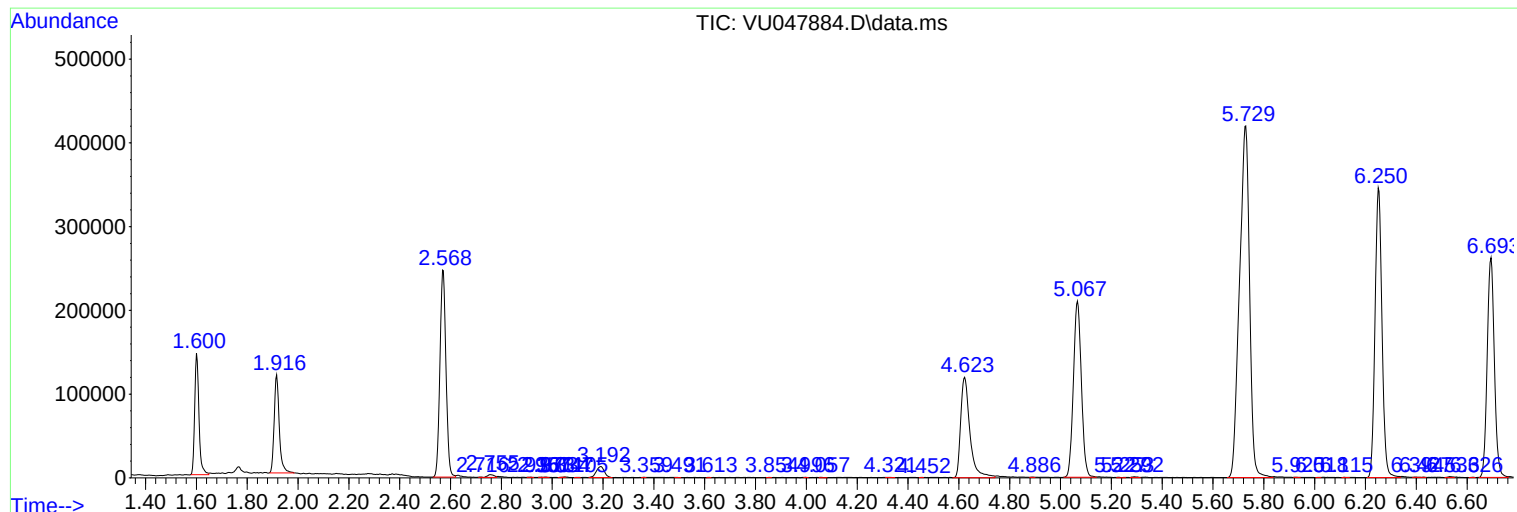

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047884.D
Acq On : 08 Apr 2022 22:01
Operator : SY/MD
Sample : N2343-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047884.D
Acq On : 08 Apr 2022 22:01
Operator : SY/MD
Sample : N2343-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc