

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047890.D
 Acq On : 09 Apr 2022 00:19
 Operator : SY/MD
 Sample : N2345-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047890.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rVB	159124	183052	9.96%	1.647%
2	1.916	171	179	196	rBV	120316	165138	8.98%	1.486%
3	2.568	370	382	397	rBV	260066	426901	23.22%	3.842%
4	2.745	434	437	441	rBV2	335	267	0.01%	0.002%
5	2.797	449	453	455	rBV3	500	487	0.03%	0.004%
6	2.842	464	467	469	rBV2	378	266	0.01%	0.002%
7	3.189	563	575	593	rVB2	4727	10918	0.59%	0.098%
8	3.276	599	602	606	rBV3	292	230	0.01%	0.002%
9	3.491	665	669	675	rBV3	278	284	0.02%	0.003%
10	3.539	680	684	687	rBV3	314	251	0.01%	0.002%
11	3.703	731	735	738	rBV2	394	424	0.02%	0.004%
12	3.748	744	749	752	rBV2	315	306	0.02%	0.003%
13	3.784	757	760	764	rBV2	330	307	0.02%	0.003%
14	3.838	773	777	778	rBV2	378	249	0.01%	0.002%
15	3.877	782	789	791	rVB3	463	452	0.02%	0.004%
16	3.938	804	808	812	rBV2	434	423	0.02%	0.004%
17	4.022	831	834	840	rVB3	318	263	0.01%	0.002%
18	4.070	845	849	851	rBV2	393	272	0.01%	0.002%
19	4.430	957	961	966	rBV2	290	237	0.01%	0.002%
20	4.514	984	987	990	rVB2	419	237	0.01%	0.002%
21	4.533	990	993	999	rVB3	368	290	0.02%	0.003%
22	4.559	999	1001	1008	rVB2	273	231	0.01%	0.002%
23	4.623	1008	1021	1048	rBV	132767	323535	17.60%	2.912%
24	4.890	1102	1104	1107	rBV	290	223	0.01%	0.002%
25	5.067	1143	1159	1185	rBV	220190	487415	26.51%	4.386%
26	5.227	1208	1209	1215	rVB2	421	277	0.02%	0.002%
27	5.288	1223	1228	1229	rBV2	691	554	0.03%	0.005%
28	5.324	1236	1239	1242	rBV4	270	249	0.01%	0.002%
29	5.385	1254	1258	1259	rBV2	408	285	0.02%	0.003%
30	5.475	1283	1286	1291	rVB3	281	230	0.01%	0.002%
31	5.536	1300	1305	1309	rBV3	421	473	0.03%	0.004%
32	5.613	1325	1329	1331	rBV	327	265	0.01%	0.002%
33	5.726	1341	1364	1373	rBV2	450577	1222724	66.50%	11.003%
34	5.973	1438	1441	1446	rBV4	470	465	0.03%	0.004%
35	6.073	1469	1472	1475	rBV2	443	345	0.02%	0.003%
36	6.173	1500	1503	1507	rVB3	465	324	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047890.D
 Acq On : 09 Apr 2022 00:19
 Operator : SY/MD
 Sample : N2345-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1548	rBV	384498	724998	39.43%	6.524%
38	6.526	1607	1613	1614	rBV3	1030	648	0.04%	0.006%
39	6.597	1633	1635	1641	rVB2	373	261	0.01%	0.002%
40	6.694	1649	1665	1686	rBV	277306	543893	29.58%	4.895%
41	6.858	1713	1716	1719	rVB3	808	541	0.03%	0.005%
42	7.047	1770	1775	1776	rBV2	378	307	0.02%	0.003%
43	7.189	1809	1819	1827	rBV4	2078	3405	0.19%	0.031%
44	7.314	1854	1858	1860	rBV	312	223	0.01%	0.002%
45	7.401	1882	1885	1890	rVB2	559	434	0.02%	0.004%
46	7.568	1924	1937	1957	rBV	147064	260102	14.15%	2.341%
47	7.687	1969	1974	1987	rVB4	1670	3145	0.17%	0.028%
48	7.796	2002	2008	2014	rBV3	579	942	0.05%	0.008%
49	7.841	2017	2022	2024	rBV2	254	268	0.01%	0.002%
50	7.899	2025	2040	2056	rBV	559478	967499	52.62%	8.707%
51	8.179	2116	2127	2146	rBV	98905	172410	9.38%	1.552%
52	8.475	2211	2219	2229	rVB2	4415	7469	0.41%	0.067%
53	8.552	2239	2243	2245	rBV3	390	296	0.02%	0.003%
54	8.632	2255	2268	2300	rBV	385023	715147	38.90%	6.436%
55	8.947	2363	2366	2373	rVB3	324	280	0.02%	0.003%
56	9.015	2384	2387	2391	rBV3	269	255	0.01%	0.002%
57	9.128	2419	2422	2430	rVB3	539	472	0.03%	0.004%
58	9.182	2436	2439	2442	rVB2	558	307	0.02%	0.003%
59	9.333	2481	2486	2487	rBV3	308	243	0.01%	0.002%
60	9.420	2498	2513	2515	rBV	585479	802364	43.64%	7.221%
61	9.632	2575	2579	2581	rBV3	376	265	0.01%	0.002%
62	9.700	2593	2600	2611	rVB7	1298	2232	0.12%	0.020%
63	9.812	2630	2635	2637	rBV4	284	263	0.01%	0.002%
64	9.902	2661	2663	2666	rBV2	369	222	0.01%	0.002%
65	10.079	2715	2718	2721	rBV2	314	223	0.01%	0.002%
66	10.147	2736	2739	2742	rBV	474	343	0.02%	0.003%
67	10.179	2746	2749	2752	rBV3	414	254	0.01%	0.002%
68	10.311	2788	2790	2793	rVV2	407	235	0.01%	0.002%
69	10.336	2795	2798	2802	rVV4	369	268	0.01%	0.002%
70	10.462	2831	2837	2839	rBV3	478	483	0.03%	0.004%
71	10.607	2880	2882	2885	rBV	408	277	0.02%	0.002%
72	10.674	2895	2903	2911	rBV4	1686	2521	0.14%	0.023%
73	10.758	2915	2929	2949	rBV	413191	666544	36.25%	5.998%
74	10.828	2949	2951	2954	rVB2	408	229	0.01%	0.002%
75	10.896	2959	2972	2982	rVB2	7333	13483	0.73%	0.121%
76	11.008	3003	3007	3008	rBV2	368	255	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047890.D
 Acq On : 09 Apr 2022 00:19
 Operator : SY/MD
 Sample : N2345-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.086	3027	3031	3034	rBV2	644	537	0.03%	0.005%
78	11.160	3050	3054	3056	rBV	395	297	0.02%	0.003%
79	11.314	3098	3102	3107	rBV2	317	307	0.02%	0.003%
80	11.462	3136	3148	3150	rBV6	1508	2051	0.11%	0.018%
81	11.584	3183	3186	3191	rBV3	426	336	0.02%	0.003%
82	11.626	3195	3199	3202	rBV3	294	256	0.01%	0.002%
83	11.664	3206	3211	3212	rBV3	544	441	0.02%	0.004%
84	11.700	3217	3222	3226	rBV3	686	976	0.05%	0.009%
85	11.745	3226	3236	3246	rBV	87189	138548	7.54%	1.247%
86	11.816	3246	3258	3259	rBV	678092	794974	43.24%	7.154%
87	12.066	3328	3336	3352	rVB3	8853	16305	0.89%	0.147%
88	12.201	3361	3378	3402	rBV2	746142	1838594	100.00%	16.546%
89	12.475	3460	3463	3465	rBV	543	367	0.02%	0.003%
90	12.716	3534	3538	3542	rBV2	536	648	0.04%	0.006%
91	12.918	3598	3601	3606	rBV3	273	296	0.02%	0.003%
92	13.047	3638	3641	3645	rVB2	358	302	0.02%	0.003%
93	13.211	3684	3692	3708	rVB3	9570	17134	0.93%	0.154%
94	13.655	3827	3830	3832	rBV3	551	337	0.02%	0.003%
95	13.841	3873	3888	3909	rBV	231965	371351	20.20%	3.342%
96	14.330	4029	4040	4055	rBV	98900	159247	8.66%	1.433%
97	14.738	4157	4167	4176	rBV8	3894	6883	0.37%	0.062%
98	15.417	4373	4378	4387	rVB4	5358	7714	0.42%	0.069%
99	15.655	4447	4452	4454	rBV3	992	1099	0.06%	0.010%
100	16.002	4552	4560	4575	rVB2	19511	30441	1.66%	0.274%



Sum of corrected areas: 11112296

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047890.D
Acq On : 09 Apr 2022 00:19
Operator : SY/MD
Sample : N2345-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

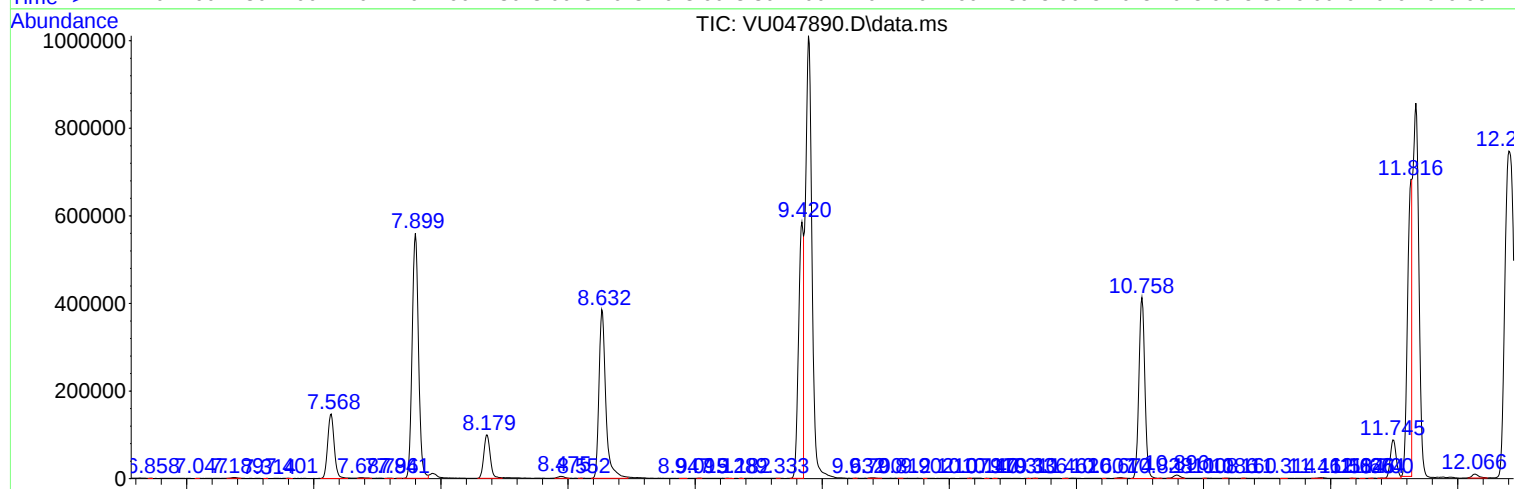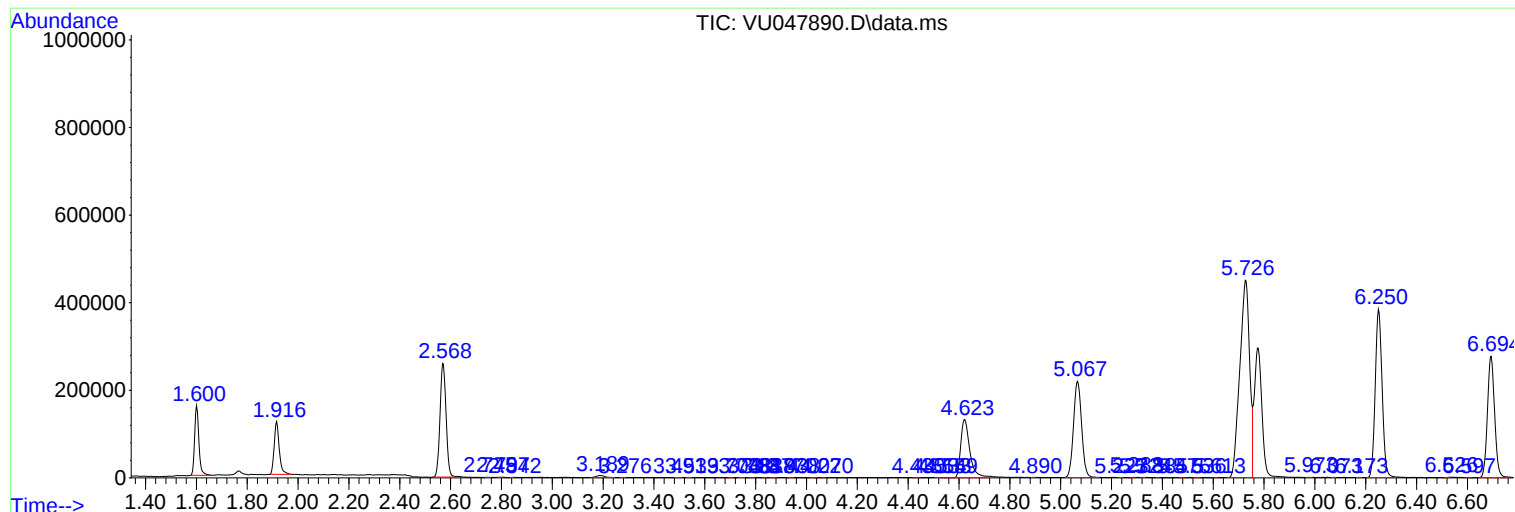

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047890.D
Acq On : 09 Apr 2022 00:19
Operator : SY/MD
Sample : N2345-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
Data File : VU047890.D
Acq On : 09 Apr 2022 00:19
Operator : SY/MD
Sample : N2345-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------