


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040922\
 Data File : VU047870.D
 Acq On : 08 Apr 2022 15:14
 Operator : SY/MD
 Sample : BFB060
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB060

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Thu Apr 14 06:53:20 2022

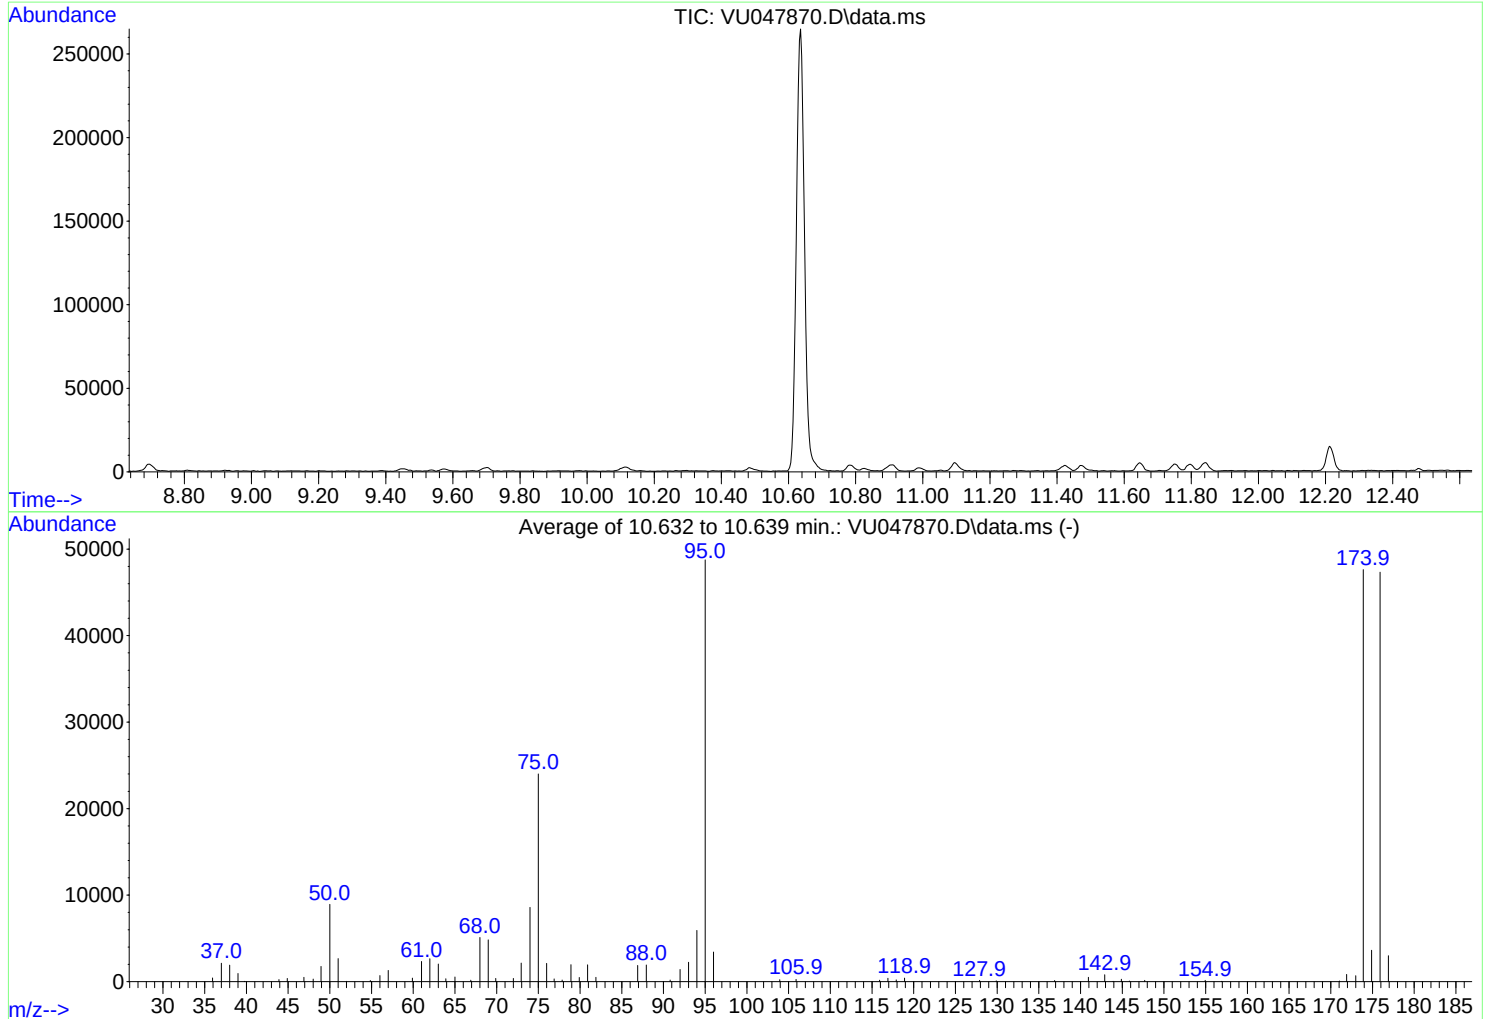

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	8926	PASS
75	95	30	80	49.2	24003	PASS
95	95	100	100	100.0	48757	PASS
96	95	5	9	7.0	3429	PASS
173	174	0.00	2	1.4	688	PASS
174	95	50	120	97.7	47635	PASS
175	174	5	9	7.6	3625	PASS
176	174	95	101	99.4	47339	PASS
177	176	5	9	6.3	2993	PASS

Scan 2878 (10.594 min): VU047870.D\data.ms
BFB060

m/z	Abundance
39.80	108.0
43.90	492.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060

m/z	Abundance
36.00	422.0
37.00	2156.0
38.00	1958.0
39.00	975.0
39.80	112.0
43.90	752.0
44.90	363.0
46.90	530.0
48.00	322.0
48.90	1744.0
50.00	9306.0
51.00	2769.0
52.00	102.0
54.90	154.0
56.00	678.0
57.00	1415.0
59.90	442.0
61.00	2310.0
62.00	2684.0
63.00	2049.0
63.90	402.0
65.00	544.0
66.90	182.0
68.00	5397.0
69.00	4876.0
69.90	390.0
72.00	346.0
73.00	2304.0
74.00	8619.0
75.00	24424.0
76.00	2018.0
76.90	274.0
77.90	189.0
78.90	2010.0
79.90	549.0
80.90	2019.0
81.90	499.0
86.90	1875.0
87.90	2014.0
90.80	224.0
92.00	1394.0
93.00	2340.0
94.00	5837.0
95.00	49456.0
96.00	3545.0
103.90	219.0
106.00	292.0
115.90	157.0
116.90	368.0
117.90	214.0
118.90	448.0
127.90	161.0
136.90	106.0
141.00	447.0
142.90	795.0
144.90	250.0
147.70	109.0
155.00	117.0
171.90	855.0
173.00	711.0
173.90	47144.0
174.90	3550.0
175.90	46144.0
176.90	2992.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060

m/z	Abundance
36.00	443.0
37.00	2204.0
38.00	1925.0
39.00	982.0
39.90	137.0
44.00	749.0
44.90	394.0
46.90	524.0
48.00	286.0
49.00	1780.0
50.00	9175.0
51.00	2769.0
54.90	117.0
56.00	720.0
57.00	1355.0
59.90	416.0
61.00	2423.0
62.00	2720.0
63.00	2107.0
63.90	335.0
65.00	556.0
66.90	170.0
68.00	5270.0
69.00	4999.0
69.90	397.0
72.00	379.0
73.00	2202.0
74.00	8981.0
75.00	24768.0
76.00	2229.0
76.90	330.0
77.90	175.0
78.90	2026.0
79.90	479.0
80.90	2007.0
81.90	533.0
86.90	1899.0
88.00	1966.0
90.80	201.0
92.00	1451.0
93.00	2314.0
94.00	6104.0
95.00	49960.0
96.00	3510.0
103.90	222.0
105.90	271.0
115.90	162.0
116.90	398.0
117.90	207.0
118.90	412.0
127.90	143.0
129.90	118.0
136.90	156.0
140.90	494.0
142.90	823.0
143.90	101.0
144.90	289.0
145.80	105.0
147.70	160.0
155.00	151.0
171.10	109.0
171.90	873.0
173.00	704.0
173.90	48880.0
174.90	3750.0
175.90	48872.0
176.90	3063.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060

m/z	Abundance
35.90	415.0
37.00	2021.0
38.00	1832.0
39.00	894.0
39.90	182.0
44.00	692.0
44.90	367.0
46.90	442.0
48.00	262.0
49.00	1730.0
50.00	8296.0
51.00	2480.0
54.70	113.0
56.00	701.0
57.00	1135.0
59.90	374.0
61.00	2287.0
62.00	2546.0
63.00	1958.0
63.90	269.0
65.00	490.0
66.90	148.0
68.00	4646.0
69.00	4613.0
69.90	326.0
72.00	366.0
72.90	1949.0
74.00	8172.0
75.00	22816.0
76.00	2076.0
76.90	319.0
77.70	213.0
78.90	1878.0
79.90	438.0
80.90	1820.0
81.90	484.0
86.90	1858.0
88.00	1774.0
90.80	159.0
92.00	1389.0
93.00	2083.0
94.00	5798.0
95.00	46856.0
96.00	3233.0
104.00	200.0
105.80	231.0
115.90	158.0
116.90	377.0
117.90	187.0
118.90	340.0
127.90	121.0
129.90	137.0
136.90	149.0
140.90	554.0
142.90	776.0
144.90	308.0
145.90	102.0
147.70	155.0
154.90	154.0
156.90	111.0
171.00	124.0
171.90	768.0
173.00	649.0
173.90	46880.0
174.90	3574.0
175.90	47000.0
176.90	2925.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060