

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040924\
 Data File : VU058507.D
 Acq On : 09 Apr 2024 12:12
 Operator : MD/SY
 Sample : P2013-04 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOMB0

Quant Time: Apr 10 01:13:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 10 01:12:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	70069	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	66866	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	28989	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	24872	5.362	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.200%
7) Chloroethane-d5	1.904	69	21626	5.364	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.200%
11) 1,1-Dichloroethene-d2	2.557	65	11201	5.335	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	106.600%
20) 2-Butanone-d5	4.631	46	43296	44.287	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.580%
24) Chloroform-d	5.052	84	46172	4.986	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
26) 1,2-Dichloroethane-d4	5.692	65	22006	5.092	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.800%
32) Benzene-d6	5.718	84	94449	5.247	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.000%
36) 1,2-Dichloropropane-d6	6.682	67	29110	5.156	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.200%
41) Toluene-d8	7.891	98	78590	4.923	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
43) trans-1,3-Dichloroprop...	8.174	79	8395	4.790	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.800%
46) 2-Hexanone-d5	8.627	63	31144	43.088	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.180%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	17257	4.330	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	22080	4.522	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.400%
Target Compounds						
5) Vinyl chloride	1.599	62	1303	0.183	ug/L	# 66
22) cis-1,2-Dichloroethene	4.657	96	39993	6.843	ug/L	96
34) Trichloroethene	6.534	95	9576	1.567	ug/L	96
47) Tetrachloroethene	8.547	164	11462	2.559	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040924\
Data File : VU058507.D
Acq On : 09 Apr 2024 12:12
Operator : MD/SY
Sample : P2013-04 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOMB0

Quant Time: Apr 10 01:13:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 10 01:12:33 2024
Response via : Initial Calibration




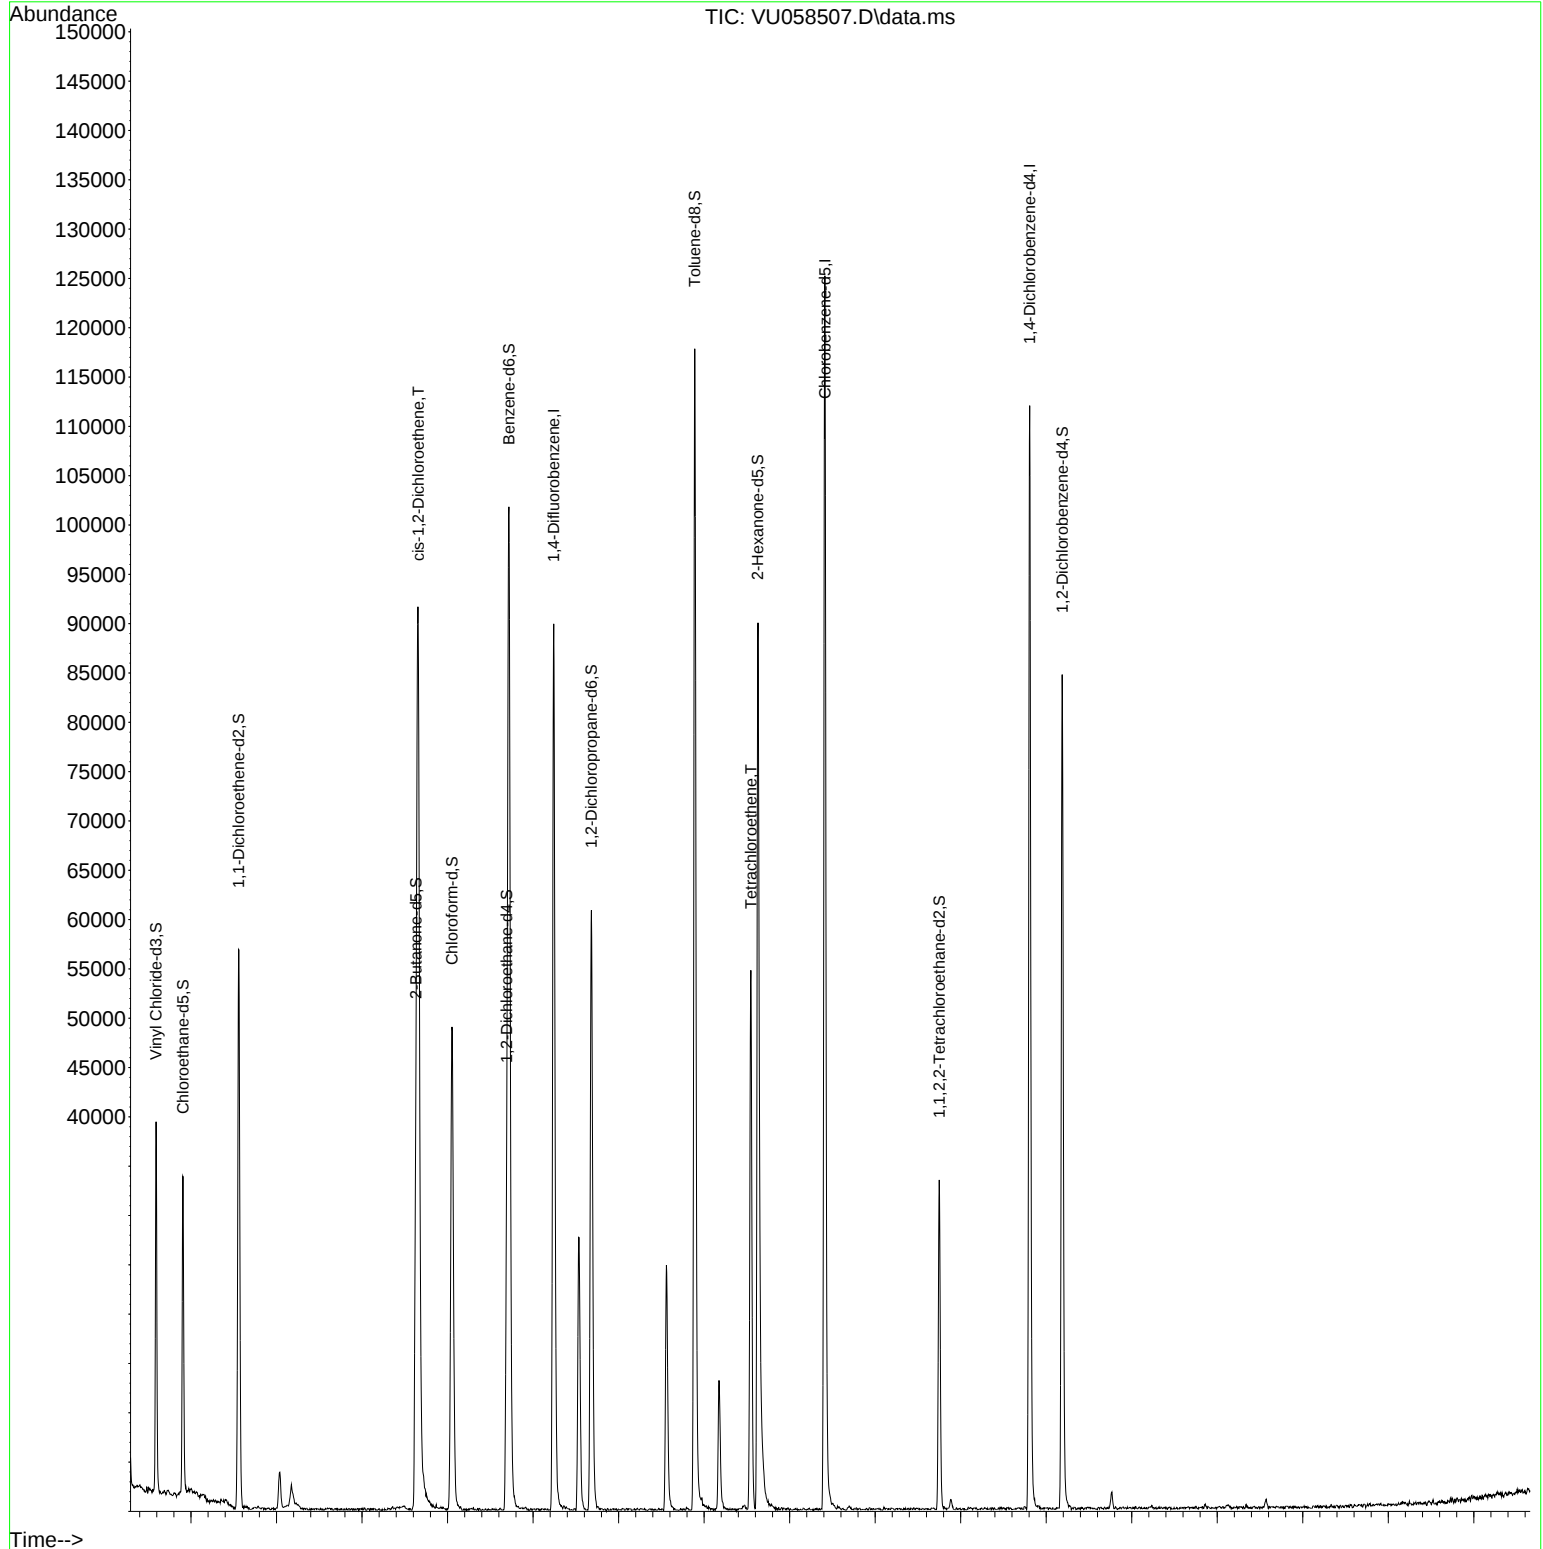


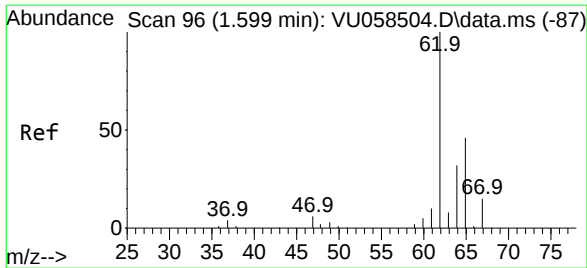

#5
 Vinyl chloride
 Concen: 0.183 ug/L
 RT: 1.599 min Scan# 96
 Delta R.T. -0.000 min
 Lab File: VU058507.D
 Acq: 09 Apr 2024 12:12




Instrument :
 MSVOA_U
 ClientSampleId :
 EOMB0


Tgt Ion: 62 Resp: 1303
 Ion Ratio Lower Upper
 62 100
 64 51.3 22.6 42.0#

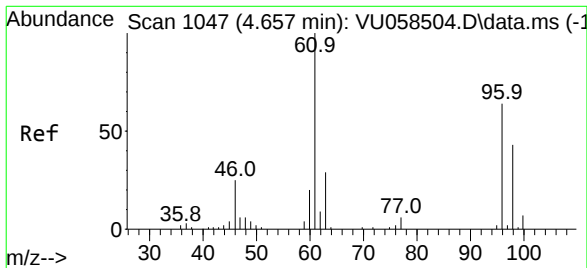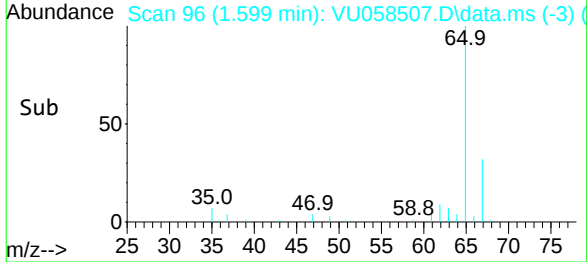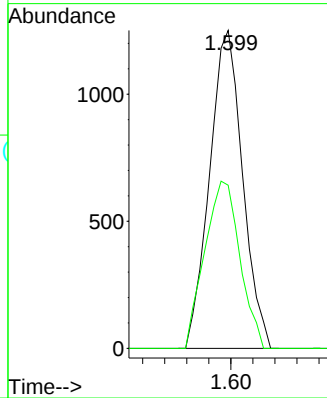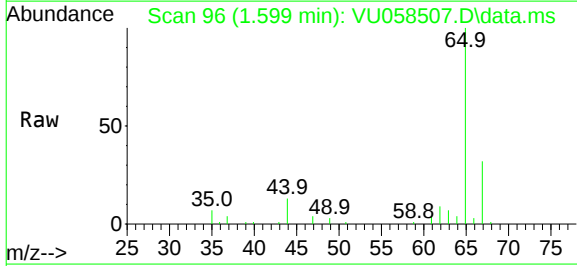

#22
 cis-1,2-Dichloroethene
 Concen: 6.843 ug/L
 RT: 4.657 min Scan# 1047
 Delta R.T. -0.000 min
 Lab File: VU058507.D
 Acq: 09 Apr 2024 12:12


Tgt Ion: 96 Resp: 39993
 Ion Ratio Lower Upper
 96 100
 61 145.8 98.1 182.3
 98 65.4 43.6 81.0

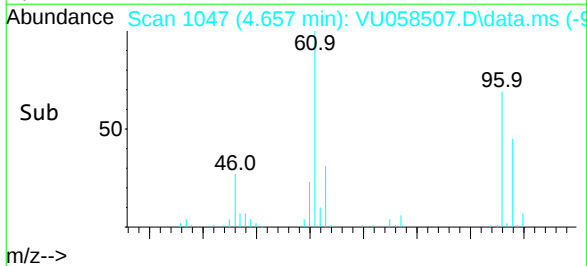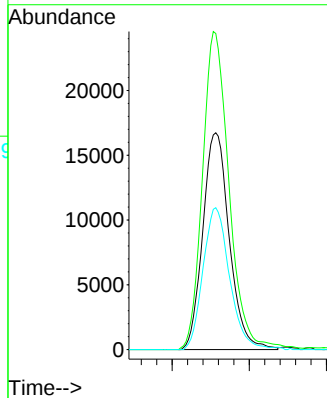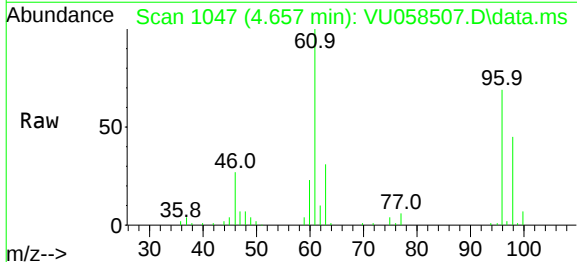



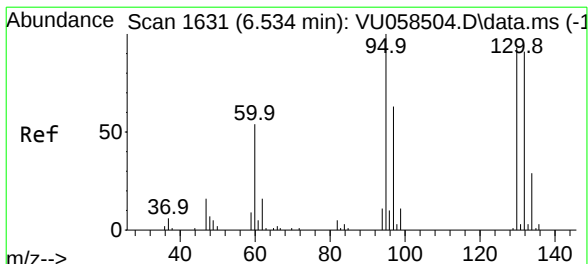


#34
 Trichloroethene
 Concen: 1.567 ug/L
 RT: 6.534 min Scan# 1631
 Delta R.T. -0.000 min
 Lab File: VU058507.D
 Acq: 09 Apr 2024 12:12

Instrument : MSVOA_U
 ClientSampleId : EOMB0

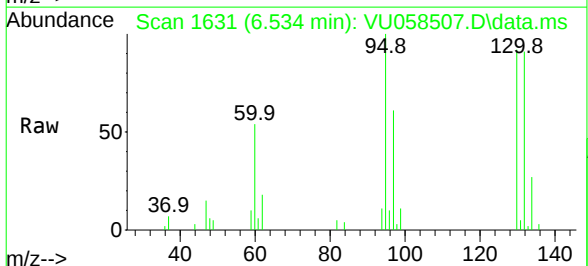

Tgt Ion	Ratio	Lower	Upper
95	100		
97	60.9	45.6	84.6
132	91.0	64.8	120.3
130	91.9	68.0	126.2

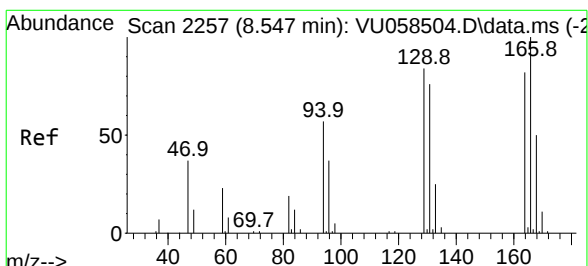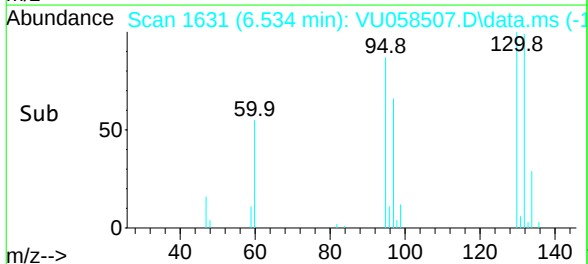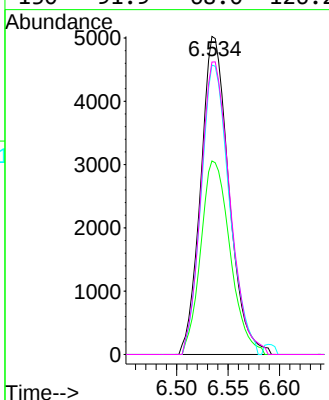

#47
 Tetrachloroethene
 Concen: 2.559 ug/L
 RT: 8.547 min Scan# 2257
 Delta R.T. -0.000 min
 Lab File: VU058507.D
 Acq: 09 Apr 2024 12:12

Tgt Ion	Ratio	Lower	Upper
164	100		
129	96.7	67.3	125.1
131	88.8	65.5	121.6
166	122.4	89.5	166.1

