

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040924\
 Data File : VU058518.D
 Acq On : 09 Apr 2024 16:25
 Operator : MD/SY
 Sample : P2012-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Apr 10 01:16:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 10 01:12:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	68461	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	68201	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	29110	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	22696	5.007	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.200%
7) Chloroethane-d5	1.904	69	19652	4.989	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.800%
11) 1,1-Dichloroethene-d2	2.560	65	10036	4.892	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	97.800%
20) 2-Butanone-d5	4.621	46	37759	39.530	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.060%
24) Chloroform-d	5.052	84	41649	4.603	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.000%
26) 1,2-Dichloroethane-d4	5.695	65	19562	4.633	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.600%
32) Benzene-d6	5.718	84	83809	4.564	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.200%
36) 1,2-Dichloropropane-d6	6.682	67	26405	4.586	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.800%
41) Toluene-d8	7.891	98	69123	4.245	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.800%
43) trans-1,3-Dichloroprop...	8.177	79	6958	3.893	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.800%
46) 2-Hexanone-d5	8.631	63	27659	37.517	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.040%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	15357	3.778	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	75.600%
66) 1,2-Dichlorobenzene-d4	12.190	152	20507	4.183	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.600%
Target Compounds					Qvalue	
16) Methylene chloride	3.033	84	2476	0.385	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040924\
Data File : VU058518.D
Acq On : 09 Apr 2024 16:25
Operator : MD/SY
Sample : P2012-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Apr 10 01:16:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 10 01:12:33 2024
Response via : Initial Calibration

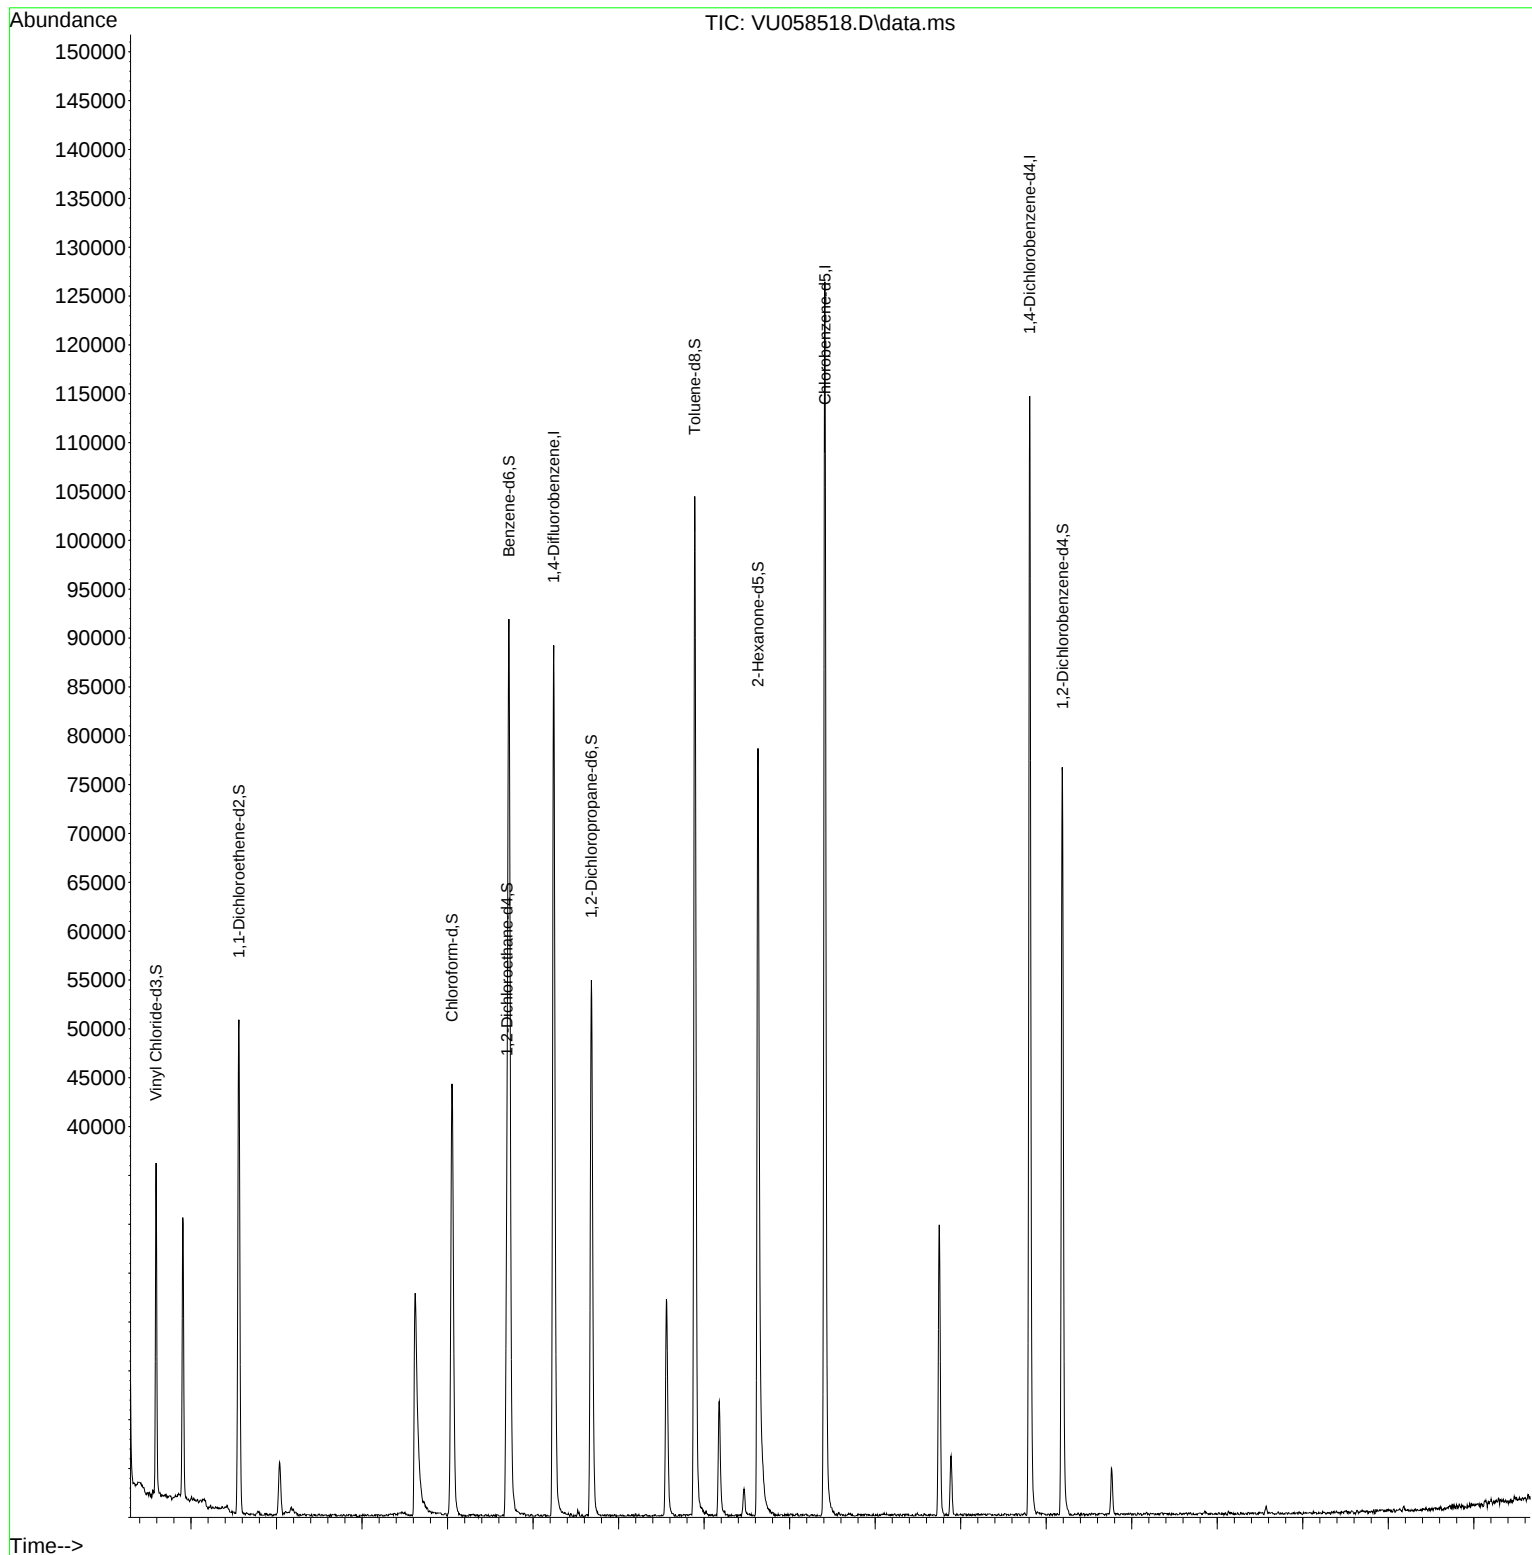

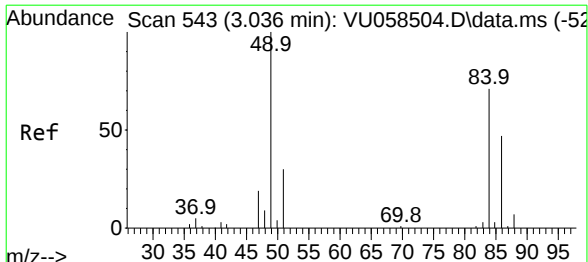

#16
Methylene chloride
Concen: 0.385 ug/L
RT: 3.033 min Scan# 54
Delta R.T. -0.003 min
Lab File: VU058518.D
Acq: 09 Apr 2024 16:25

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

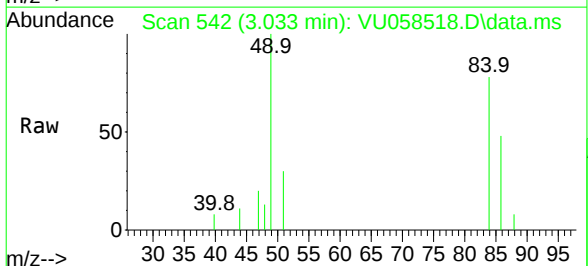

Tgt Ion:	84	Resp:	2476
Ion	Ratio	Lower	Upper
84	100		
86	62.0	44.3	82.3
49	128.2	96.0	178.2

