

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040924\
 Data File : VU058537.D
 Acq On : 10 Apr 2024 00:41
 Operator : MD/SY
 Sample : P2014-03 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0MD0

Quant Time: Apr 10 02:18:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 10 02:08:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	62748	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	61681	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	25557	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	21753	5.236	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.800%
7) Chloroethane-d5	1.907	69	17875	4.951	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.000%
11) 1,1-Dichloroethene-d2	2.560	65	9536	5.071	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	101.400%
20) 2-Butanone-d5	4.637	46	39450	45.061	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.120%
24) Chloroform-d	5.052	84	39653	4.781	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	5.695	65	19150	4.948	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%
32) Benzene-d6	5.718	84	79800	4.805	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.200%
36) 1,2-Dichloropropane-d6	6.682	67	25242	4.847	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.000%
41) Toluene-d8	7.891	98	64909	4.408	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.200%
43) trans-1,3-Dichloroprop...	8.177	79	6533	4.041	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.800%
46) 2-Hexanone-d5	8.631	63	25252	37.873	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.740%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	14714	4.002	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.000%
66) 1,2-Dichlorobenzene-d4	12.187	152	18861	4.382	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.600%
Target Compounds					Qvalue	
22) cis-1,2-Dichloroethene	4.660	96	1137	0.217	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040924\
Data File : VU058537.D
Acq On : 10 Apr 2024 00:41
Operator : MD/SY
Sample : P2014-03 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0MD0


Quant Time: Apr 10 02:18:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 10 02:08:42 2024
Response via : Initial Calibration

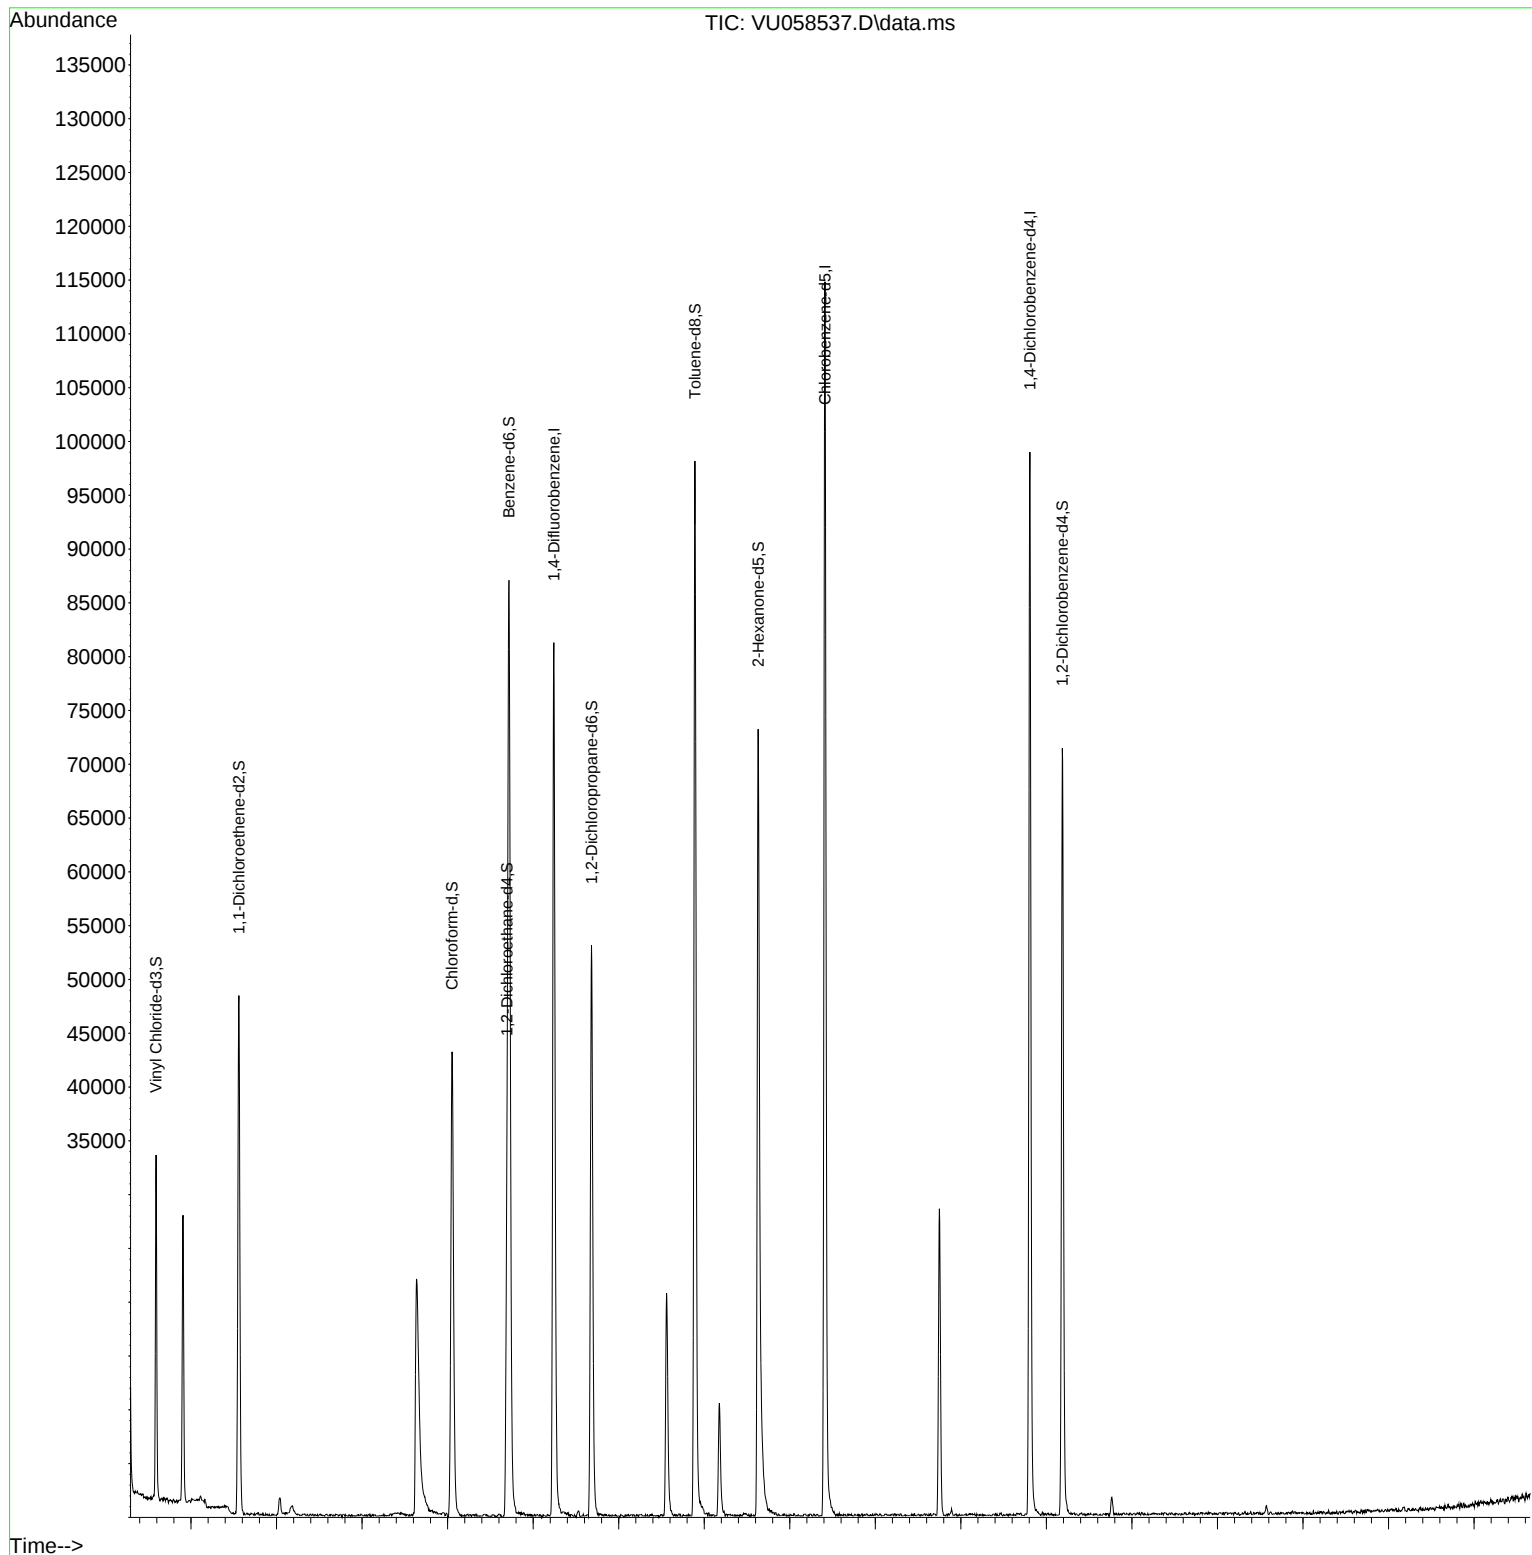

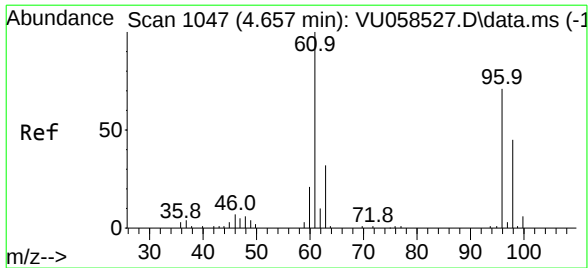

#22
 cis-1,2-Dichloroethene
 Concen: 0.217 ug/L
 RT: 4.660 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VU058537.D
 Acq: 10 Apr 2024 00:41

Instrument :
 MSVOA_U
 ClientSampleId :
 E0MD0

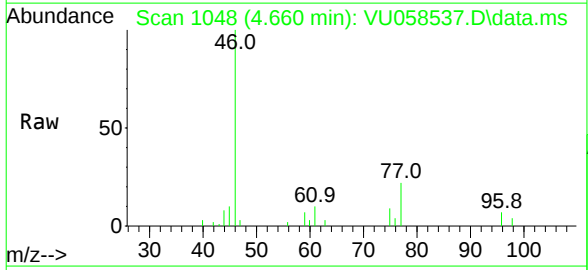

Tgt Ion:	96	Resp:	1137
Ion	Ratio	Lower	Upper
96	100		
61	135.8	98.1	182.3
98	55.8	43.6	81.0

