

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040924\
 Data File : VU058531.D
 Acq On : 09 Apr 2024 22:19
 Operator : MD/SY
 Sample : P1970-13 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU058531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	107	rBV	32936	37072	15.80%	1.855%
2	1.907	183	192	200	rBV	29716	37247	15.88%	1.864%
3	2.566	383	397	415	rVB3	80768	159737	68.09%	7.992%
4	3.036	534	543	555	rBV2	4004	6961	2.97%	0.348%
5	3.174	576	586	602	rVB2	1437	3252	1.39%	0.163%
6	4.631	1025	1039	1077	rBV2	25907	76758	32.72%	3.840%
7	5.052	1156	1170	1190	rBV2	45941	102848	43.84%	5.146%
8	5.306	1234	1249	1270	rVB2	51566	115733	49.33%	5.790%
9	5.717	1358	1377	1404	rBV2	92484	234612	100.00%	11.738%
10	6.241	1527	1540	1564	rBV	82883	159024	67.78%	7.956%
11	6.682	1665	1677	1706	rBV	57530	112676	48.03%	5.637%
12	7.560	1939	1950	1972	rBV	23263	42084	17.94%	2.106%
13	7.891	2042	2053	2076	rBV	103832	181993	77.57%	9.106%
14	8.177	2131	2142	2157	rBV2	12049	21315	9.09%	1.066%
15	8.630	2272	2283	2317	rBV2	78659	166969	71.17%	8.354%
16	9.412	2515	2526	2550	rBV	115650	199314	84.95%	9.972%
17	10.749	2930	2942	2956	rBV	30791	50096	21.35%	2.506%
18	11.807	3260	3271	3290	rBV	98794	160941	68.60%	8.052%
19	12.187	3377	3389	3419	rBV	74800	126700	54.00%	6.339%
20	12.769	3558	3570	3577	rBV2	1952	3364	1.43%	0.168%

Sum of corrected areas: 1998696




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040924\
Data File : VU058531.D
Acq On : 09 Apr 2024 22:19
Operator : MD/SY
Sample : P1970-13 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

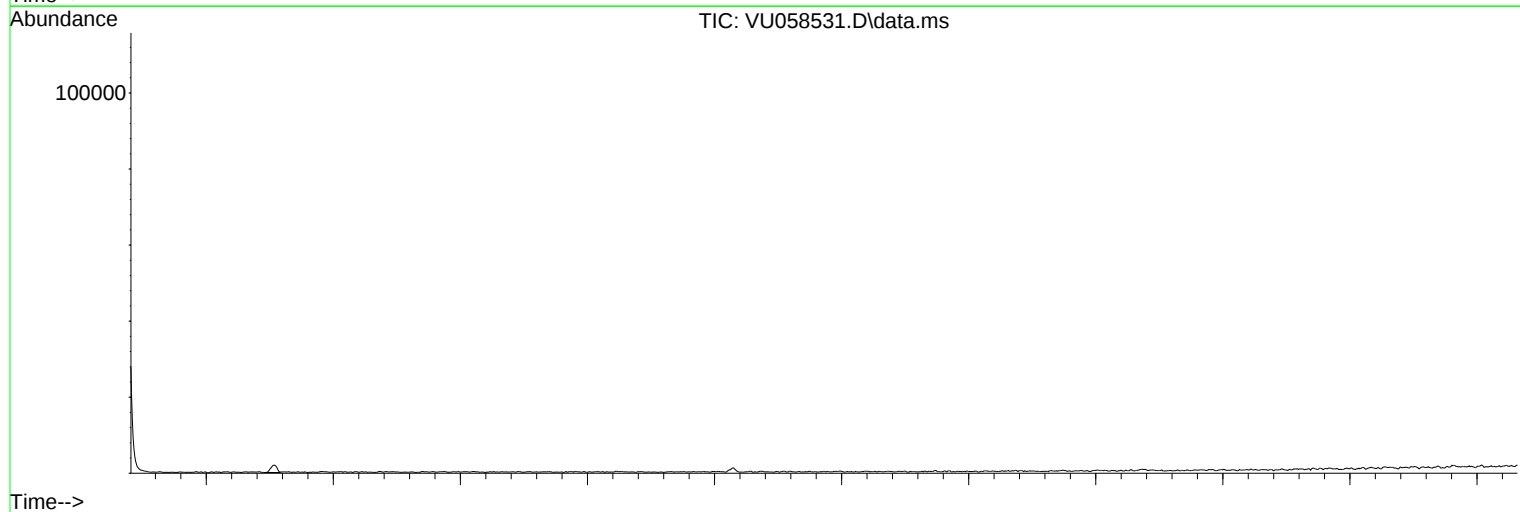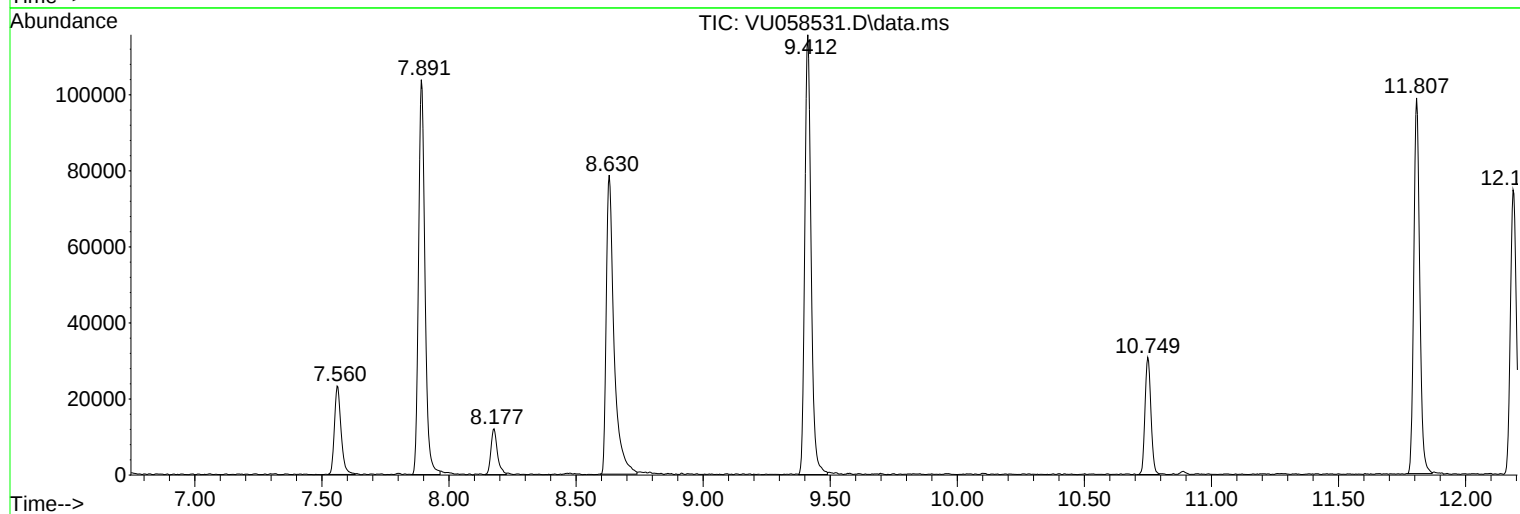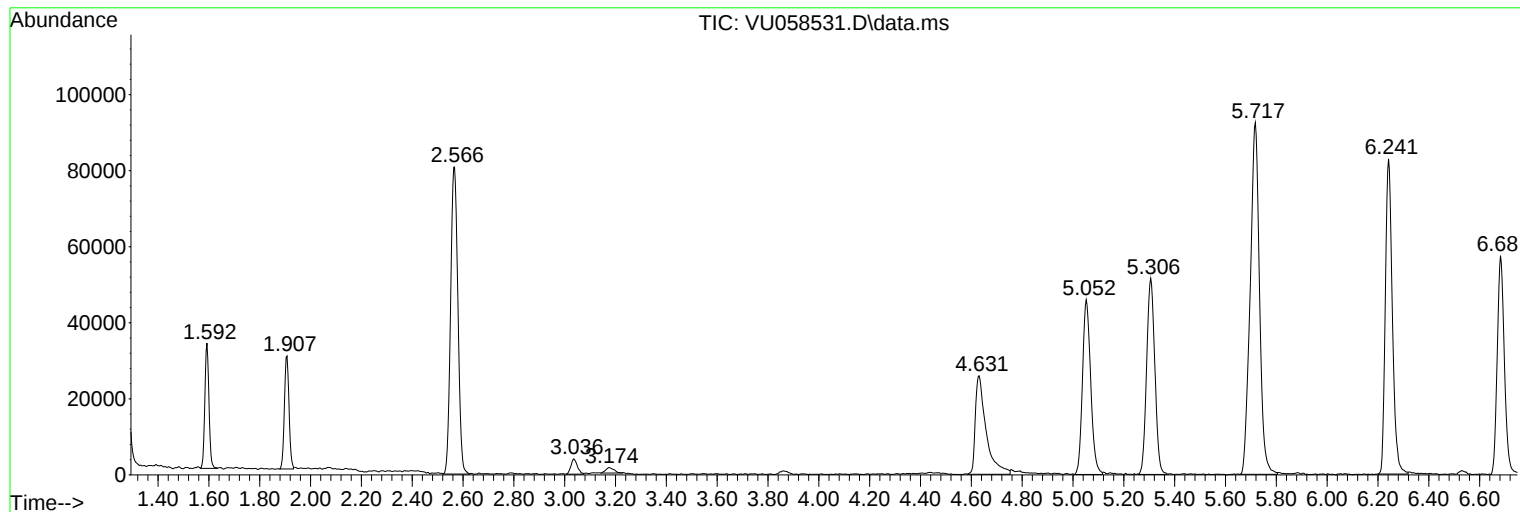

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040924\
Data File : VU058531.D
Acq On : 09 Apr 2024 22:19
Operator : MD/SY
Sample : P1970-13 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040924\
Data File : VU058531.D
Acq On : 09 Apr 2024 22:19
Operator : MD/SY
Sample : P1970-13 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------