
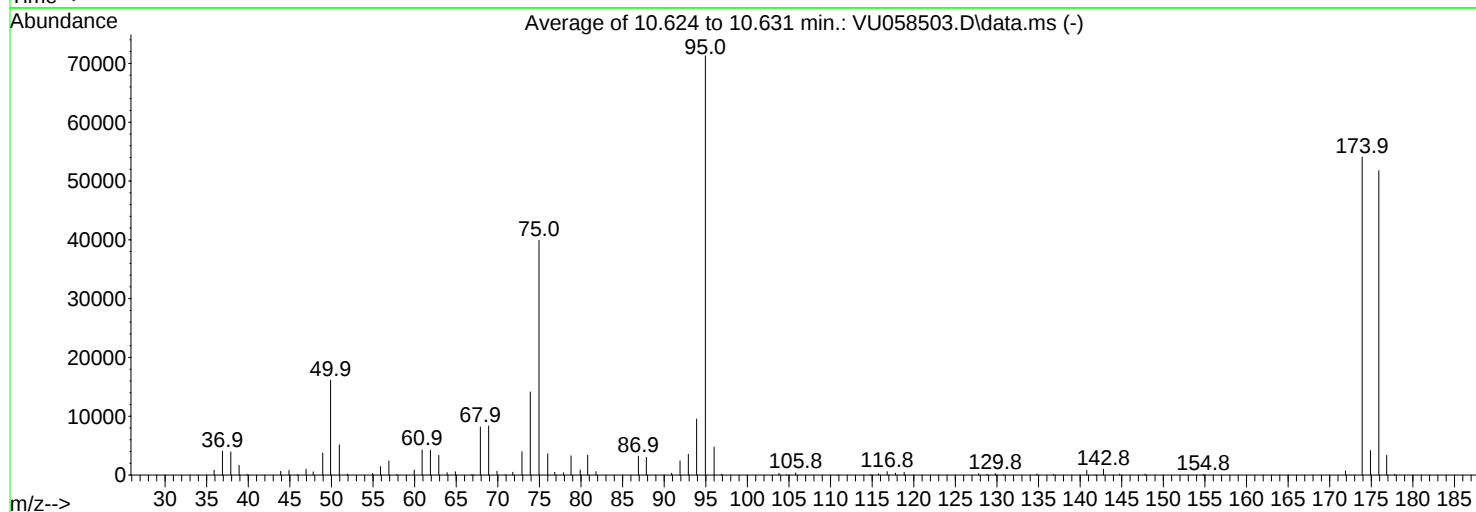


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040924\
Data File : VU058503.D
Acq On : 09 Apr 2024 08:38
Operator : MD/SY
Sample : BFB139
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB139

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 10 02:08:42 2024

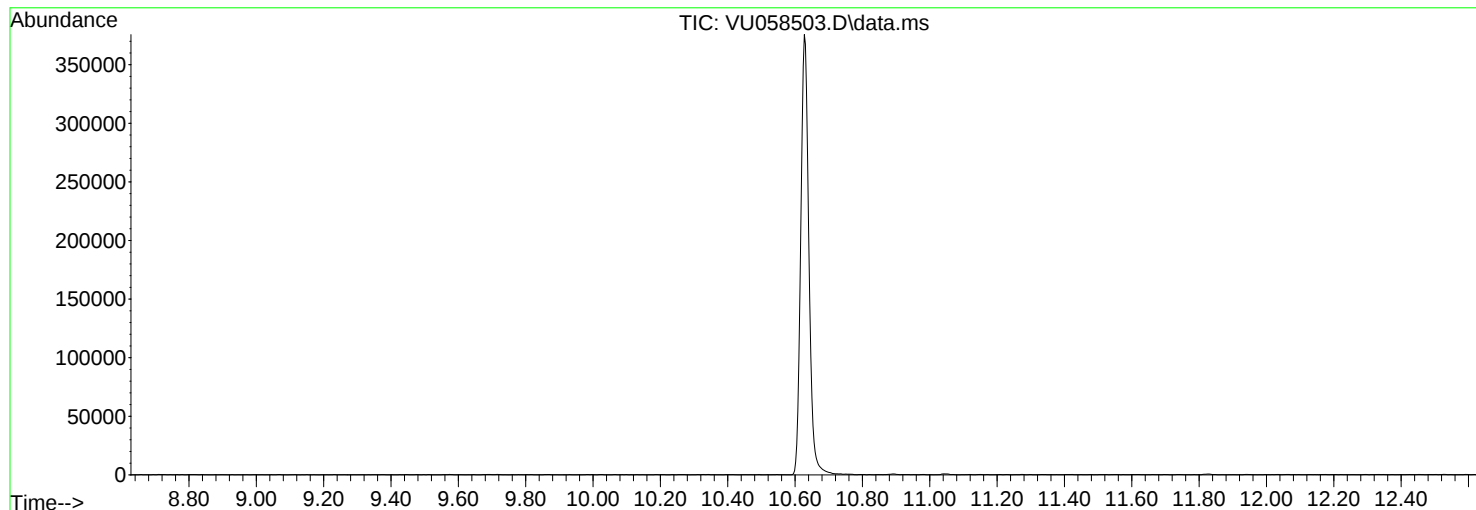

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	16159	PASS
75	95	30	80	56.0	39923	PASS
95	95	100	100	100.0	71304	PASS
96	95	5	9	6.7	4763	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.8	54067	PASS
175	174	5	9	7.7	4164	PASS
176	174	95	101	95.7	51768	PASS
177	176	5	9	6.5	3358	PASS

m/z	Abundance
43.80	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
35.90	818.0
36.90	4014.0
37.90	3919.0
38.90	1604.0
39.80	143.0
44.00	779.0
44.90	813.0
45.90	122.0
47.00	974.0
47.80	512.0
49.00	3716.0
49.90	15691.0
51.00	4978.0
51.90	185.0
54.90	275.0
55.90	1369.0
56.90	2405.0
59.90	843.0
60.90	4108.0
61.90	4145.0
62.90	3342.0
63.90	431.0
64.90	550.0
66.80	143.0
67.90	8021.0
68.90	8207.0
69.90	681.0
71.80	445.0
72.90	3769.0
73.90	13487.0
74.90	38616.0
76.00	3459.0
76.80	478.0
77.90	415.0
78.80	3253.0
79.90	859.0
80.80	3283.0
81.80	605.0
86.90	3067.0
87.90	3096.0
90.90	324.0
91.90	2293.0
92.90	3396.0
93.90	9209.0
95.00	68096.0
96.00	4771.0
96.90	151.0
103.80	277.0
104.70	113.0
105.80	370.0
115.80	229.0
116.80	544.0
117.80	319.0
118.90	432.0
127.80	265.0
128.80	119.0
129.80	262.0
134.80	172.0
136.80	132.0
140.80	797.0
142.80	966.0
144.80	196.0
147.80	166.0
154.80	122.0
171.90	663.0
173.90	50752.0
174.90	3947.0
175.90	48568.0
176.90	3232.0
177.80	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
35.90	871.0
36.90	4215.0
37.90	4043.0
38.90	1723.0
39.80	142.0
44.00	788.0
44.90	826.0
45.90	108.0
46.90	1017.0
47.80	573.0
49.00	3953.0
49.90	16712.0
51.00	5344.0
51.90	197.0
55.00	288.0
55.90	1464.0
56.90	2495.0
57.80	125.0
59.90	874.0
60.90	4438.0
61.90	4334.0
62.90	3423.0
63.90	445.0
64.90	585.0
67.90	8350.0
68.90	8612.0
69.90	666.0
70.90	104.0
71.80	504.0
72.90	4113.0
73.90	14584.0
75.00	41304.0
76.00	3784.0
76.80	474.0
77.90	425.0
78.80	3427.0
79.90	912.0
80.80	3546.0
81.80	621.0
86.90	3323.0
87.80	3086.0
90.90	336.0
91.90	2483.0
92.90	3660.0
93.90	9789.0
95.00	73528.0
96.00	4884.0
96.90	136.0
103.80	300.0
104.70	108.0
105.80	392.0
110.80	102.0
114.80	107.0
115.80	265.0
116.80	627.0
117.80	345.0
118.90	478.0
127.80	289.0
128.80	146.0
129.80	285.0
130.80	114.0
134.80	202.0
136.80	135.0
140.80	858.0
142.80	1040.0
144.80	205.0
147.80	180.0
154.80	119.0
171.90	735.0
173.90	55768.0
174.90	4264.0
175.90	53344.0
176.90	3460.0
177.80	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
35.90	837.0
36.90	4030.0
37.90	3841.0
38.90	1687.0
39.90	129.0
43.90	735.0
44.90	739.0
47.00	987.0
47.80	587.0
48.90	3639.0
49.90	16075.0
50.90	5124.0
51.90	184.0
55.00	269.0
55.90	1493.0
56.90	2315.0
57.90	152.0
60.00	845.0
60.90	4301.0
61.90	4195.0
62.90	3327.0
63.90	414.0
64.90	559.0
67.10	175.0
67.90	8158.0
68.90	8229.0
69.90	622.0
70.90	101.0
71.80	502.0
72.90	4012.0
73.90	14336.0
75.00	39848.0
76.00	3635.0
76.90	439.0
77.90	350.0
78.80	3151.0
79.90	863.0
80.80	3327.0
81.80	572.0
86.90	3265.0
87.80	2916.0
90.90	300.0
91.90	2463.0
92.90	3591.0
93.90	9559.0
94.90	72288.0
96.00	4635.0
96.90	109.0
103.80	343.0
105.80	376.0
114.80	113.0
115.70	257.0
116.80	624.0
117.80	353.0
118.80	479.0
127.80	266.0
128.80	152.0
129.80	278.0
130.80	125.0
134.80	189.0
136.80	113.0
140.80	784.0
141.80	101.0
142.80	993.0
144.70	184.0
147.80	180.0
154.80	127.0
171.90	701.0
173.90	55680.0
174.90	4282.0
175.90	53392.0
176.80	3382.0
177.80	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139