


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030942.D
Acq On : 09 Apr 2019 07:51
Operator : JC/SP
Sample : K2286-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 34 Sample Multiplier: 1




Quant Time: Apr 09 08:35:54 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Apr 09 08:28:51 2019
Response via : Initial Calibration

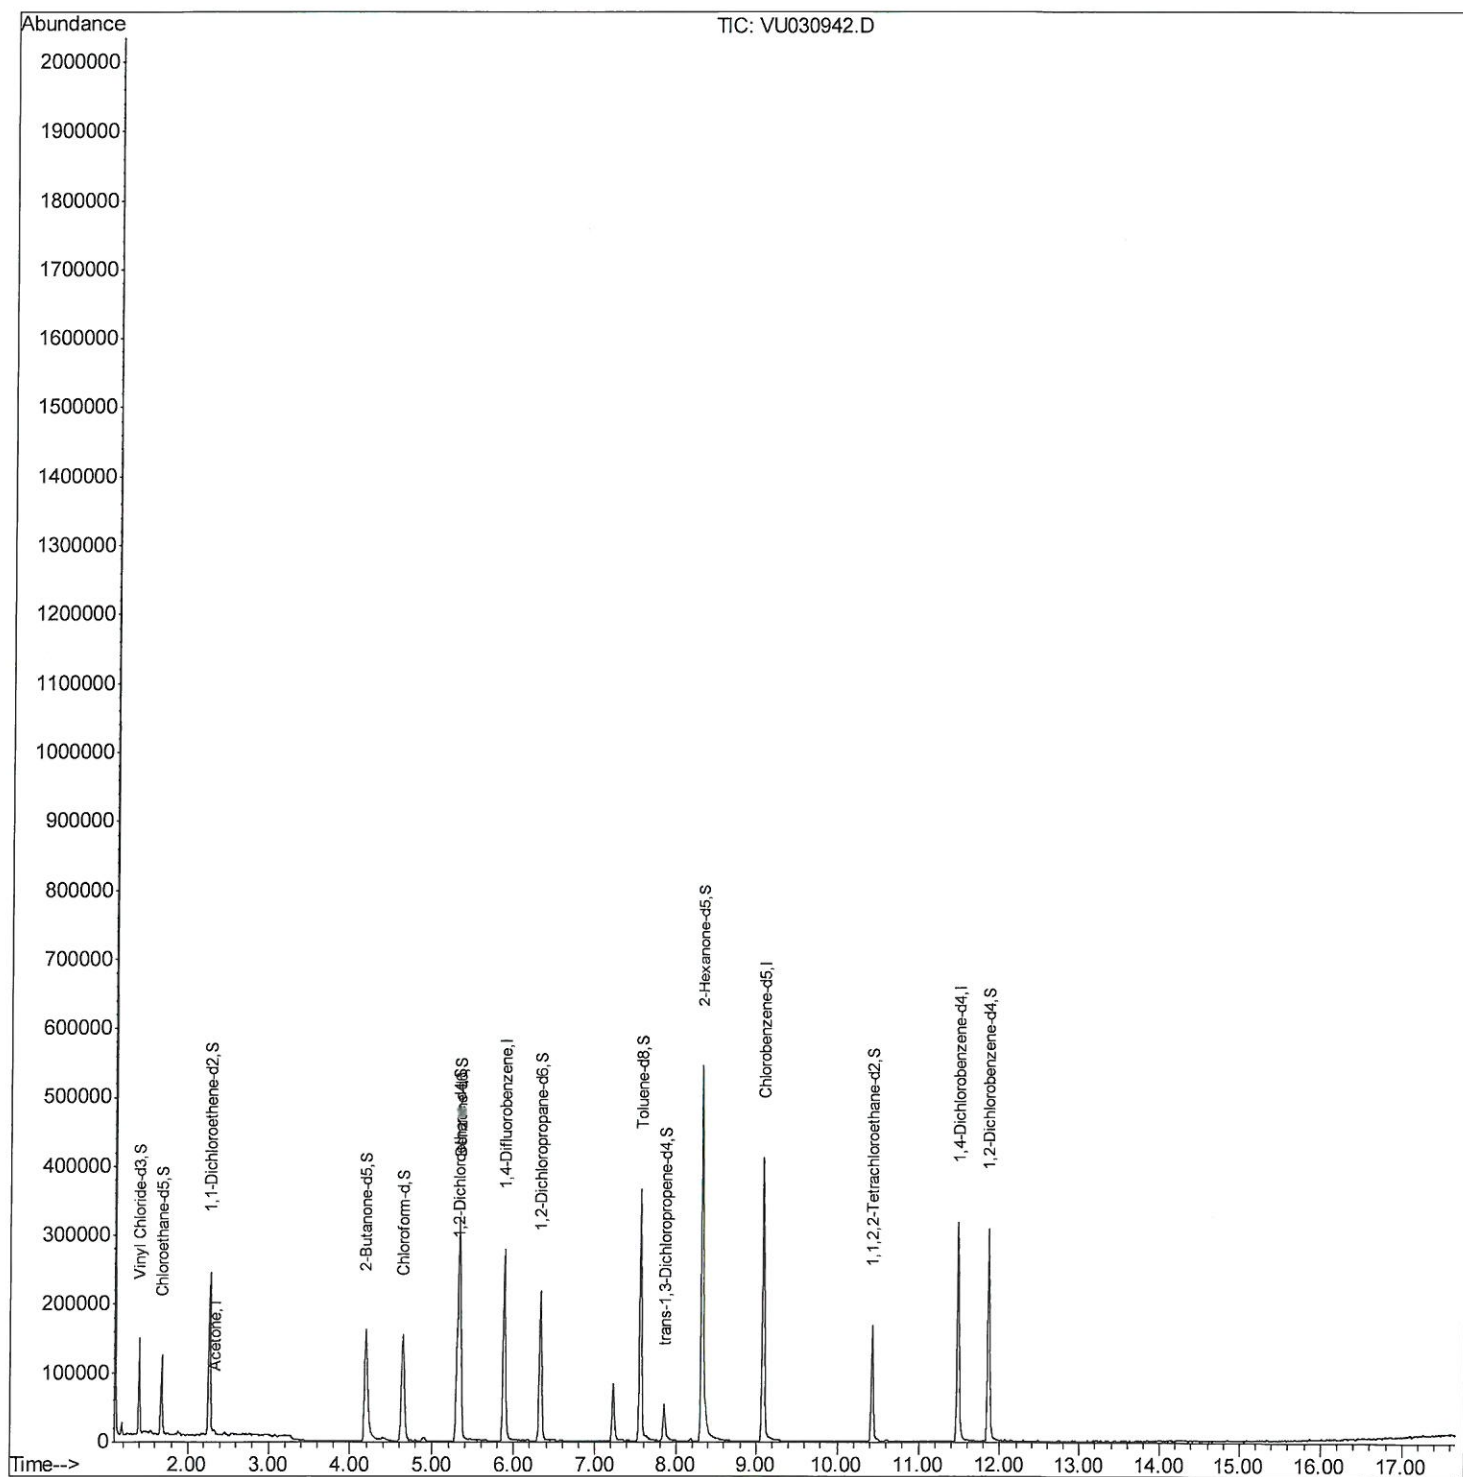

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030942.D
 Acq On : 09 Apr 2019 07:51
 Operator : JC/SP
 Sample : K2286-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Quant Time: Apr 09 08:33:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Apr 09 08:28:51 2019
 Response via : Initial Calibration

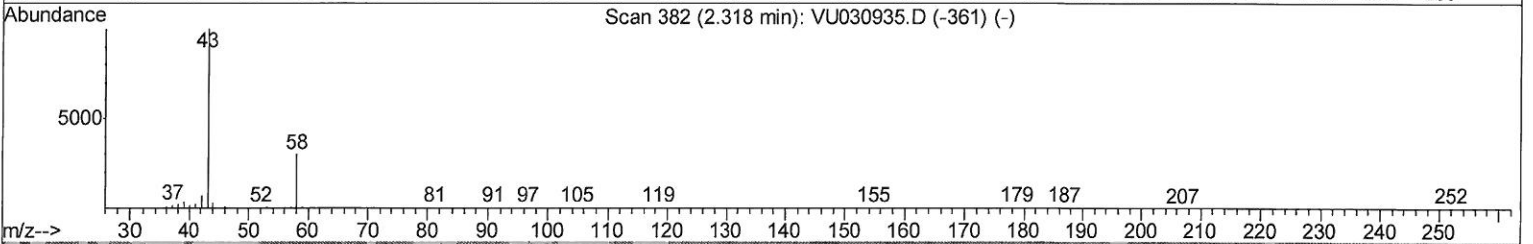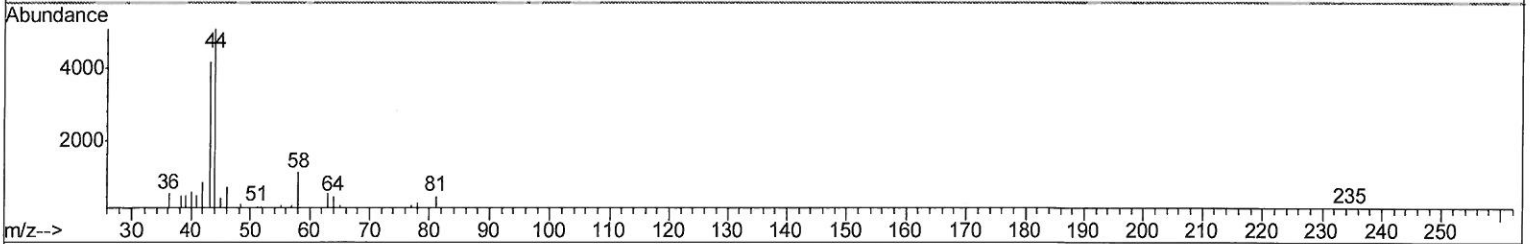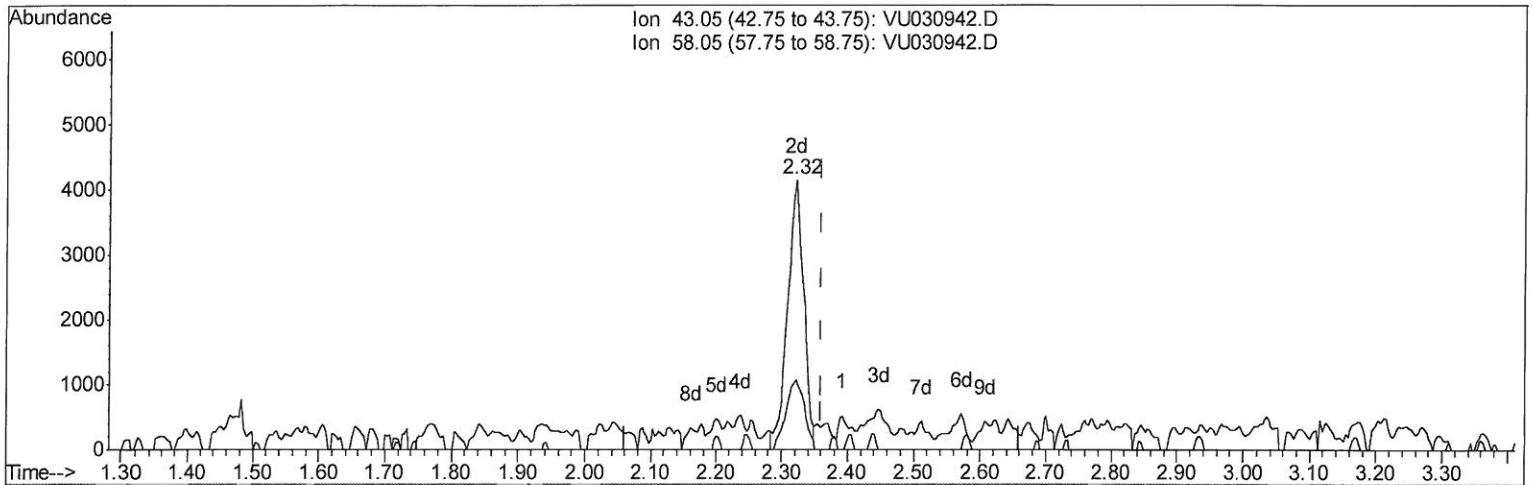

TIC: VU030942.D

(13) Acetone (T)

2.321min (-0.039) 2.08ug/L m

response 7084




Ion	Exp%	Act%
43.05	100	100
58.05	31.40	1.91
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten: 7MD / 4/13/19

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030942.D
 Acq On : 09 Apr 2019 07:51
 Operator : JC/SP
 Sample : K2286-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Quant Time: Apr 09 08:33:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Apr 09 08:28:51 2019
 Response via : Initial Calibration

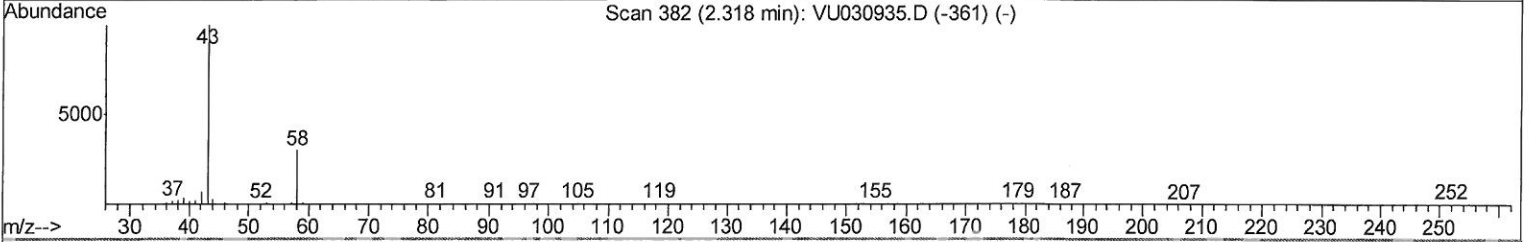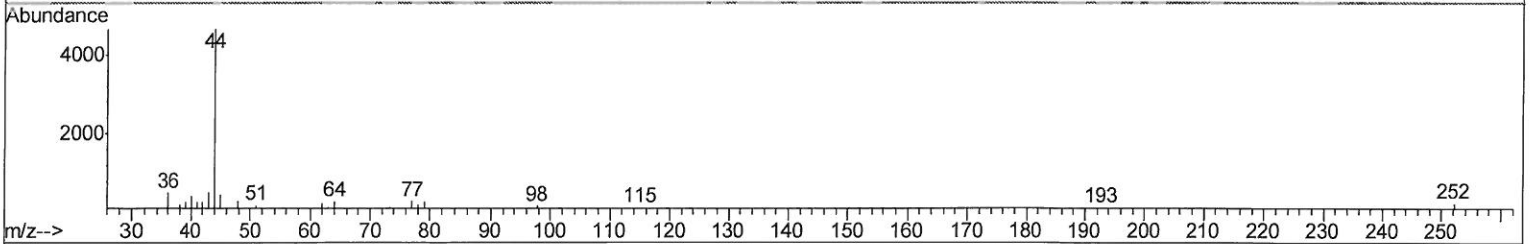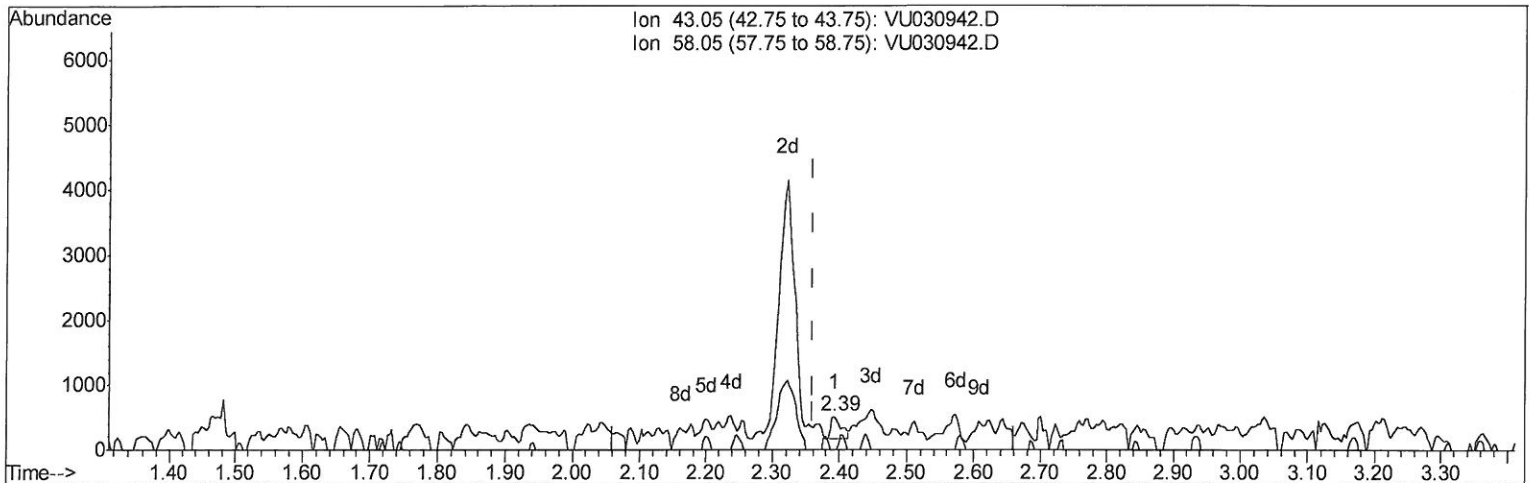

TIC: VU030942.D

(13) Acetone (T)

2.392min (+0.032) 0.11ug/L

response 379

Ion	Exp%	Act%
43.05	100	100
58.05	31.40	35.62
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030942.D
 Acq On : 09 Apr 2019 07:51
 Operator : JC/SP
 Sample : K2286-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Quant Time: Apr 09 08:35:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Apr 09 08:28:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	223900	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	229797	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	90114	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	90587	5.29	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.80%
7) Chloroethane-d5	1.68	69	80631	5.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.80%
11) 1,1-Dichloroethene-d2	2.27	63	143894	4.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.20%
20) 2-Butanone-d5	4.19	46	282671	64.11	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.22%
24) Chloroform-d	4.64	84	155289	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.00%
26) 1,2-Dichloroethane-d4	5.31	65	95076	6.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	123.40%
32) Benzene-d6	5.33	84	312489	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.20%
36) 1,2-Dichloropropane-d6	6.33	67	109156	5.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.60%
41) Toluene-d8	7.56	98	242390	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
43) trans-1,3-Dichloropropene-	7.85	79	34413	4.57	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.40%
46) 2-Hexanone-d5	8.31	63	178555	54.48	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.96%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	90727	6.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	124.80%#
64) 1,2-Dichlorobenzene-d4	11.86	152	87037	5.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.40%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.32	43	7084m	2.078	ug/L	7 mD 4/11/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed