

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030921.D
 Acq On : 08 Apr 2019 21:45
 Operator : JC/SP
 Sample : K2284-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZB2

Quant Time: Apr 09 02:33:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Apr 09 01:11:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	247053	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	256402	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	99116	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	103123	5.46	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.20%
7) Chloroethane-d5	1.68	69	88798	5.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.60%
11) 1,1-Dichloroethene-d2	2.27	63	157276	4.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.40%
20) 2-Butanone-d5	4.19	46	327512	67.32	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	134.64%#
24) Chloroform-d	4.64	84	155534	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
26) 1,2-Dichloroethane-d4	5.31	65	105851	6.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	124.60%
32) Benzene-d6	5.33	84	354220	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.80%
36) 1,2-Dichloropropane-d6	6.33	67	118696	5.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.80%
41) Toluene-d8	7.56	98	277944	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
43) trans-1,3-Dichloropropene-	7.85	79	42576	5.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.20%
46) 2-Hexanone-d5	8.31	63	216916	59.31	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.62%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	99842	6.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	123.20%#
64) 1,2-Dichlorobenzene-d4	11.86	152	98516	5.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.80%


Target Compounds					Ovalue
13) Acetone	2.32	43	4654	1.237 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030921.D
Acq On : 08 Apr 2019 21:45
Operator : JC/SP
Sample : K2284-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZB2

Quant Time: Apr 09 02:33:13 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Apr 09 01:11:42 2019
Response via : Initial Calibration

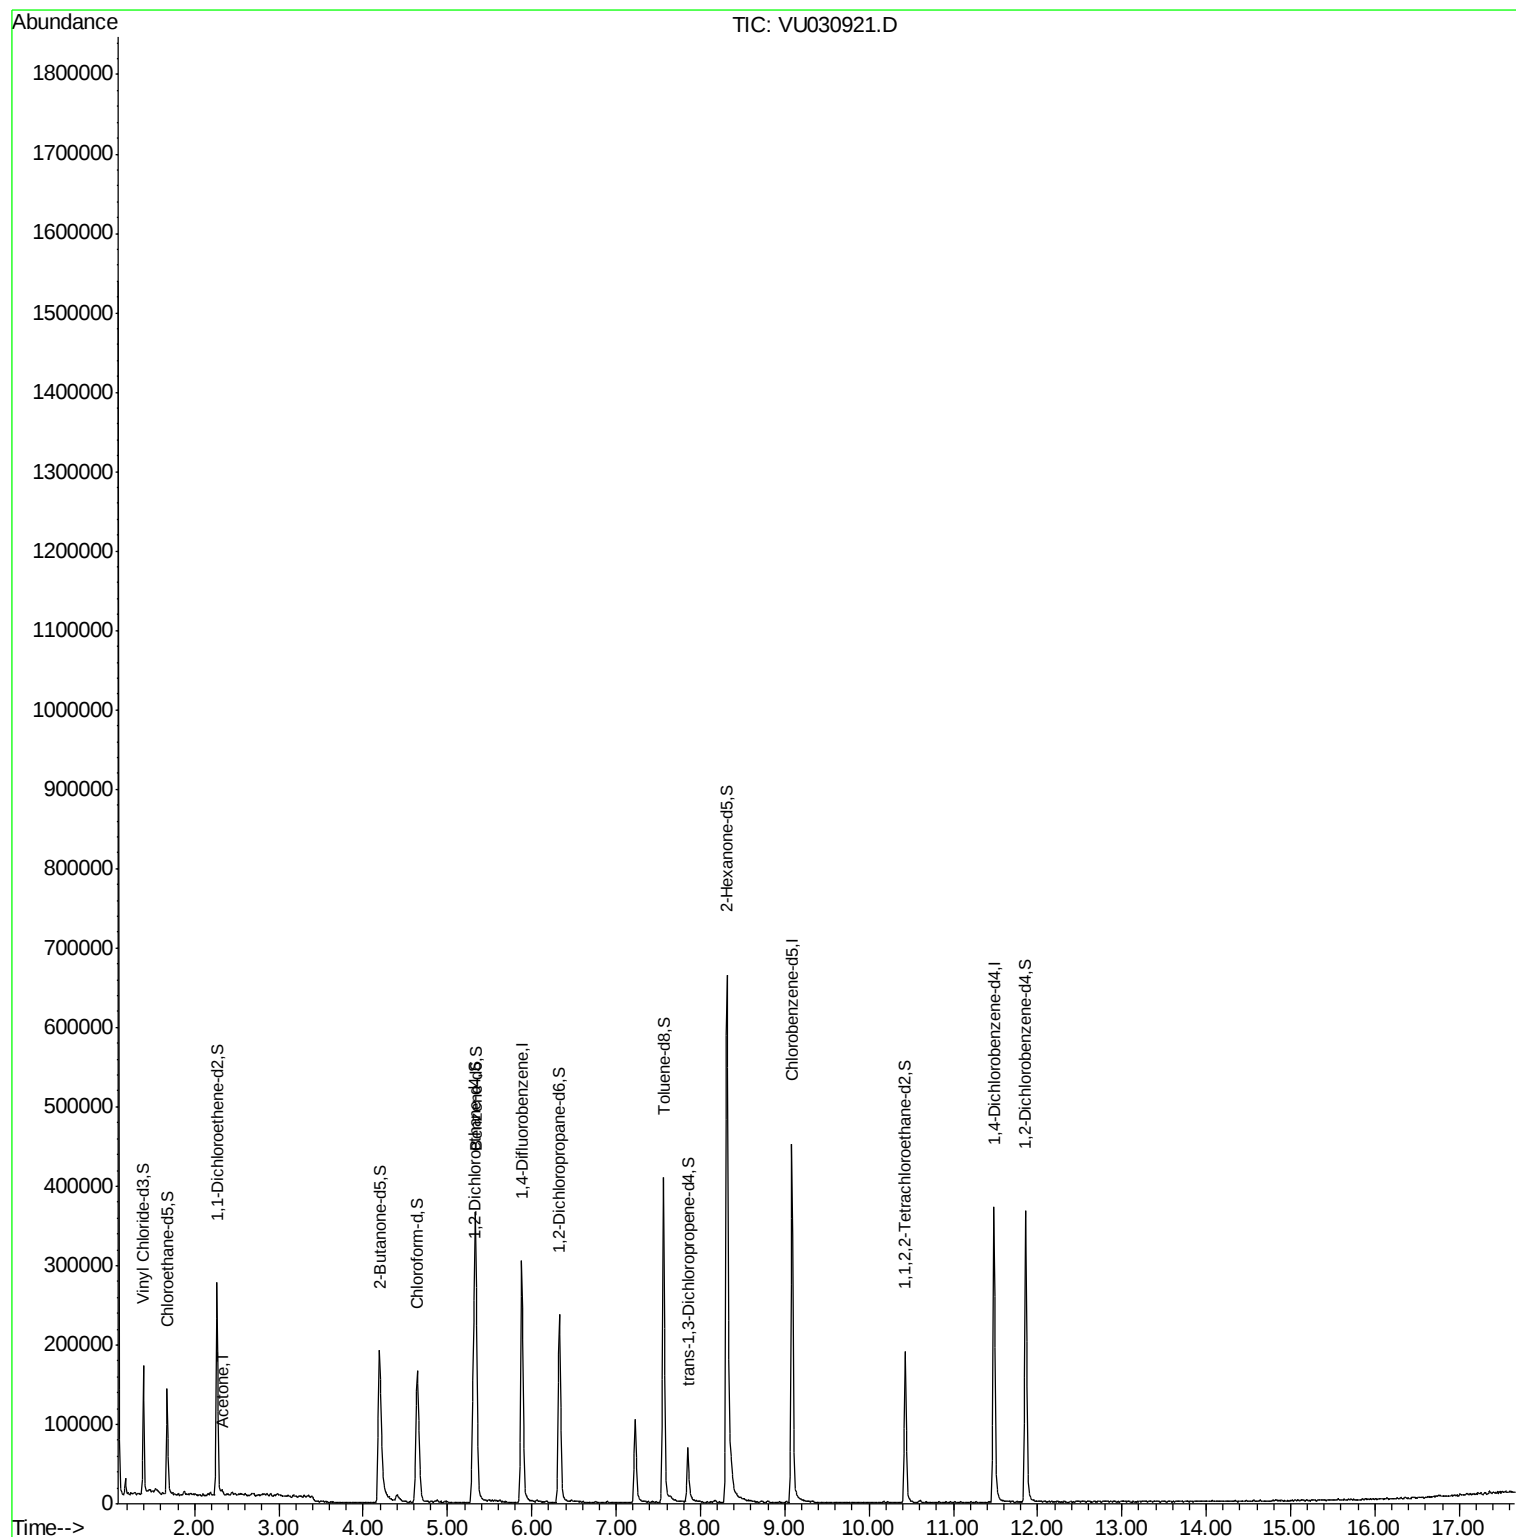

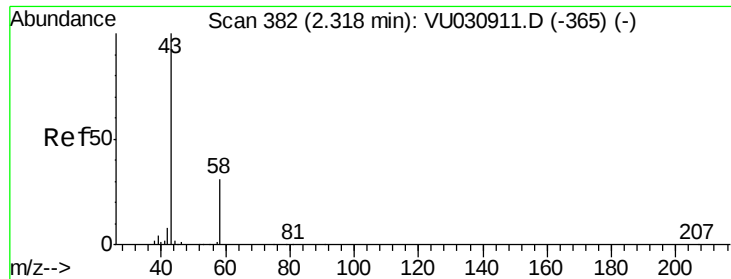

#13

Acetone

Concen: 1.237 ug/L

RT: 2.32 min Scan# 382

Delta R.T. -0.04 min

Lab File: VU030921.D

Acq: 08 Apr 2019 21:45

Instrument :

MSVOA_U

ClientSampleId :


BEZB2

Tot Ion: 43 Resp: 4654

Ion Ratio Lower Upper

43 100

58 30.4 0.0 62.8

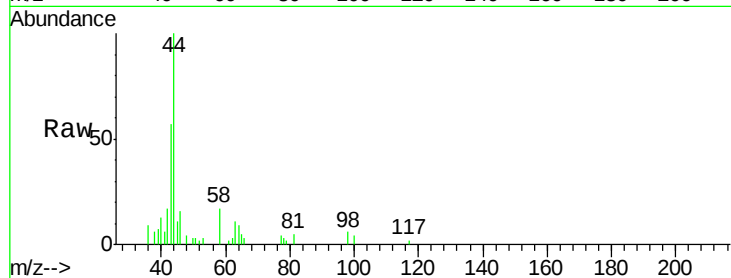

Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 58.05 (57.75 to 58.75): VU0

