

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030925.D
 Acq On : 08 Apr 2019 23:23
 Operator : JC/SP
 Sample : K2284-20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZB8

Quant Time: Apr 09 03:20:22 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Apr 09 01:11:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	198789	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	205200	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	81993	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	84472	5.56	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.20%
7) Chloroethane-d5	1.68	69	73154	5.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	119.40%
11) 1,1-Dichloroethene-d2	2.27	63	126713	4.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.40%
20) 2-Butanone-d5	4.19	46	285179	72.85	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	145.70%#
24) Chloroform-d	4.64	84	129441	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
26) 1,2-Dichloroethane-d4	5.31	65	87945	6.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	128.60%
32) Benzene-d6	5.33	84	292696	5.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.20%
36) 1,2-Dichloropropane-d6	6.33	67	99986	5.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.20%
41) Toluene-d8	7.56	98	224865	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
43) trans-1,3-Dichloropropene-	7.85	79	33354	4.96	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.20%
46) 2-Hexanone-d5	8.31	63	172464	58.93	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	117.86%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	83912	6.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	129.20%#
64) 1,2-Dichlorobenzene-d4	11.86	152	80564	5.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.40%


Target Compounds				Ovalue
13) Acetone	2.32	43	8593	2.839 ug/L 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030925.D
Acq On : 08 Apr 2019 23:23
Operator : JC/SP
Sample : K2284-20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZB8

Quant Time: Apr 09 03:20:22 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Apr 09 01:11:42 2019
Response via : Initial Calibration

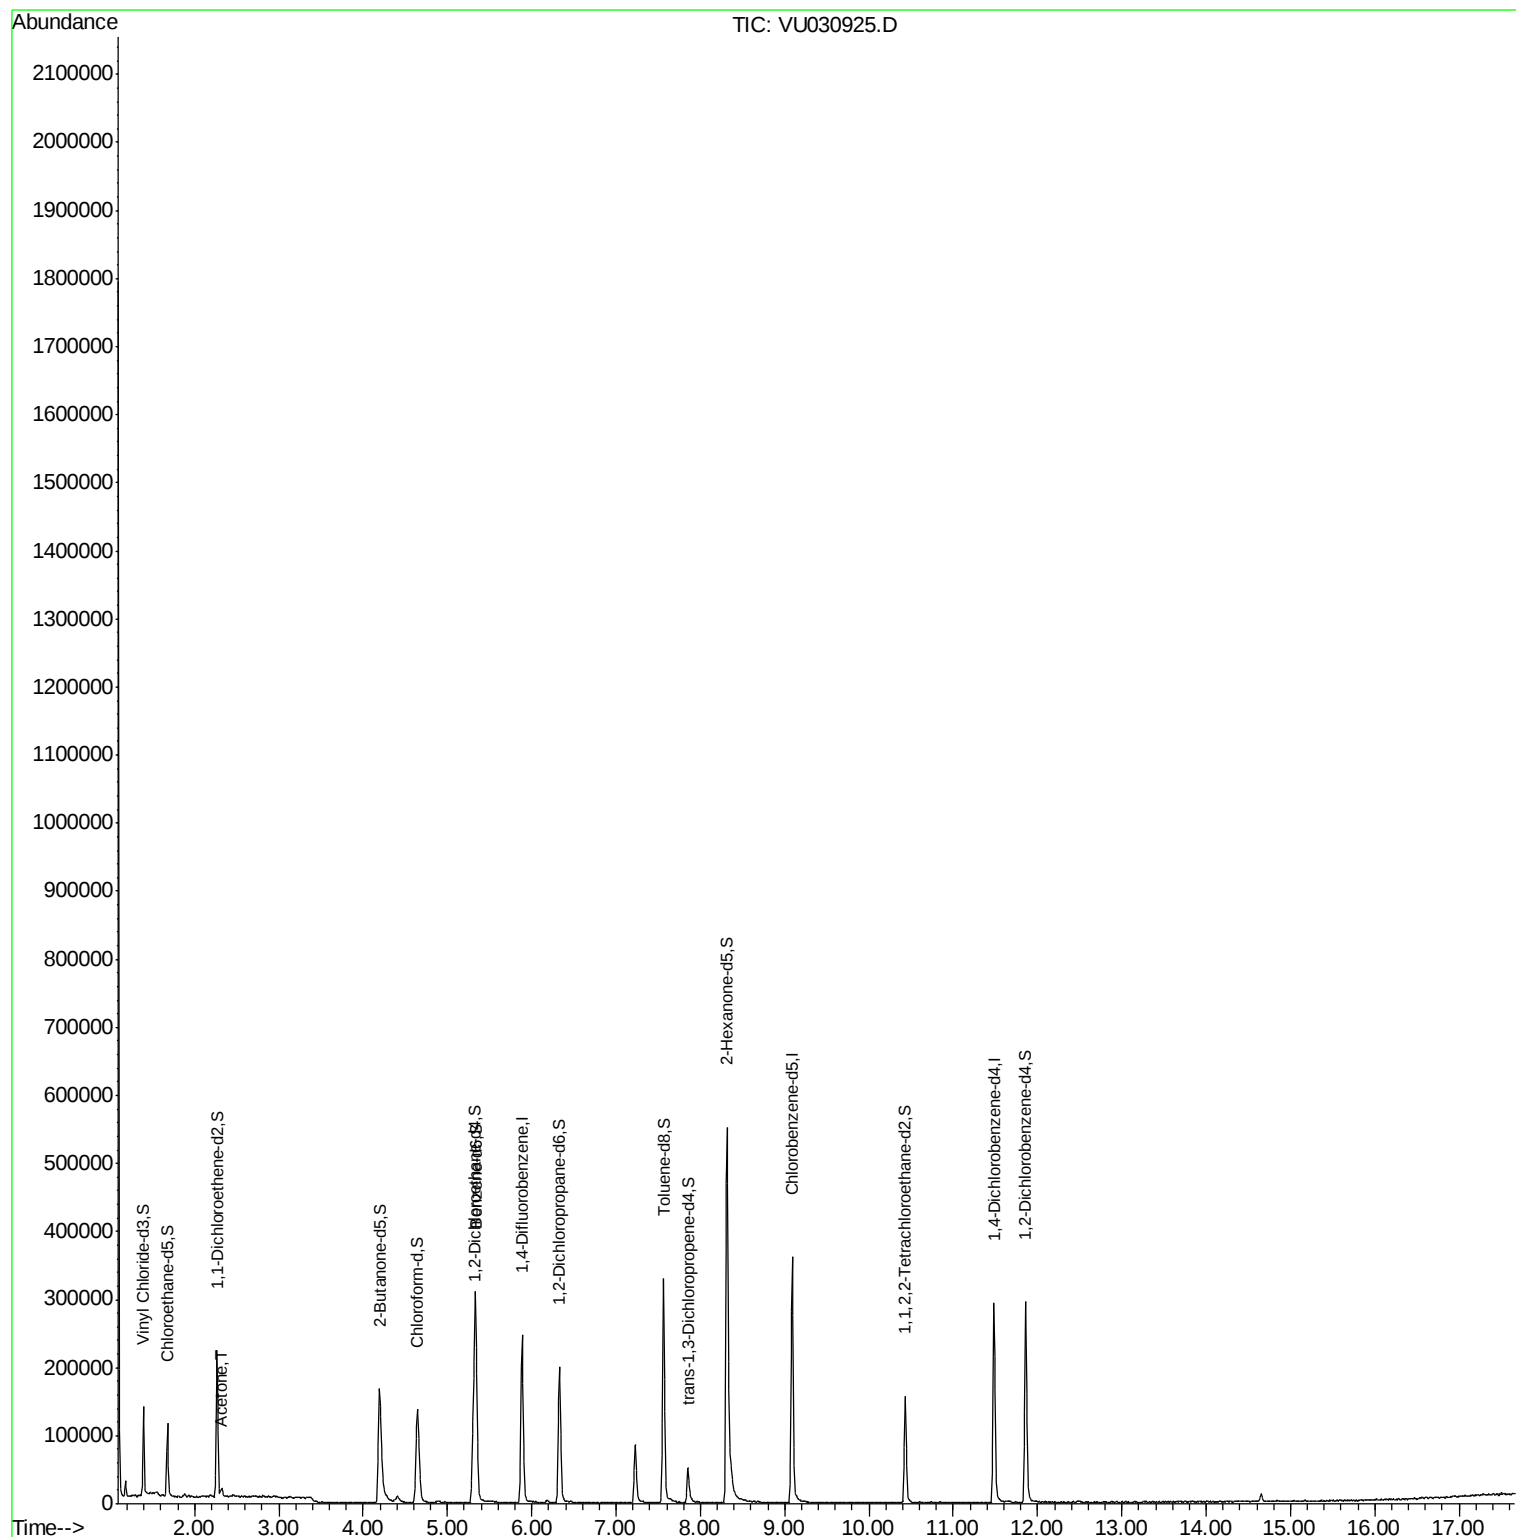

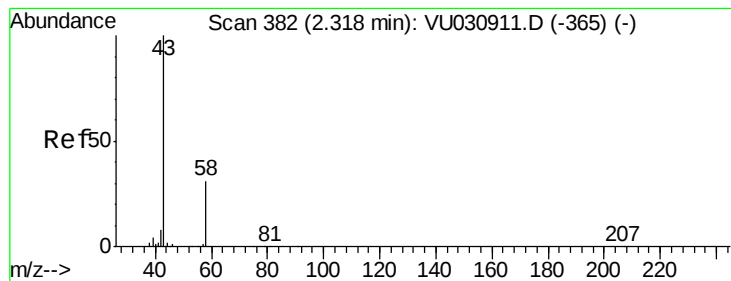

#13
 Acetone
 Concen: 2.839 ug/L
 RT: 2.32 min Scan# 383
 Delta R.T. -0.04 min
 Lab File: VU030925.D
 Acq: 08 Apr 2019 23:23

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZB8

Tot Ion: 43 Resp: 8593
 Ion Ratio Lower Upper
 43 100
 58 28.3 0.0 62.8

