

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030942.D
 Acq On : 09 Apr 2019 08:15
 Operator : JC/SP
 Sample : K2286-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZE2

Quant Time: Apr 09 08:48:33 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Apr 09 08:40:40 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	219786	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	225151	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	89173	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	86408	5.14	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.80%
7) Chloroethane-d5	1.68	69	78083	5.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.40%
11) 1,1-Dichloroethene-d2	2.27	63	137670	4.00	ug/L	-0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.00%
20) 2-Butanone-d5	4.19	46	278424	64.33	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.66%
24) Chloroform-d	4.64	84	164138	5.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.20%
26) 1,2-Dichloroethane-d4	5.31	65	95754	6.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	126.60%
32) Benzene-d6	5.33	84	308706	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
36) 1,2-Dichloropropane-d6	6.33	67	110244	5.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.80%
41) Toluene-d8	7.56	98	244600	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
43) trans-1,3-Dichloropropene-	7.85	79	33805	4.58	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.60%
46) 2-Hexanone-d5	8.31	63	182023	56.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.36%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	88580	6.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	124.40%#
64) 1,2-Dichlorobenzene-d4	11.86	152	83663	5.61	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	6690	1.999 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030942.D
Acq On : 09 Apr 2019 08:15
Operator : JC/SP
Sample : K2286-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZE2

Quant Time: Apr 09 08:48:33 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Apr 09 08:40:40 2019
Response via : Initial Calibration

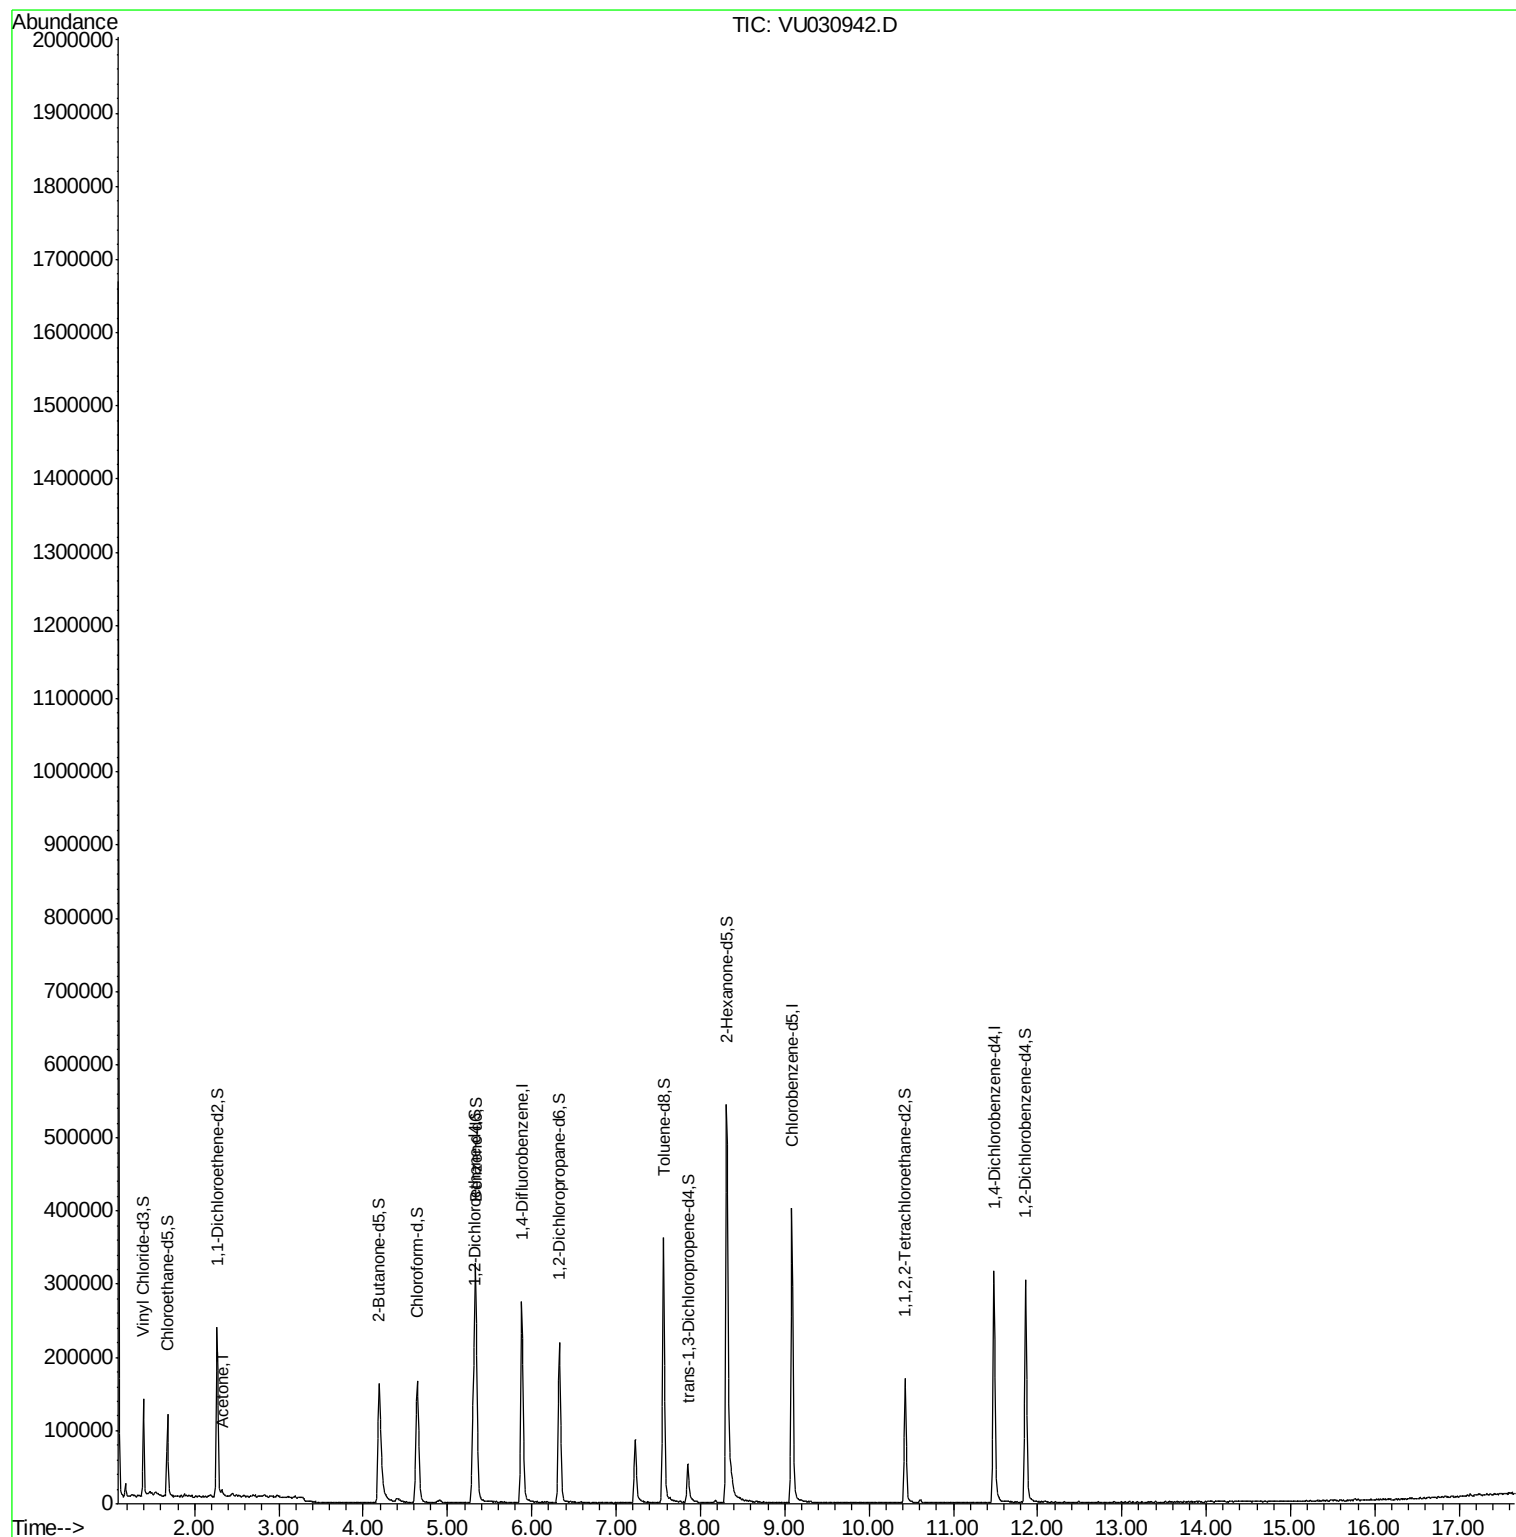

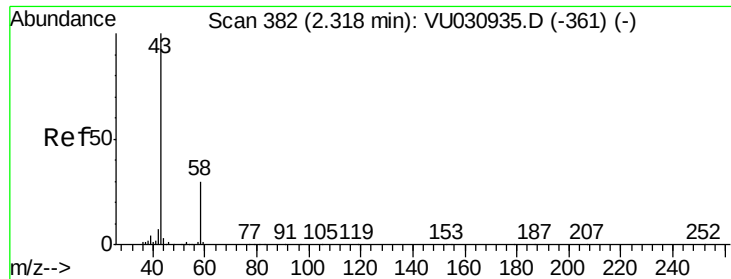

#13
Acetone
Concen: 1.999 ug/L
RT: 2.32 min Scan# 383
Delta R.T. -0.04 min
Lab File: VU030942.D
Acq: 09 Apr 2019 08:15

Instrument :
MSVOA_U
ClientSampleId :
BEZE2

Tot Ion: 43 Resp: 6690
Ion Ratio Lower Upper
43 100
58 30.9 0.0 62.8

