

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030944.D
 Acq On : 09 Apr 2019 09:04
 Operator : JC/SP
 Sample : K2286-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZE4

Quant Time: Apr 10 01:28:31 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 01:14:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	209903	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	219079	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	84529	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	88844	5.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	110.80%
7) Chloroethane-d5	1.68	69	80028	6.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	123.80%
11) 1,1-Dichloroethene-d2	2.27	63	139351	4.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.80%
20) 2-Butanone-d5	4.19	46	278287	67.33	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	134.66%#
24) Chloroform-d	4.64	84	157387	5.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.60%
26) 1,2-Dichloroethane-d4	5.31	65	96062	6.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	133.00%#
32) Benzene-d6	5.33	84	308230	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.80%
36) 1,2-Dichloropropane-d6	6.33	67	107078	5.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.60%
41) Toluene-d8	7.56	98	242893	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.40%
43) trans-1,3-Dichloropropene-	7.85	79	31748	4.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.40%
46) 2-Hexanone-d5	8.31	63	170145	54.45	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.90%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	87657	6.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	126.60%#
64) 1,2-Dichlorobenzene-d4	11.86	152	87239	6.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	123.40%#


Target Compounds				Ovalue
13) Acetone	2.32	43	17434	5.456 ug/L 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030944.D
Acq On : 09 Apr 2019 09:04
Operator : JC/SP
Sample : K2286-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZE4

Quant Time: Apr 10 01:28:31 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 01:14:30 2019
Response via : Initial Calibration

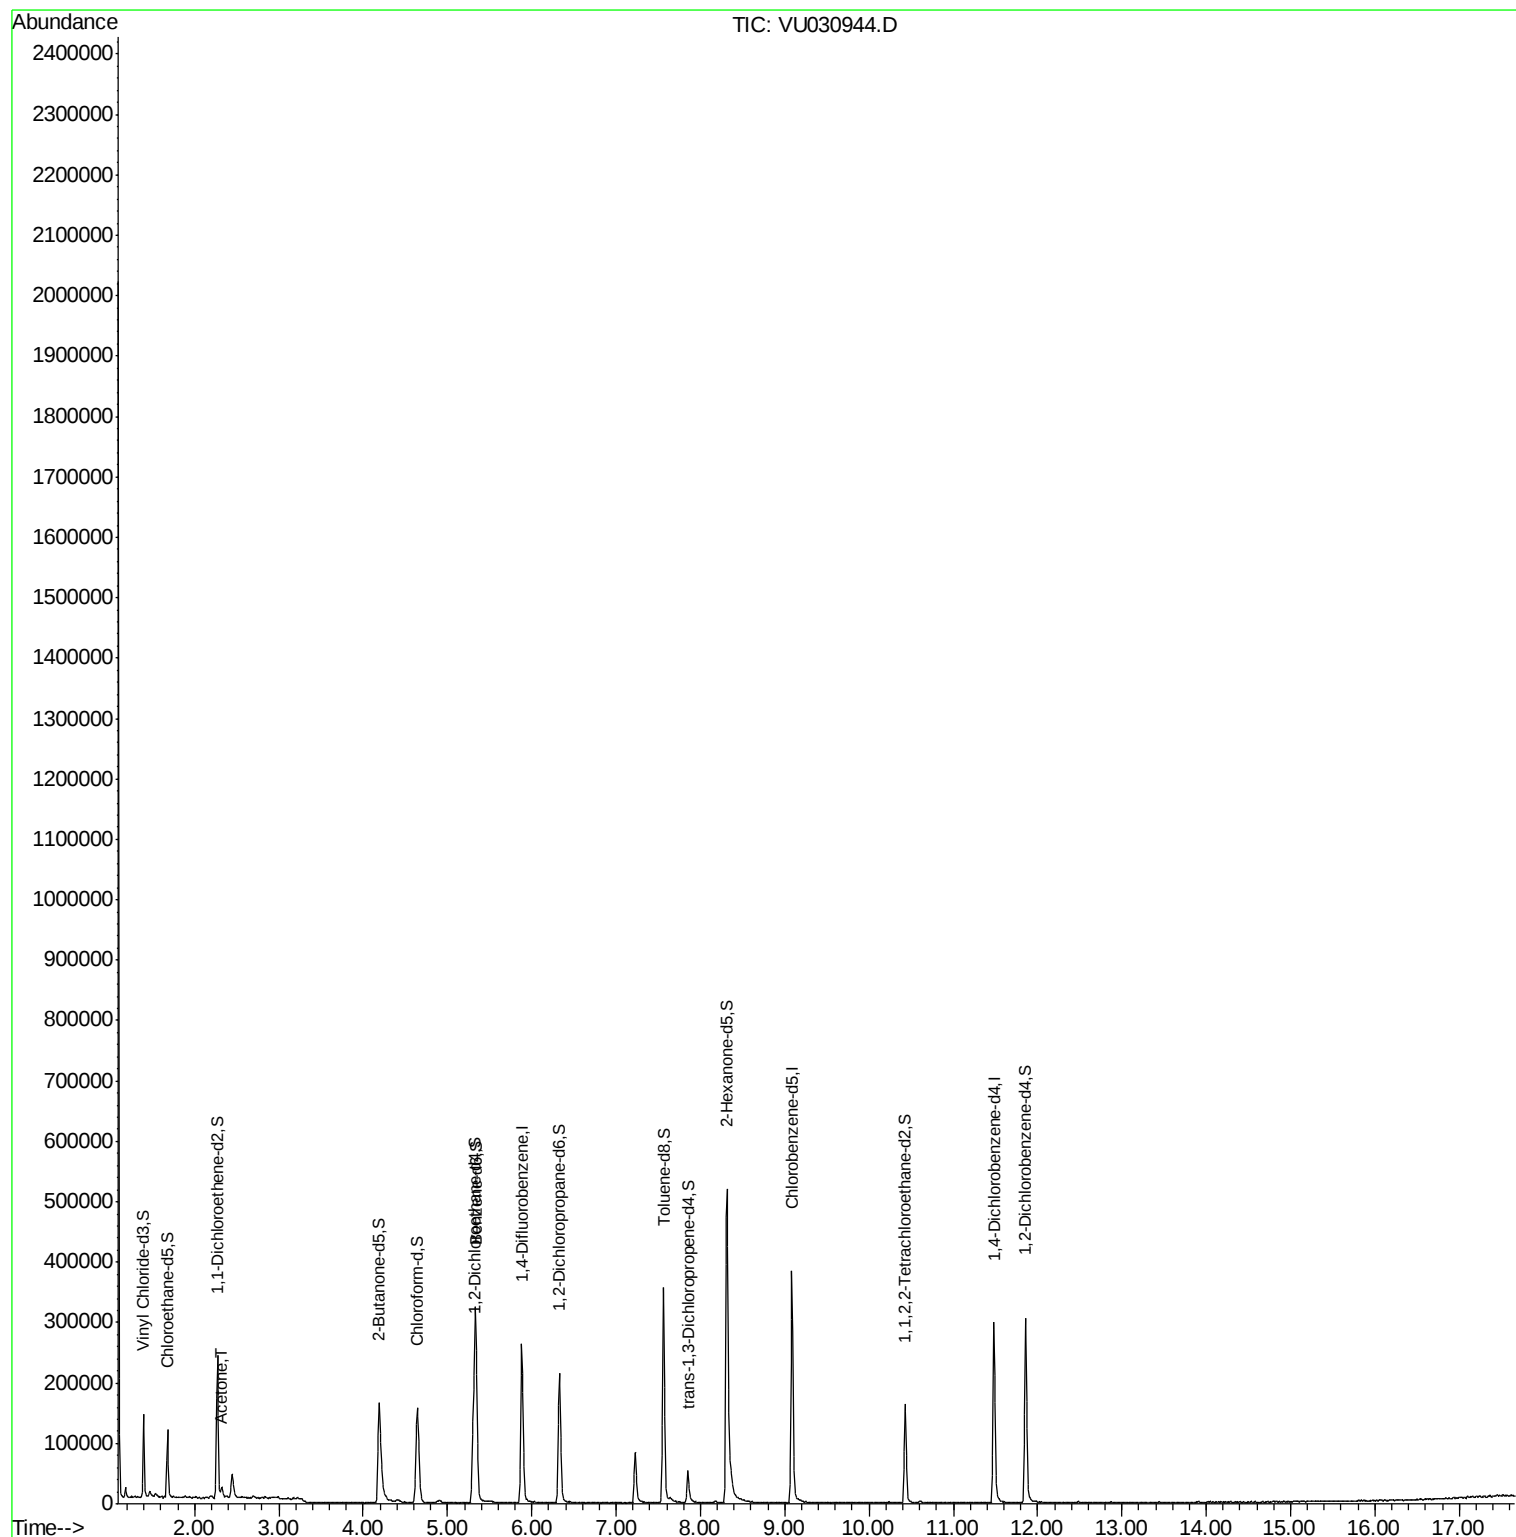

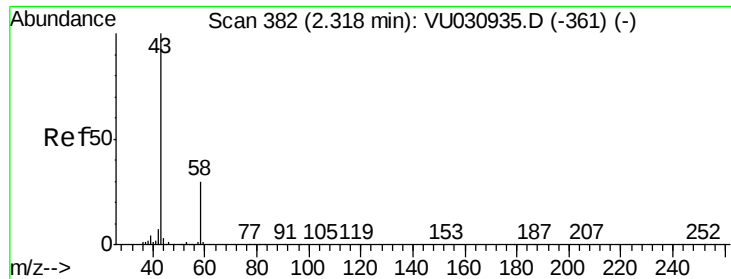

#13

Acetone

Concen: 5.456 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.04 min

Lab File: VU030944.D

Acq: 09 Apr 2019 09:04

Instrument :
MSVOA_U
ClientSampleId :
BEZE4

Tot Ion: 43 Resp: 17434

Ion Ratio Lower Upper

43 100

58 29.2 0.0 62.8

