

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030945.D
 Acq On : 09 Apr 2019 09:28
 Operator : JC/SP
 Sample : K2286-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZE5

Quant Time: Apr 10 01:31:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 01:14:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	215924	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	218188	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	83603	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	83110	5.04	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.80%
7) Chloroethane-d5	1.68	69	73764	5.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.80%
11) 1,1-Dichloroethene-d2	2.27	63	129064	3.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.40%
20) 2-Butanone-d5	4.19	46	262486	61.74	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	123.48%
24) Chloroform-d	4.64	84	138135	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	5.31	65	89602	6.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.60%
32) Benzene-d6	5.33	84	284426	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.33	67	99762	5.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.40%
41) Toluene-d8	7.56	98	222455	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
43) trans-1,3-Dichloropropene-	7.85	79	30550	4.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.40%
46) 2-Hexanone-d5	8.31	63	155584	49.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.98%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	83270	6.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	120.60%#
64) 1,2-Dichlorobenzene-d4	11.86	152	81593	5.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.60%


Target Compounds				Ovalue
13) Acetone	2.32	43	8459m	2.573 ug/L


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030945.D
Acq On : 09 Apr 2019 09:28
Operator : JC/SP
Sample : K2286-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZE5

Quant Time: Apr 10 01:31:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 01:14:30 2019
Response via : Initial Calibration

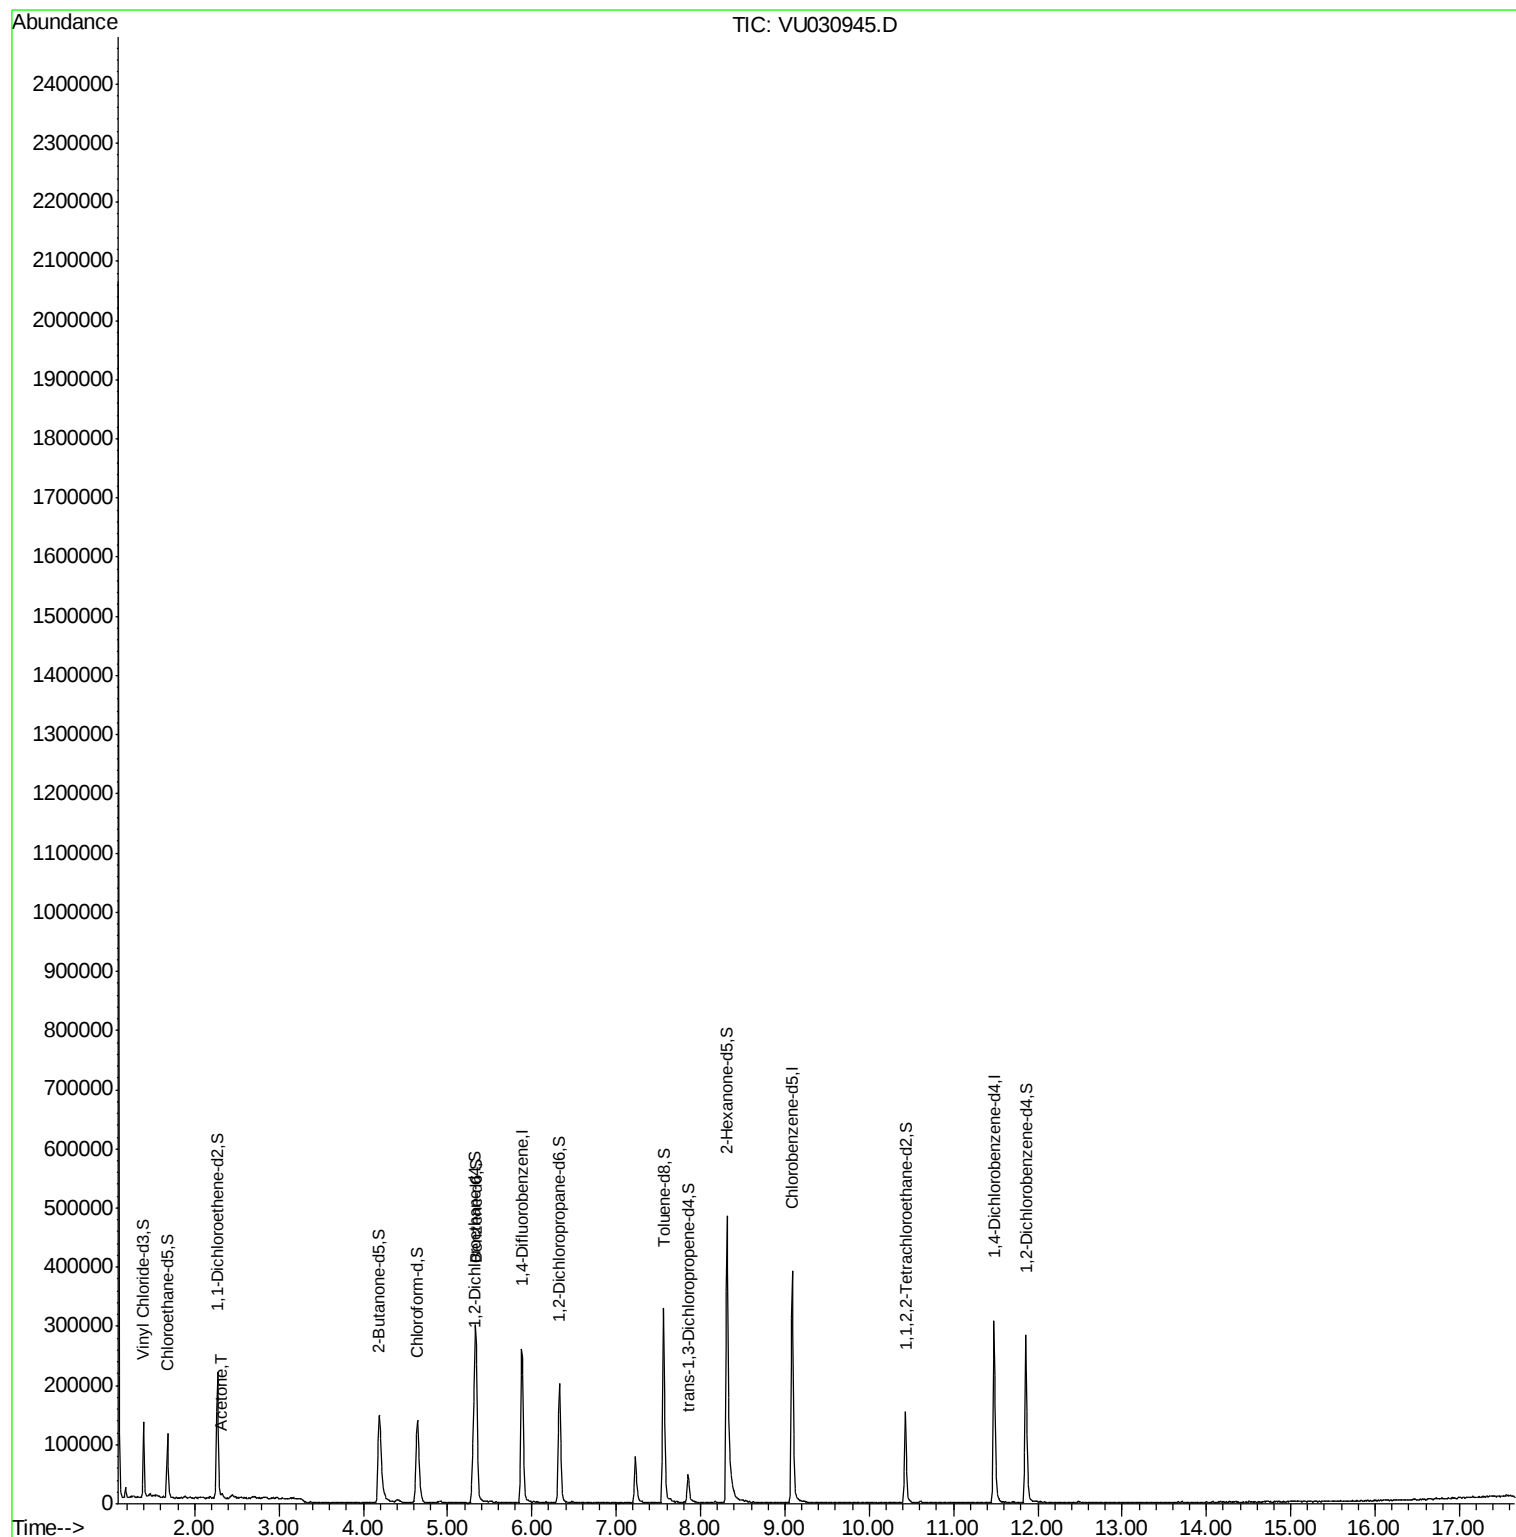

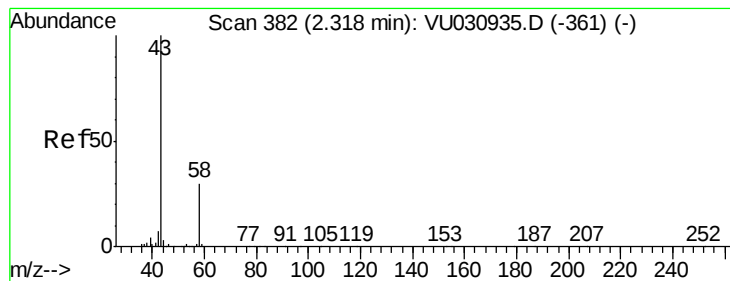

#13
 Acetone
 Concen: 2.573 ug/L m
 RT: 2.32 min Scan# 382
 Delta R.T. -0.04 min
 Lab File: VU030945.D
 Acq: 09 Apr 2019 09:28

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZE5

Tot Ion: 43 Resp: 8459
 Ion Ratio Lower Upper
 43 100
 58 1.0 0.0 62.8

