

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030952.D
 Acq On : 09 Apr 2019 12:54
 Operator : JC/SP
 Sample : K2286-12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZF0

Quant Time: Apr 10 02:21:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 01:53:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	238663	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	236273	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	94696	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	89301	4.90	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.00%
7) Chloroethane-d5	1.68	69	83718	5.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.80%
11) 1,1-Dichloroethene-d2	2.27	63	140558	3.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.20%
20) 2-Butanone-d5	4.19	46	283642	60.36	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.72%
24) Chloroform-d	4.64	84	156304	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
26) 1,2-Dichloroethane-d4	5.31	65	94775	5.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.40%
32) Benzene-d6	5.33	84	315984	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
36) 1,2-Dichloropropane-d6	6.33	67	107976	5.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.40%
41) Toluene-d8	7.56	98	250331	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.20%
43) trans-1,3-Dichloropropene-	7.85	79	37670	4.86	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.20%
46) 2-Hexanone-d5	8.31	63	178134	52.86	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.72%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	90431	6.05	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	121.00%#
64) 1,2-Dichlorobenzene-d4	11.86	152	87954	5.55	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.00%


Target Compounds				Ovalue
13) Acetone	2.32	43	8458	2.328 ug/L 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030952.D
Acq On : 09 Apr 2019 12:54
Operator : JC/SP
Sample : K2286-12
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZF0

Quant Time: Apr 10 02:21:13 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 01:53:07 2019
Response via : Initial Calibration

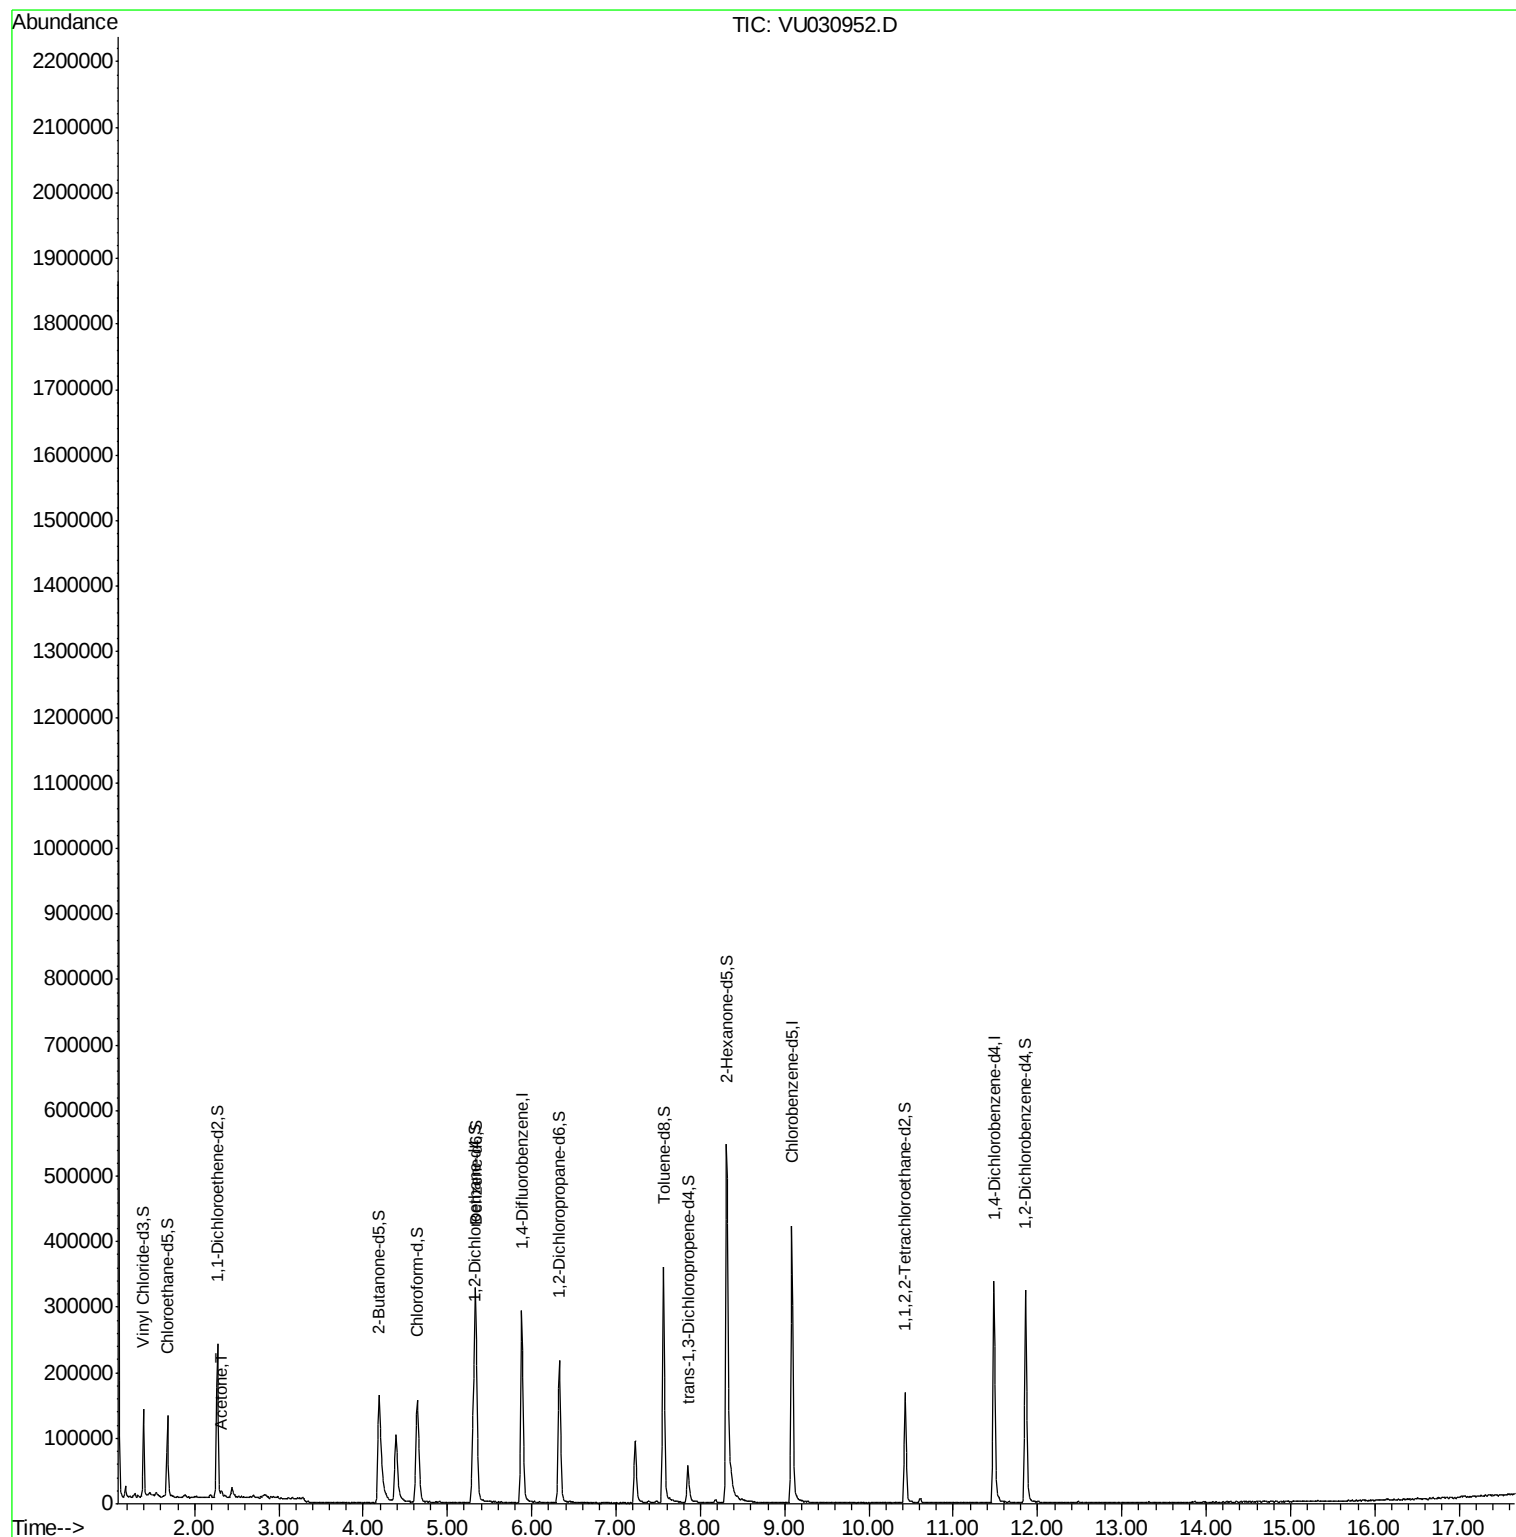

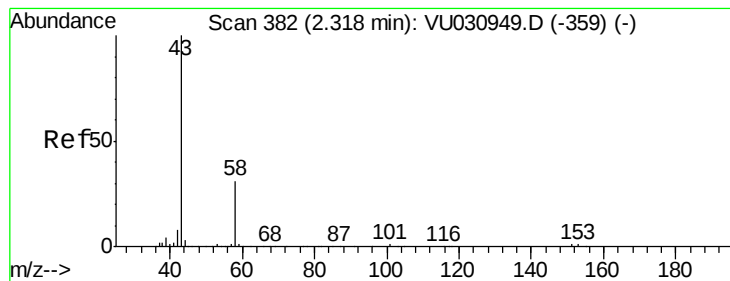

#13

Acetone

Concen: 2.328 ug/L

RT: 2.32 min Scan# 384

Delta R.T. 0.01 min

Lab File: VU030952.D

Acq: 09 Apr 2019 12:54

Instrument :
MSVOA_U
ClientSampleId :
BEZF0

Tot Ion: 43 Resp: 8458

Ion Ratio Lower Upper

43 100

58 27.8 0.0 62.8

