

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030954.D
 Acq On : 09 Apr 2019 13:42
 Operator : JC/SP
 Sample : K2286-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZF2

Quant Time: Apr 10 03:08:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 01:53:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	220493	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	225758	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	88045	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	86573	5.14	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.80%
7) Chloroethane-d5	1.68	69	78620	5.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.80%
11) 1,1-Dichloroethene-d2	2.27	63	132669	3.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.00%
20) 2-Butanone-d5	4.19	46	273591	63.01	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.02%
24) Chloroform-d	4.64	84	154178	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.80%
26) 1,2-Dichloroethane-d4	5.31	65	93044	6.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	122.80%
32) Benzene-d6	5.33	84	299697	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
36) 1,2-Dichloropropane-d6	6.32	67	105295	5.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.60%
41) Toluene-d8	7.56	98	234263	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.20%
43) trans-1,3-Dichloropropene-	7.85	79	34954	4.72	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.40%
46) 2-Hexanone-d5	8.31	63	169792	52.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.46%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	86596	6.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	121.20%#
64) 1,2-Dichlorobenzene-d4	11.86	152	83740	5.69	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.80%


Target Compounds					Ovalue
13) Acetone	2.32	43	37569	11.192 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030954.D
Acq On : 09 Apr 2019 13:42
Operator : JC/SP
Sample : K2286-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZF2

Quant Time: Apr 10 03:08:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 01:53:07 2019
Response via : Initial Calibration

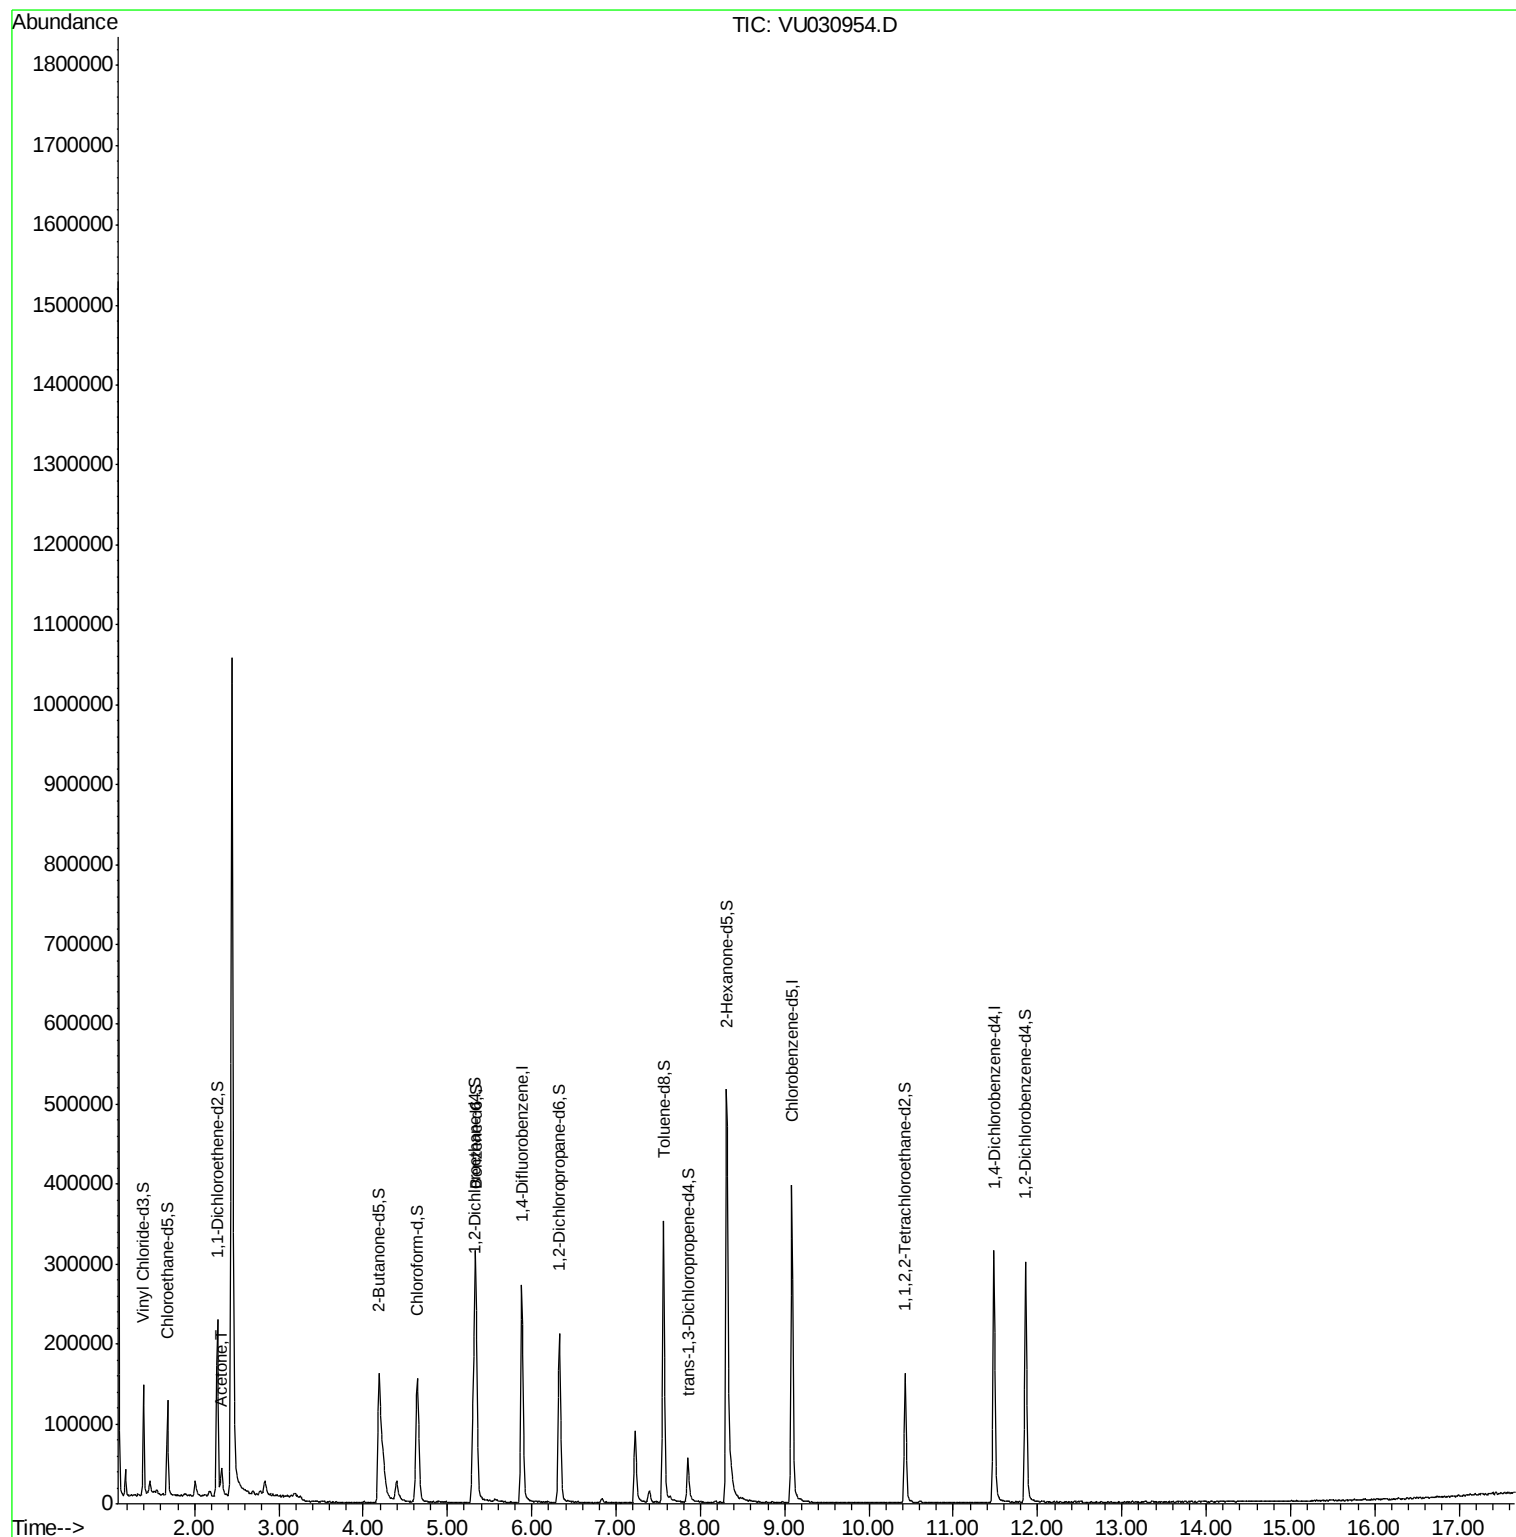

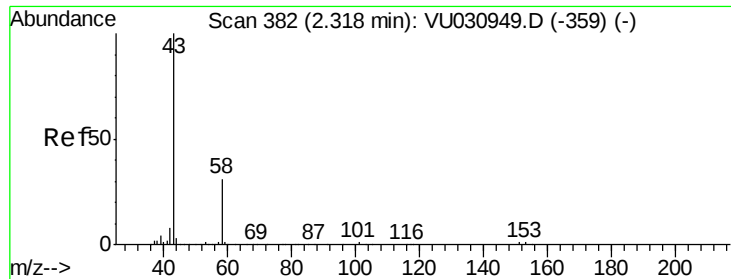

#13

Acetone

Concen: 11.192 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU030954.D

Acq: 09 Apr 2019 13:42

Instrument :
MSVOA_U
ClientSampleId :
BEZF2

Tot Ion: 43 Resp: 37569

Ion Ratio Lower Upper

43 100

58 30.9 0.0 62.8

